


Data Path : Z:\HPCHEM1\BNA G\Data\BG031518\
 Data File : BG033176.D
 Acq On : 15 Mar 2018 14:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 13:59:34 2018

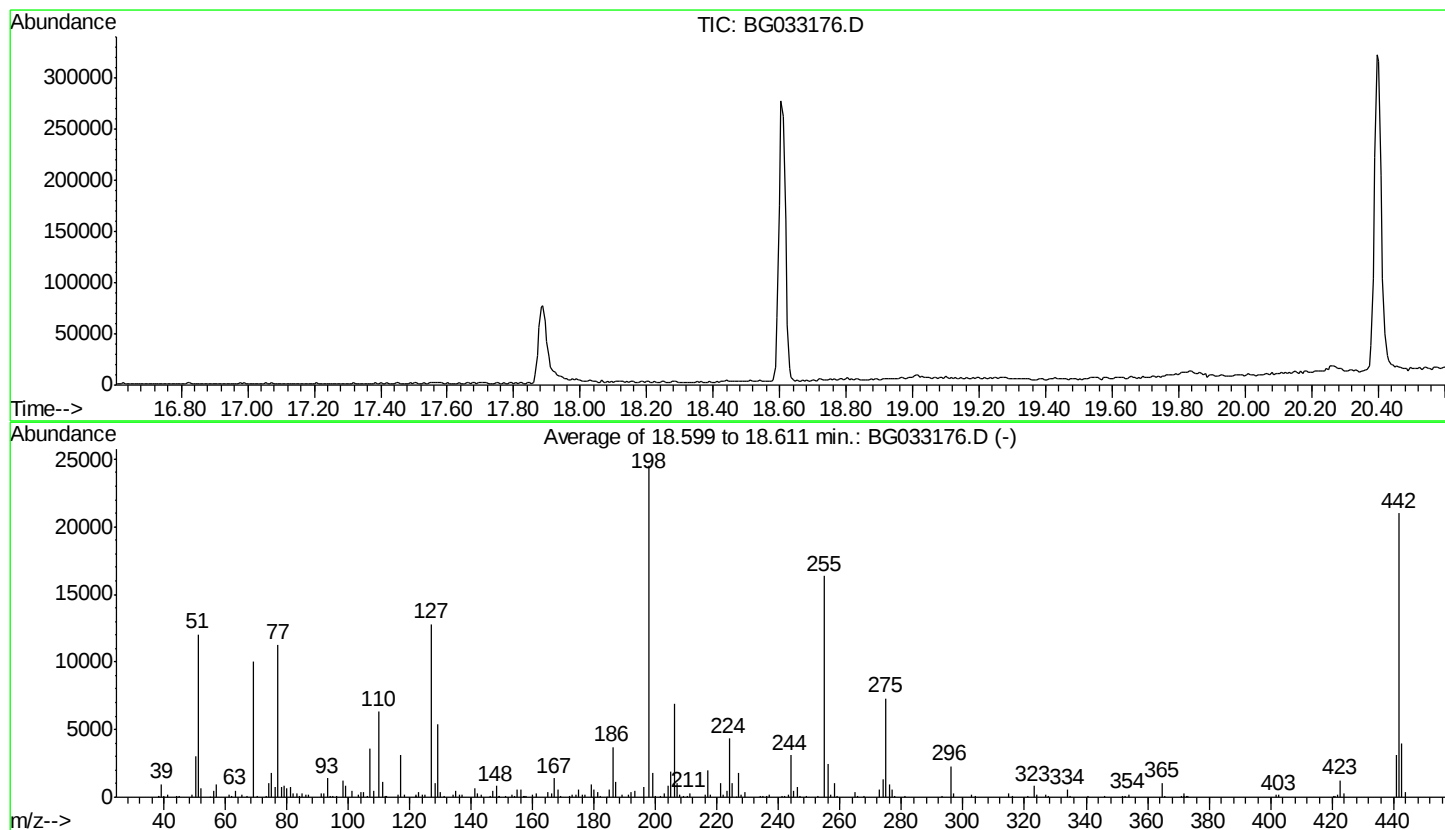

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	12061	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.0	10053	PASS
70	69	0.00	2	0.5	54	PASS
127	198	10	80	52.3	12824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24514	PASS
199	198	5	9	7.2	1772	PASS
275	198	10	60	29.9	7330	PASS
365	198	1	100	4.3	1054	PASS
441	442	0.01	24	14.8	3103	PASS
442	198	50	100	85.5	20971	PASS
443	442	15	24	19.1	4010	PASS