
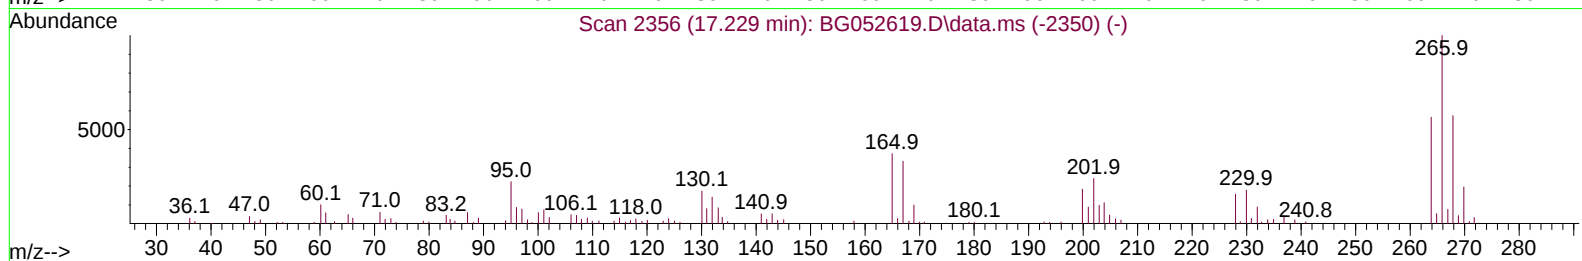
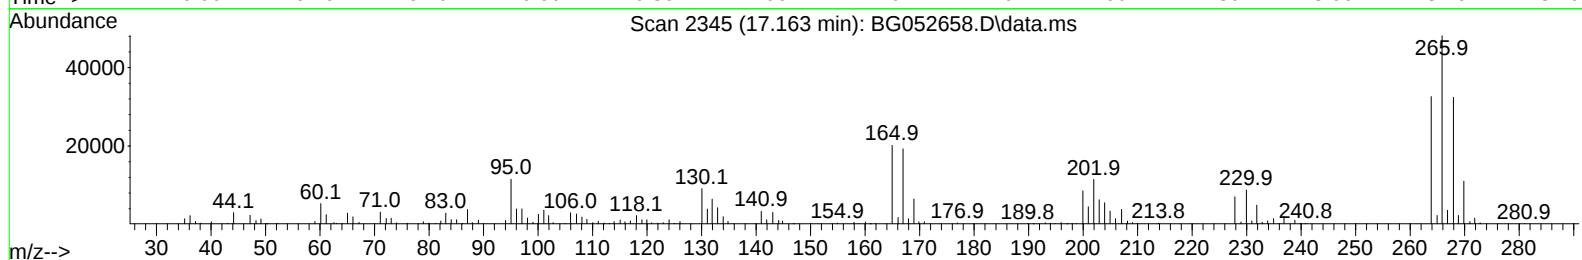


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
Data File : BG052658.D
Acq On : 15 Mar 2022 9:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 11:46:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 11:46:28 2022
Response via : Initial Calibration

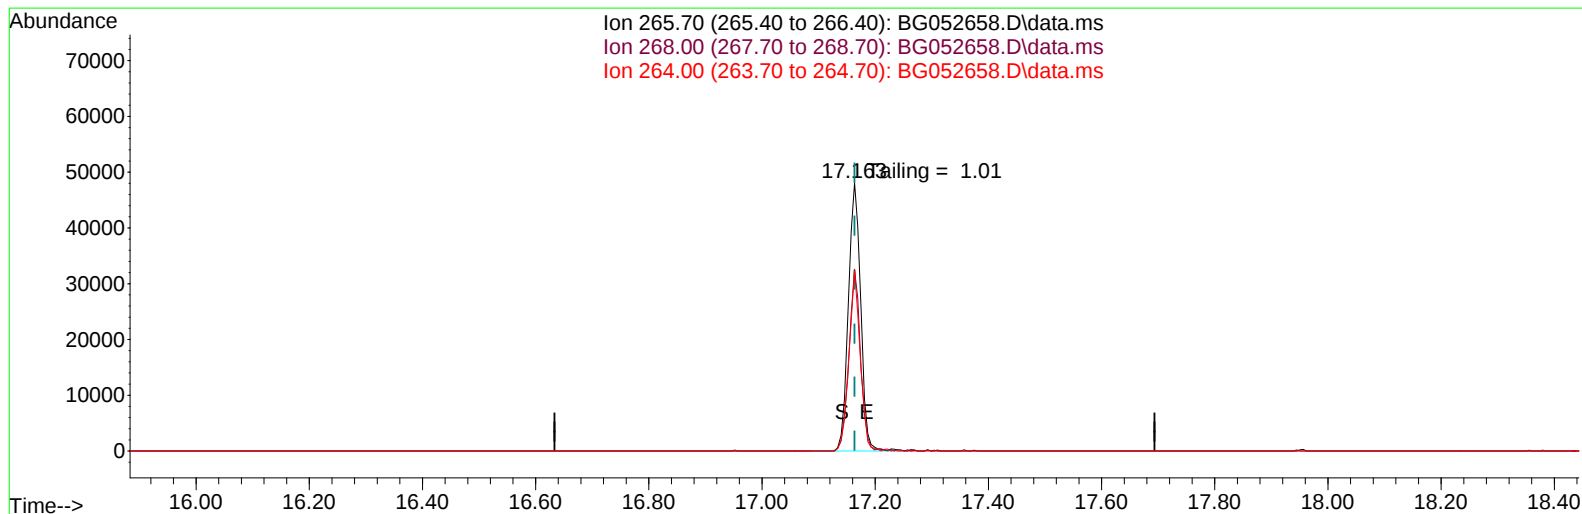

TIC: BG052658.D\data.ms

(70) Pentachlorophenol (C)




17.163min (0.000) 28646.61 ng

response 72352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.35
264.00	56.60	67.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
Data File : BG052658.D
Acq On : 15 Mar 2022 9:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 11:46:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 11:46:28 2022
Response via : Initial Calibration

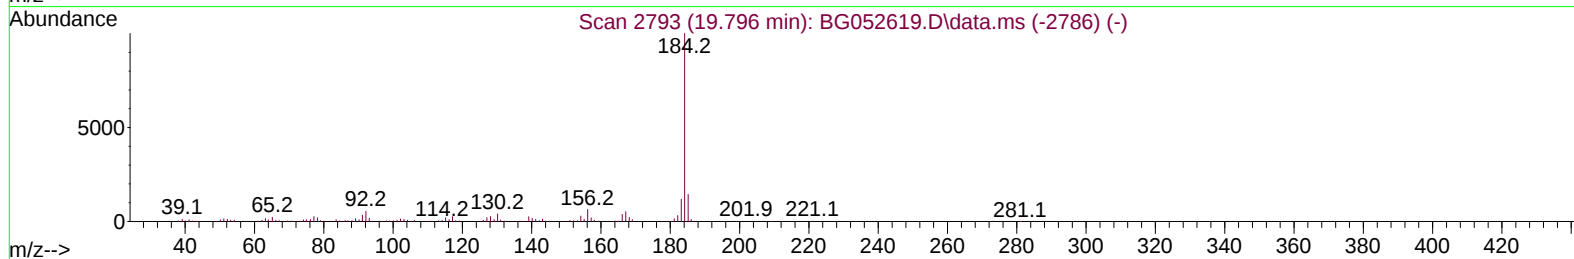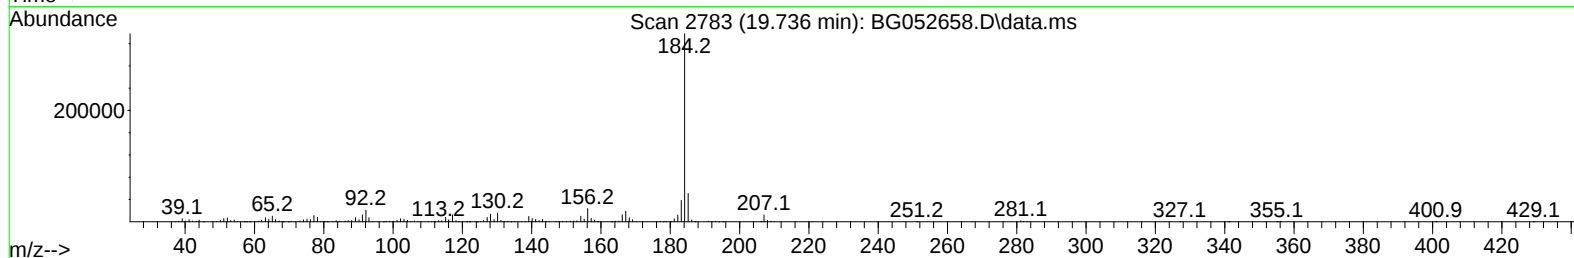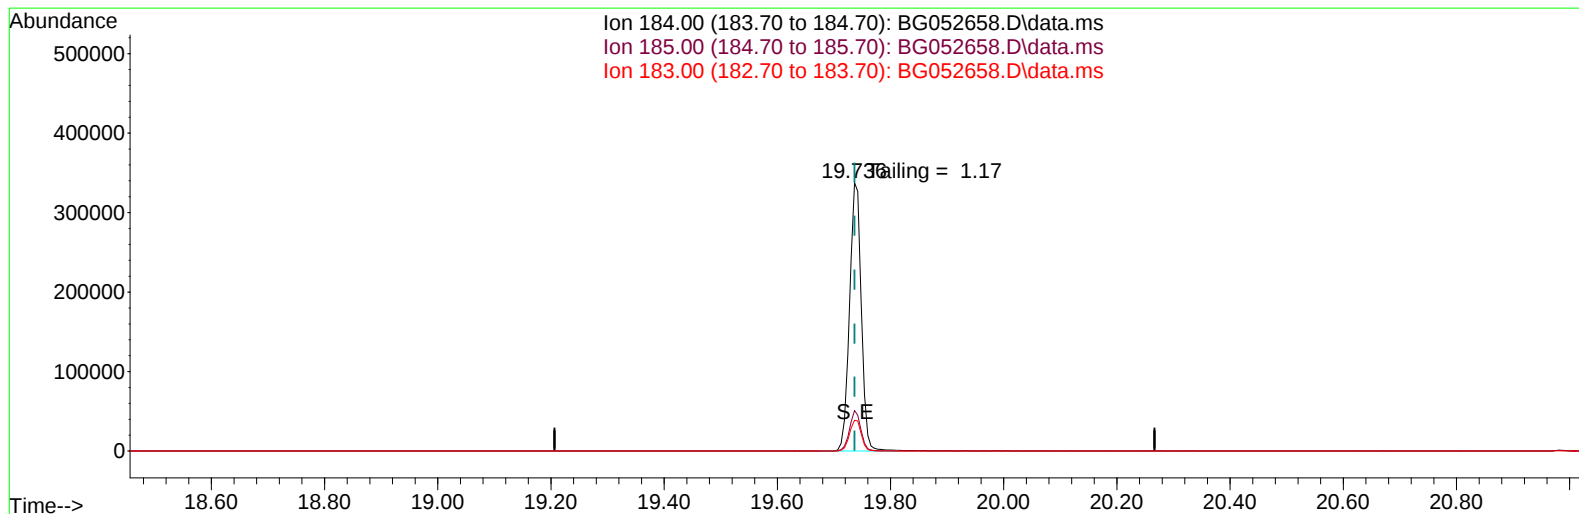

TIC: BG052658.D\data.ms

(77) Benzidine**19.736min (0.000) 426525.49 ng****response 486644**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.11
183.00	11.80	11.46
0.00	0.00	0.00