

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
 Data File : BG052667.D
 Acq On : 15 Mar 2022 15:38
 Operator : CG/JU
 Sample : PB143358BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143358BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.710	388	395	403	rBV	786080	1260531	32.14%	8.869%
2	7.302	656	666	675	rBV	780296	1396224	35.60%	9.824%
3	8.154	803	811	819	rBV	140001	243775	6.22%	1.715%
4	9.317	997	1009	1017	rBV	468219	852714	21.74%	6.000%
5	10.968	1283	1290	1299	rVB	192001	342295	8.73%	2.408%
6	13.406	1697	1705	1715	rVB	1319942	2037001	51.94%	14.332%
7	14.774	1931	1938	1947	rVB	302533	480284	12.25%	3.379%
8	16.255	2182	2190	2200	rBV	1000757	1536303	39.17%	10.809%
9	17.518	2399	2405	2412	rBV	431032	638064	16.27%	4.489%
10	20.126	2843	2849	2854	rBV	2792804	3922012	100.00%	27.595%
11	21.806	3129	3135	3142	rVB2	477558	781924	19.94%	5.501%
12	25.131	3692	3701	3713	rVB	241790	721854	18.41%	5.079%




Sum of corrected areas: 14212981

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
Data File : BG052667.D
Acq On : 15 Mar 2022 15:38
Operator : CG/JU
Sample : PB143358BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

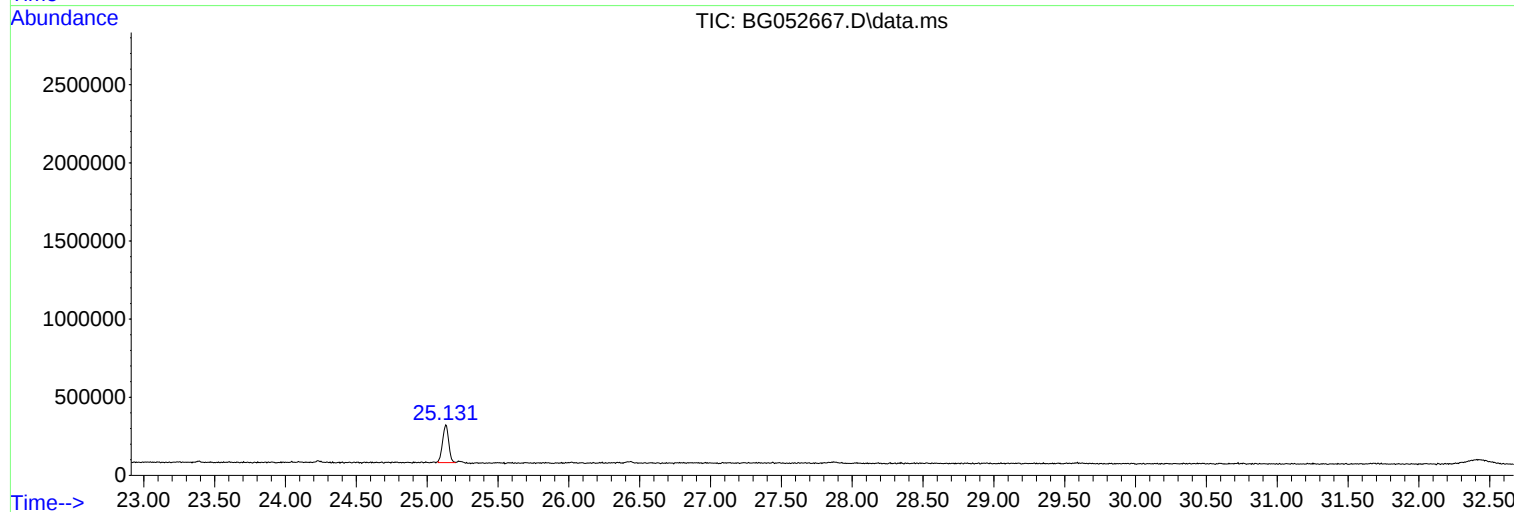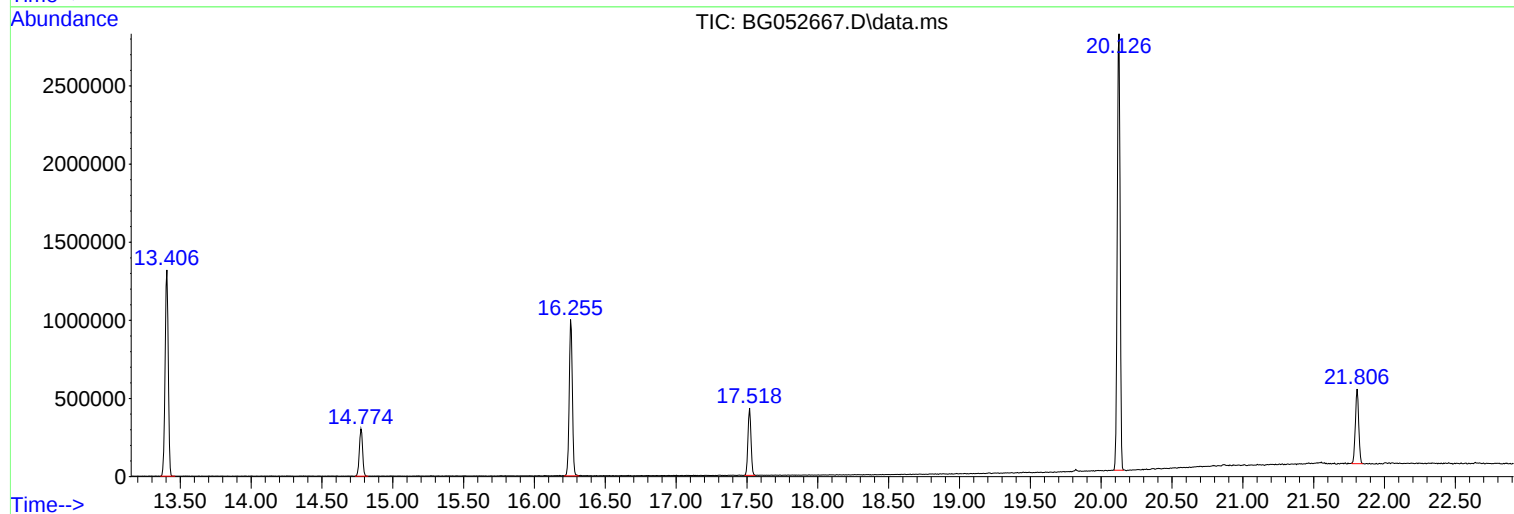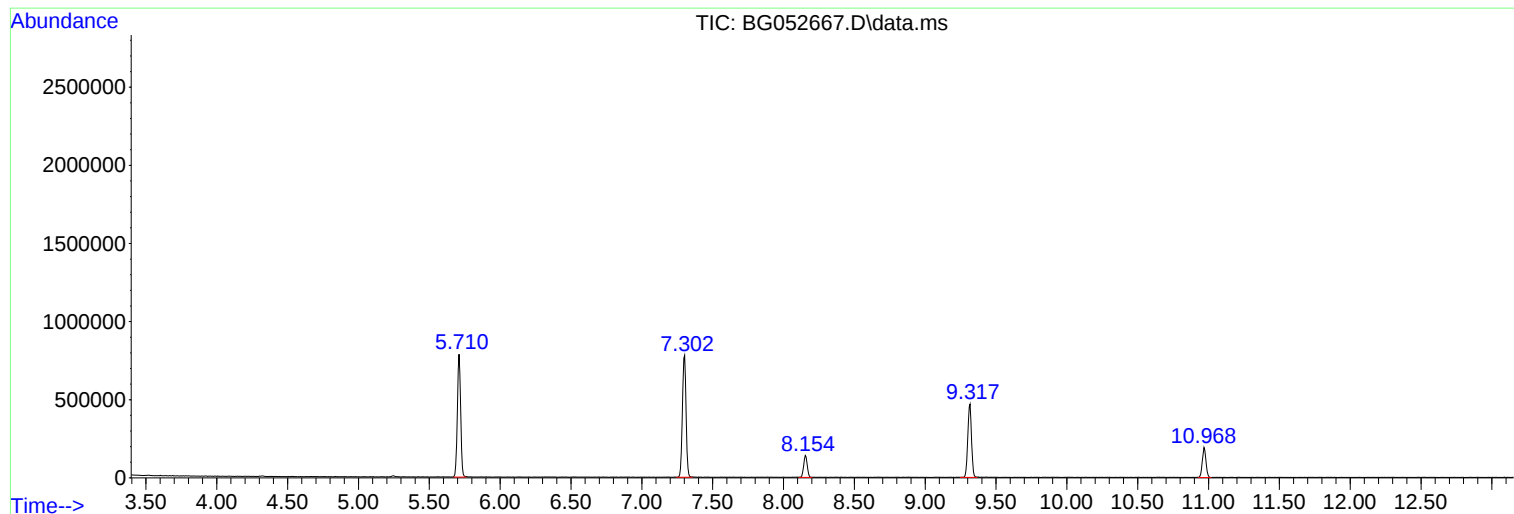

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
Data File : BG052667.D
Acq On : 15 Mar 2022 15:38
Operator : CG/JU
Sample : PB143358BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
Data File : BG052667.D
Acq On : 15 Mar 2022 15:38
Operator : CG/JU
Sample : PB143358BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143358BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------