
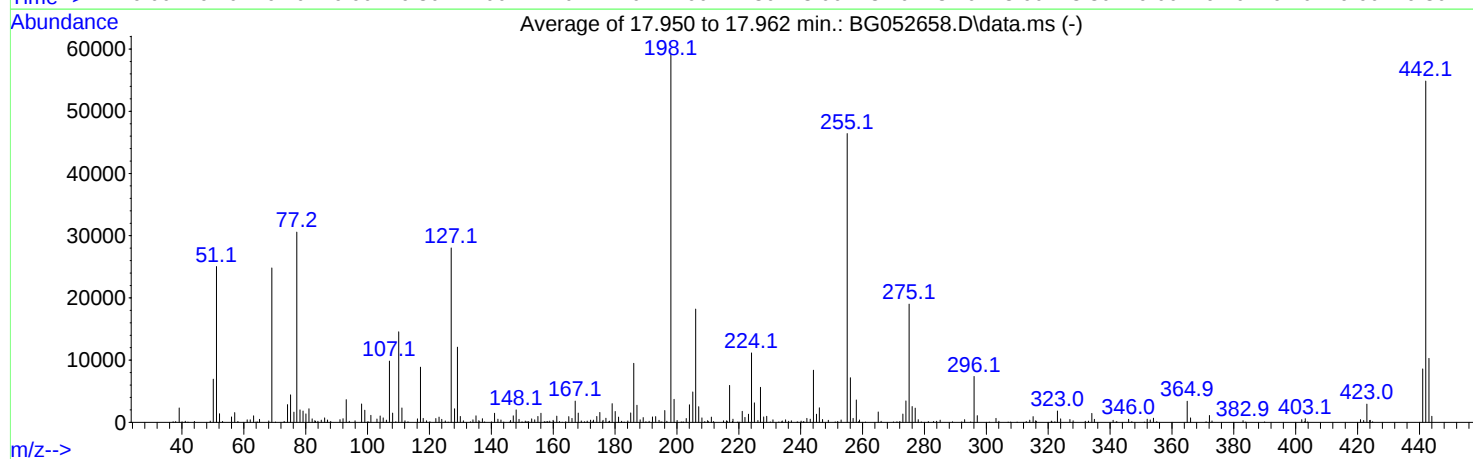


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
 Data File : BG052658.D
 Acq On : 15 Mar 2022 9:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 15 15:56:10 2022

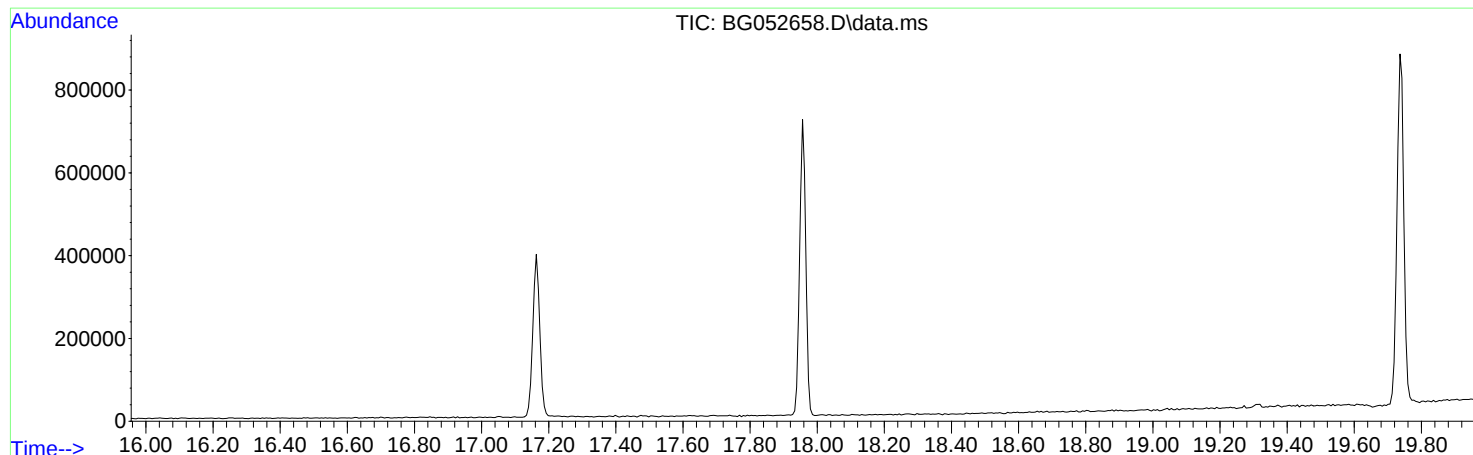




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	25040	PASS
68	69	0.00	2	1.0	238	PASS
69	198	0.00	100	42.0	24816	PASS
70	69	0.00	2	0.2	60	PASS
127	198	10	80	47.4	28029	PASS
197	198	0.00	2	0.3	168	PASS
198	198	100	100	100.0	59125	PASS
199	198	5	9	6.3	3708	PASS
275	198	10	60	32.1	18994	PASS
365	198	1	100	5.7	3390	PASS
441	198	0.01	100	14.5	8592	PASS
442	442	50	100	100.0	54845	PASS
443	442	15	24	18.8	10286	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
Data File : BG052658.D
Acq On : 15 Mar 2022 9:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 15 11:46:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 11:46:28 2022
Response via : Initial Calibration

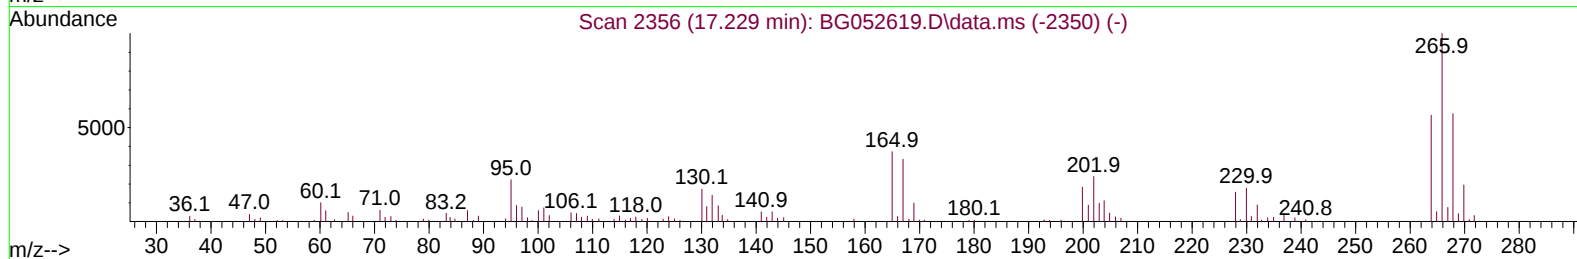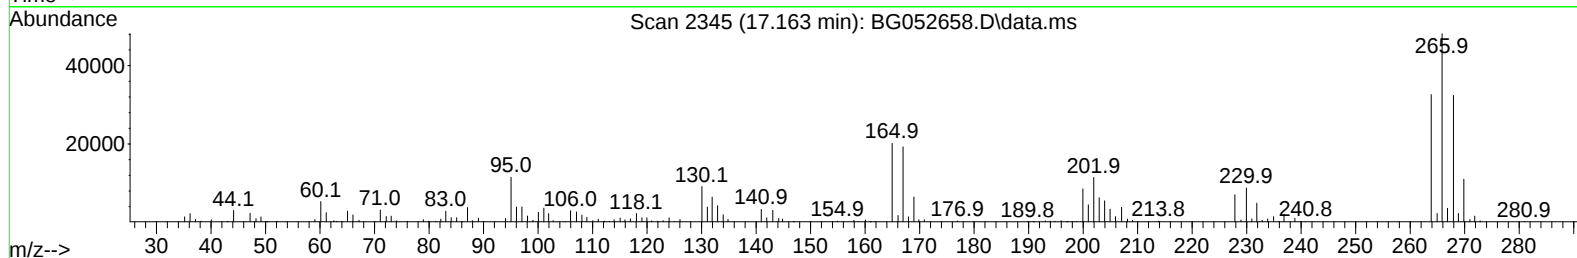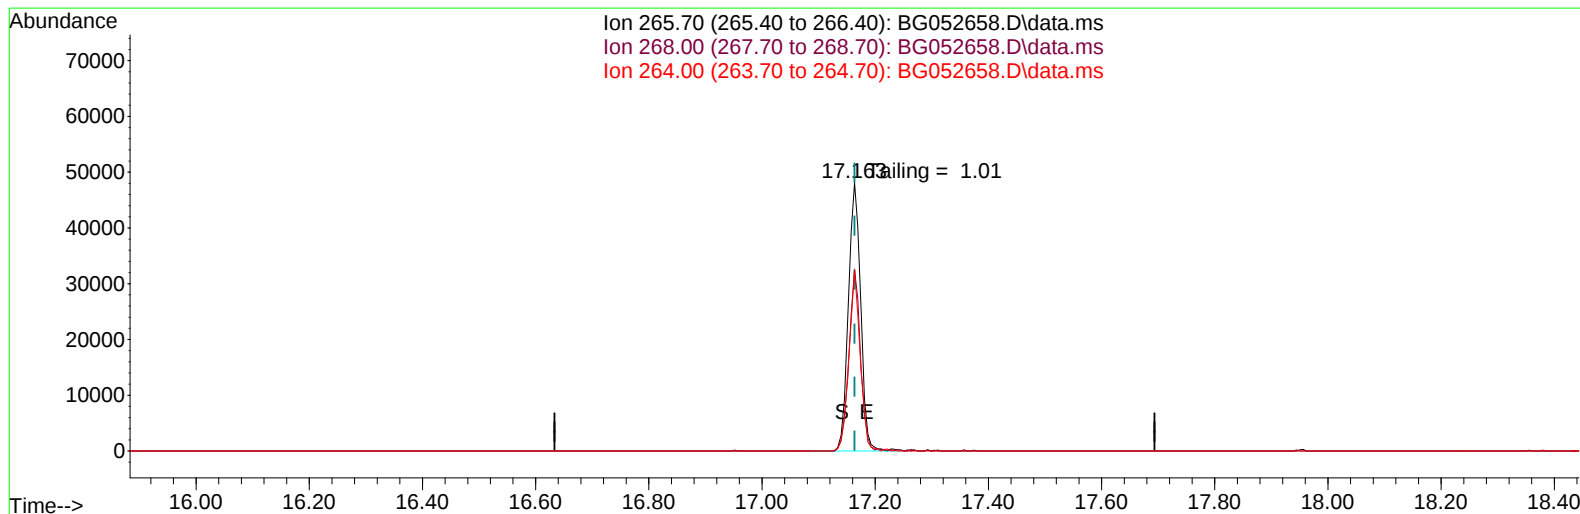

TIC: BG052658.D\data.ms

(70) Pentachlorophenol (C)

17.163min (0.000) 28646.61 ng




response 72352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.35
264.00	56.60	67.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031522\
 Data File : BG052658.D
 Acq On : 15 Mar 2022 9:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 15 11:46:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 11:46:28 2022
 Response via : Initial Calibration

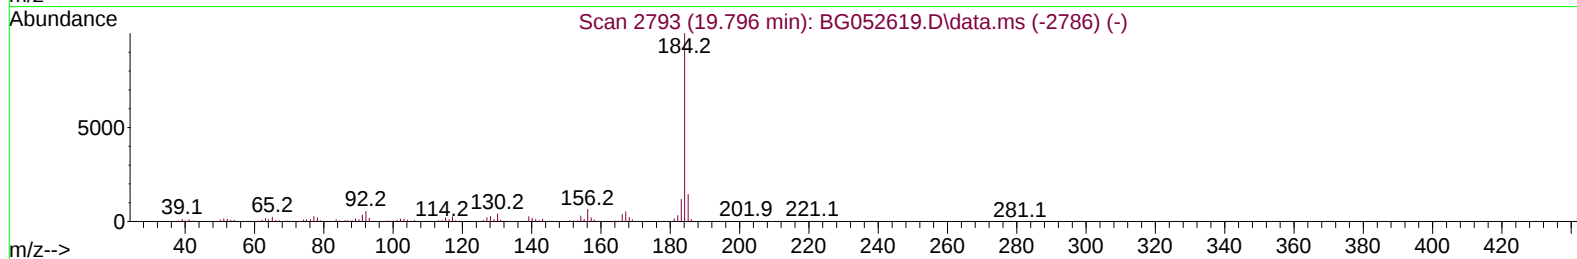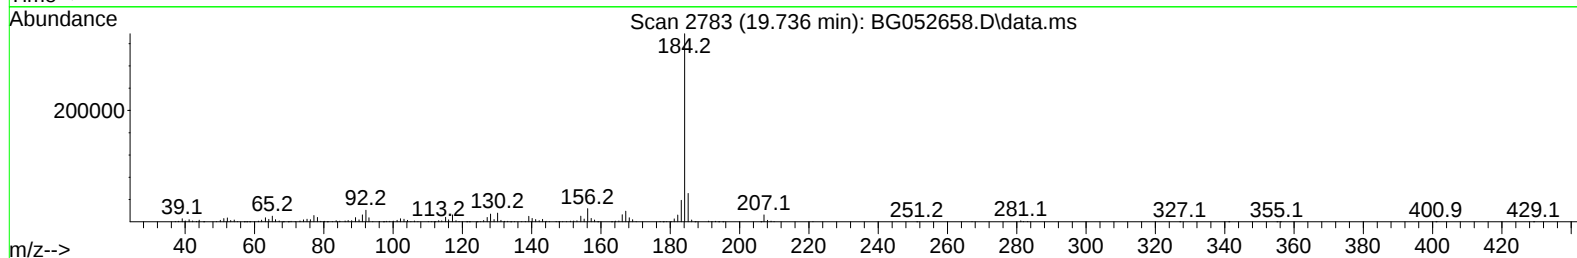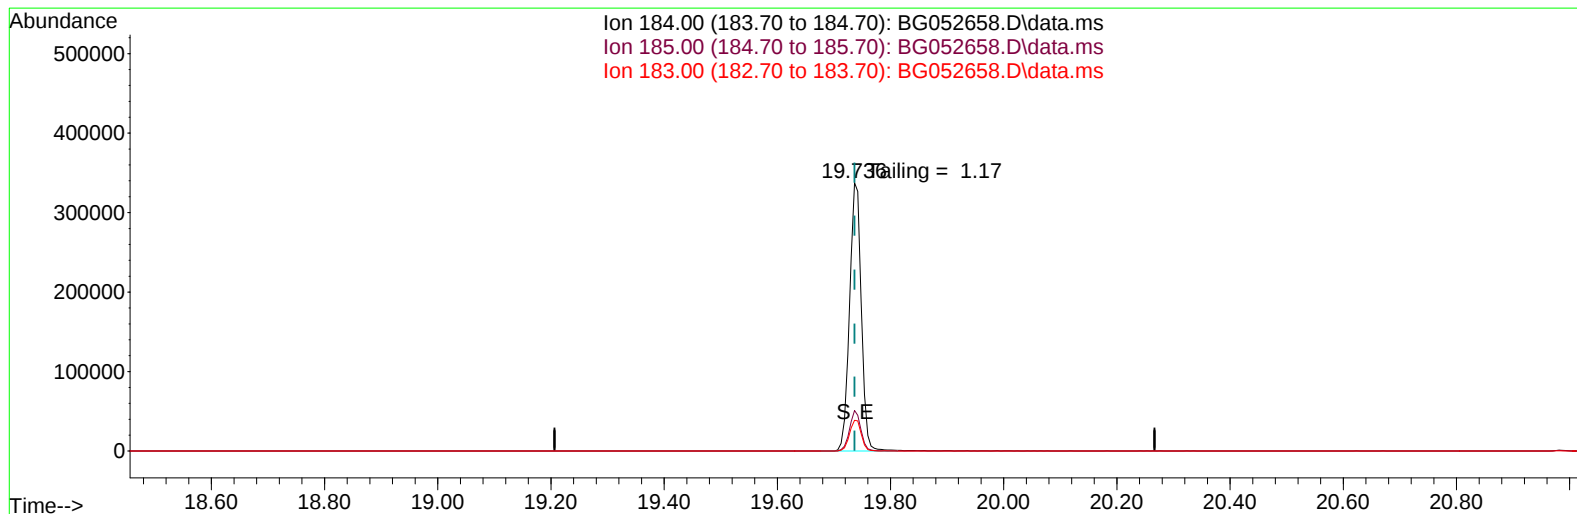

TIC: BG052658.D\data.ms

(77) Benzidine

19.736min (0.000) 426525.49 ng

response 486644

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.11
183.00	11.80	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/15/2022	BNA_G	<u>BG052658.D</u>
Compound Name	Response	Retention Time
DDT	200565	20.98
DDD	601	20.52
DDE	0	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
601	201166	0.30

Instrument :
BNA_G
ClientSampleId :
DFTPP