
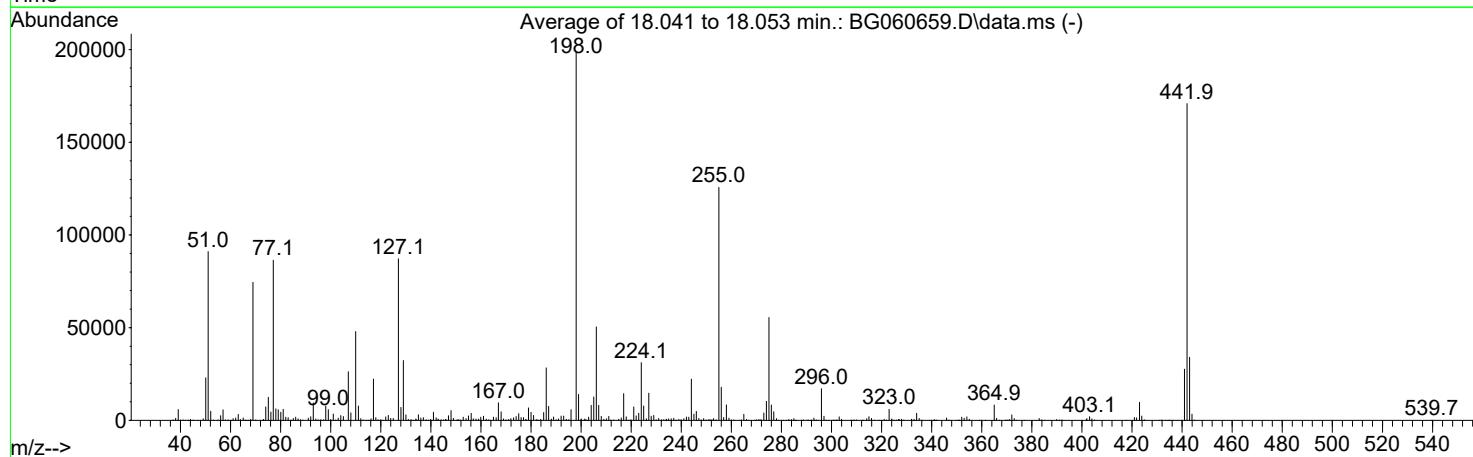


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031524\
Data File : BG060659.D
Acq On : 15 Mar 2024 11:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 00:45:22 2024

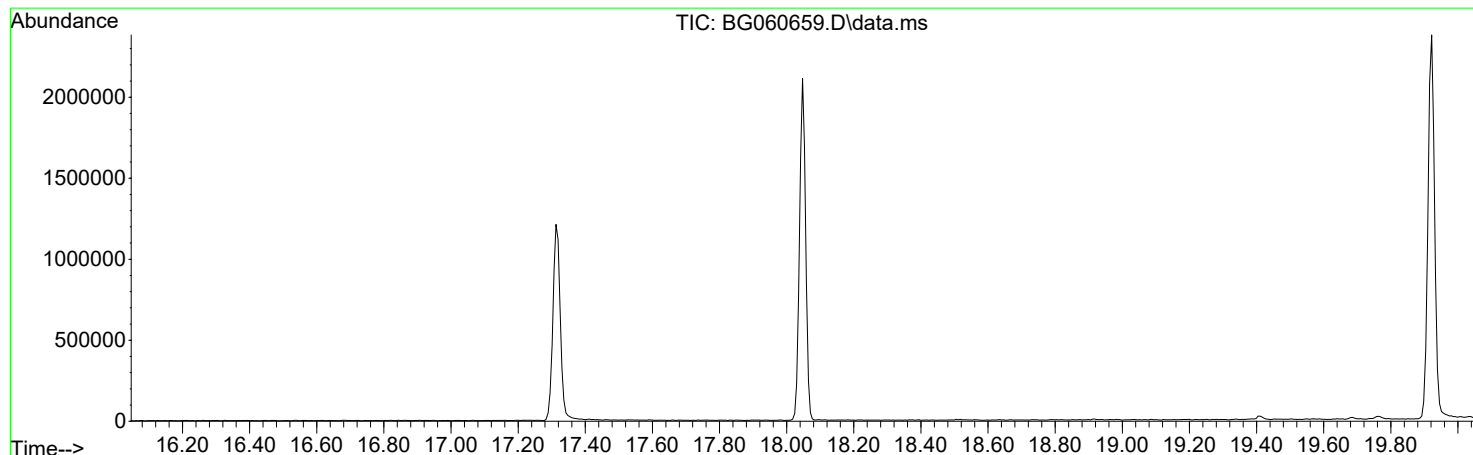

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.9	91094	PASS
68	69	0.00	2	0.8	604	PASS
69	198	0.00	100	37.5	74459	PASS
70	69	0.00	2	0.3	229	PASS
127	198	10	80	43.9	87192	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	198421	PASS
199	198	5	9	7.1	14029	PASS
275	198	10	60	28.0	55536	PASS
365	198	1	100	4.2	8291	PASS
441	198	0.01	100	13.9	27648	PASS
442	442	50	100	100.0	170888	PASS
443	442	15	24	19.9	34037	PASS