
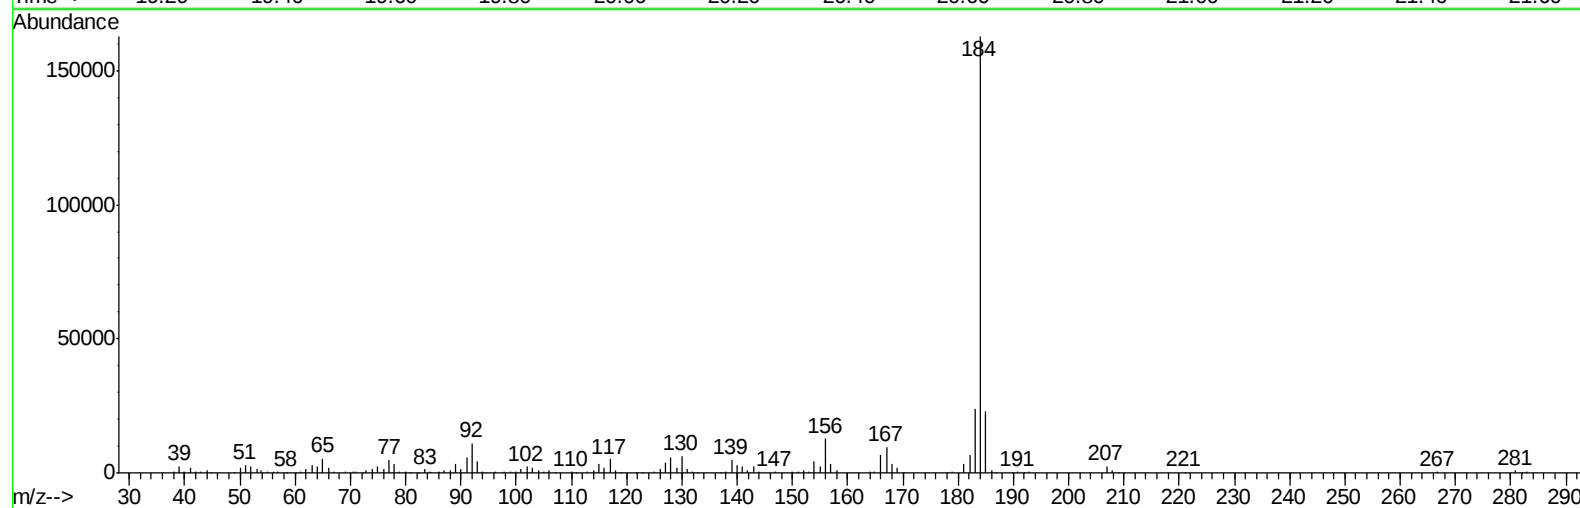


Data Path : Z:\HPCHEM1\BNA G\Data\BG031618\
Data File : BG033195.D
Acq On : 16 Mar 2018 11:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 05:58:47 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 13:59:34 2018
Response via : Initial Calibration

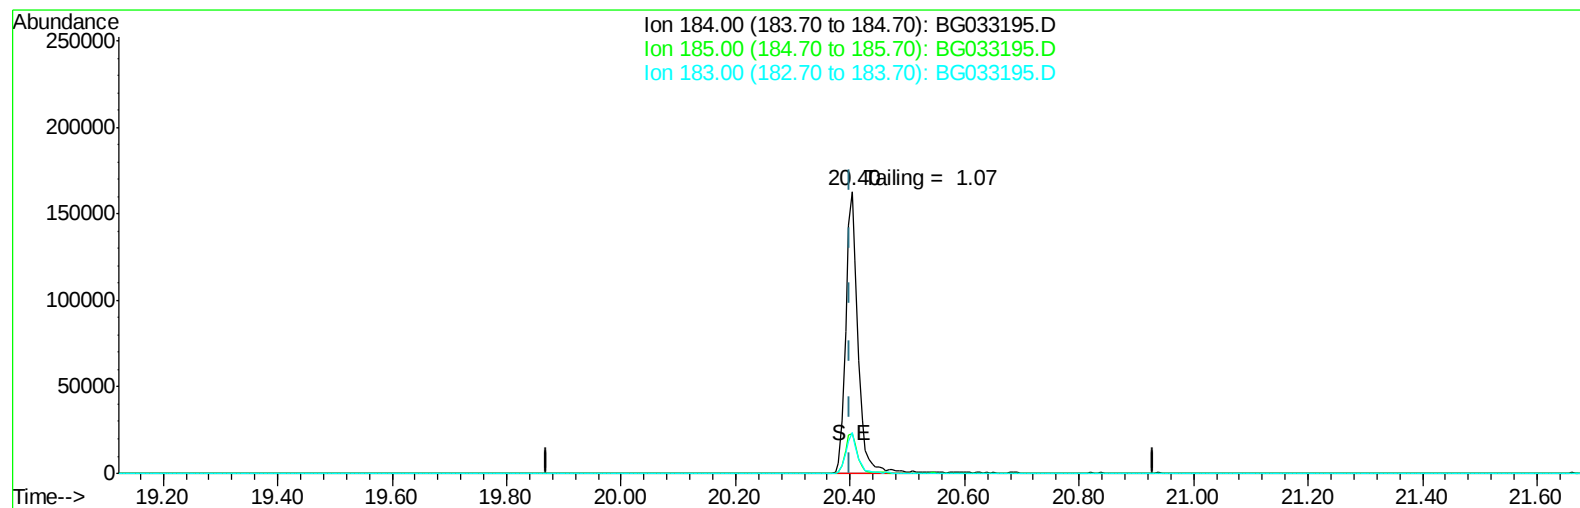

TIC: BG033195.D

(76) Benzidine



20.403min (+0.004) 0.00ng

response 245188

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.20
183.00	13.30	14.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG031618\
Data File : BG033195.D
Acq On : 16 Mar 2018 11:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 05:58:47 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 13:59:34 2018
Response via : Initial Calibration

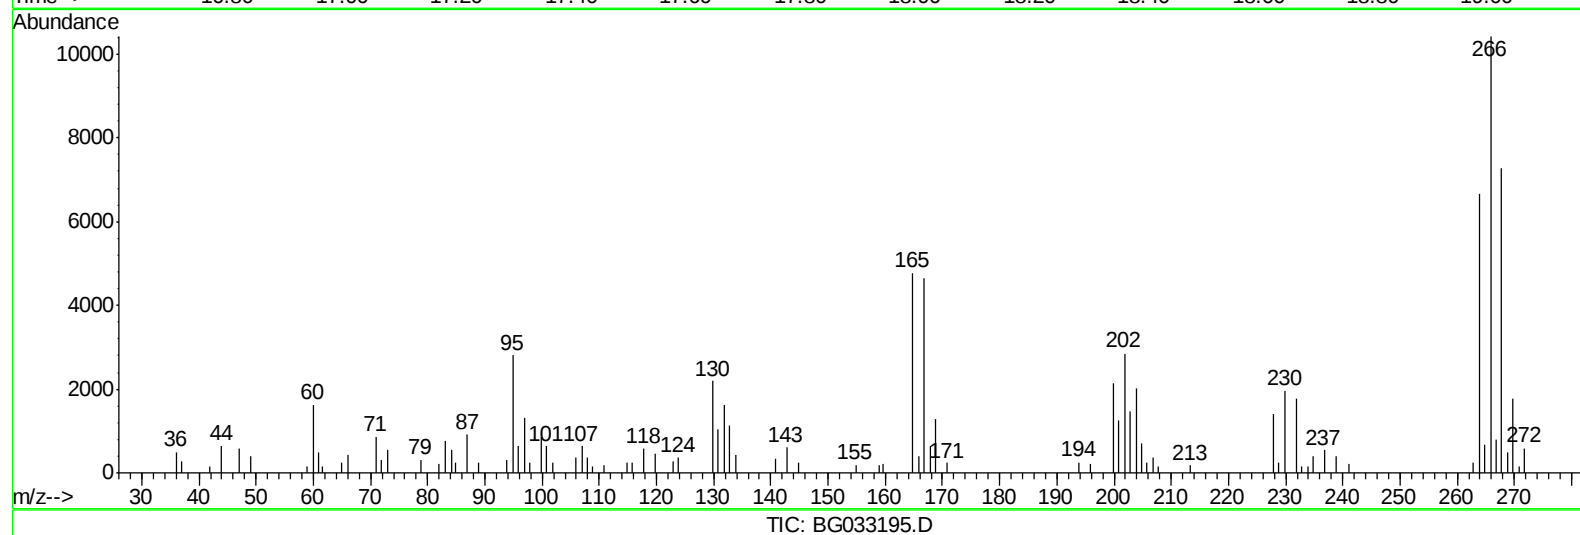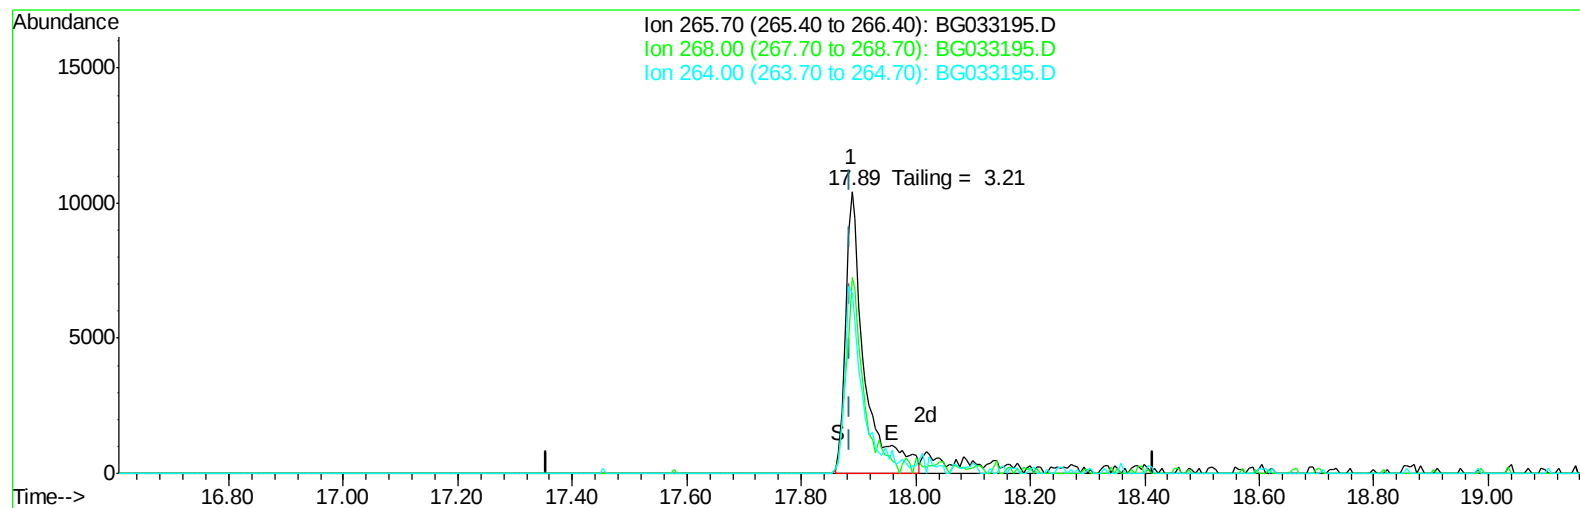

(69) Pentachlorophenol (C)

17.889min (+0.003) 14424.37ng

response 21906

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.74
264.00	62.00	64.07
0.00	0.00	0.00