

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031618\
 Data File : BG033211.D
 Acq On : 16 Mar 2018 22:25
 Operator : SJ/JU
 Sample : PB107389BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB107389BL

Quant Time: Mar 17 05:54:31 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 14 13:59:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.89	152	41149	20.00	ng	0.00
21) Naphthalene-d8	11.78	136	168547	20.00	ng	0.00
38) Acenaphthene-d10	15.51	164	116730	20.00	ng	0.00
63) Phenanthrene-d10	18.24	188	313163	20.00	ng	0.00
75) Chrysene-d12	22.60	240	324848	20.00	ng	-0.01
86) Perylene-d12	26.39	264	346943	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.31	112	338533	131.62	ng	0.00
7) Phenol-d6	8.00	99	487022	135.85	ng	-0.01
23) Nitrobenzene-d5	10.09	82	314375	124.25	ng	0.00
41) 2,4,6-Tribromophenol	16.99	330	205154	167.15	ng	0.00
44) 2-Fluorobiphenyl	14.14	172	722264	89.24	ng	0.00
78) Terphenyl-d14	20.76	244	1305201	90.27	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031618\
Data File : BG033211.D
Acq On : 16 Mar 2018 22:25
Operator : SJ/JU
Sample : PB107389BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB107389BL

Quant Time: Mar 17 05:54:31 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 14 13:59:34 2018
Response via : Initial Calibration

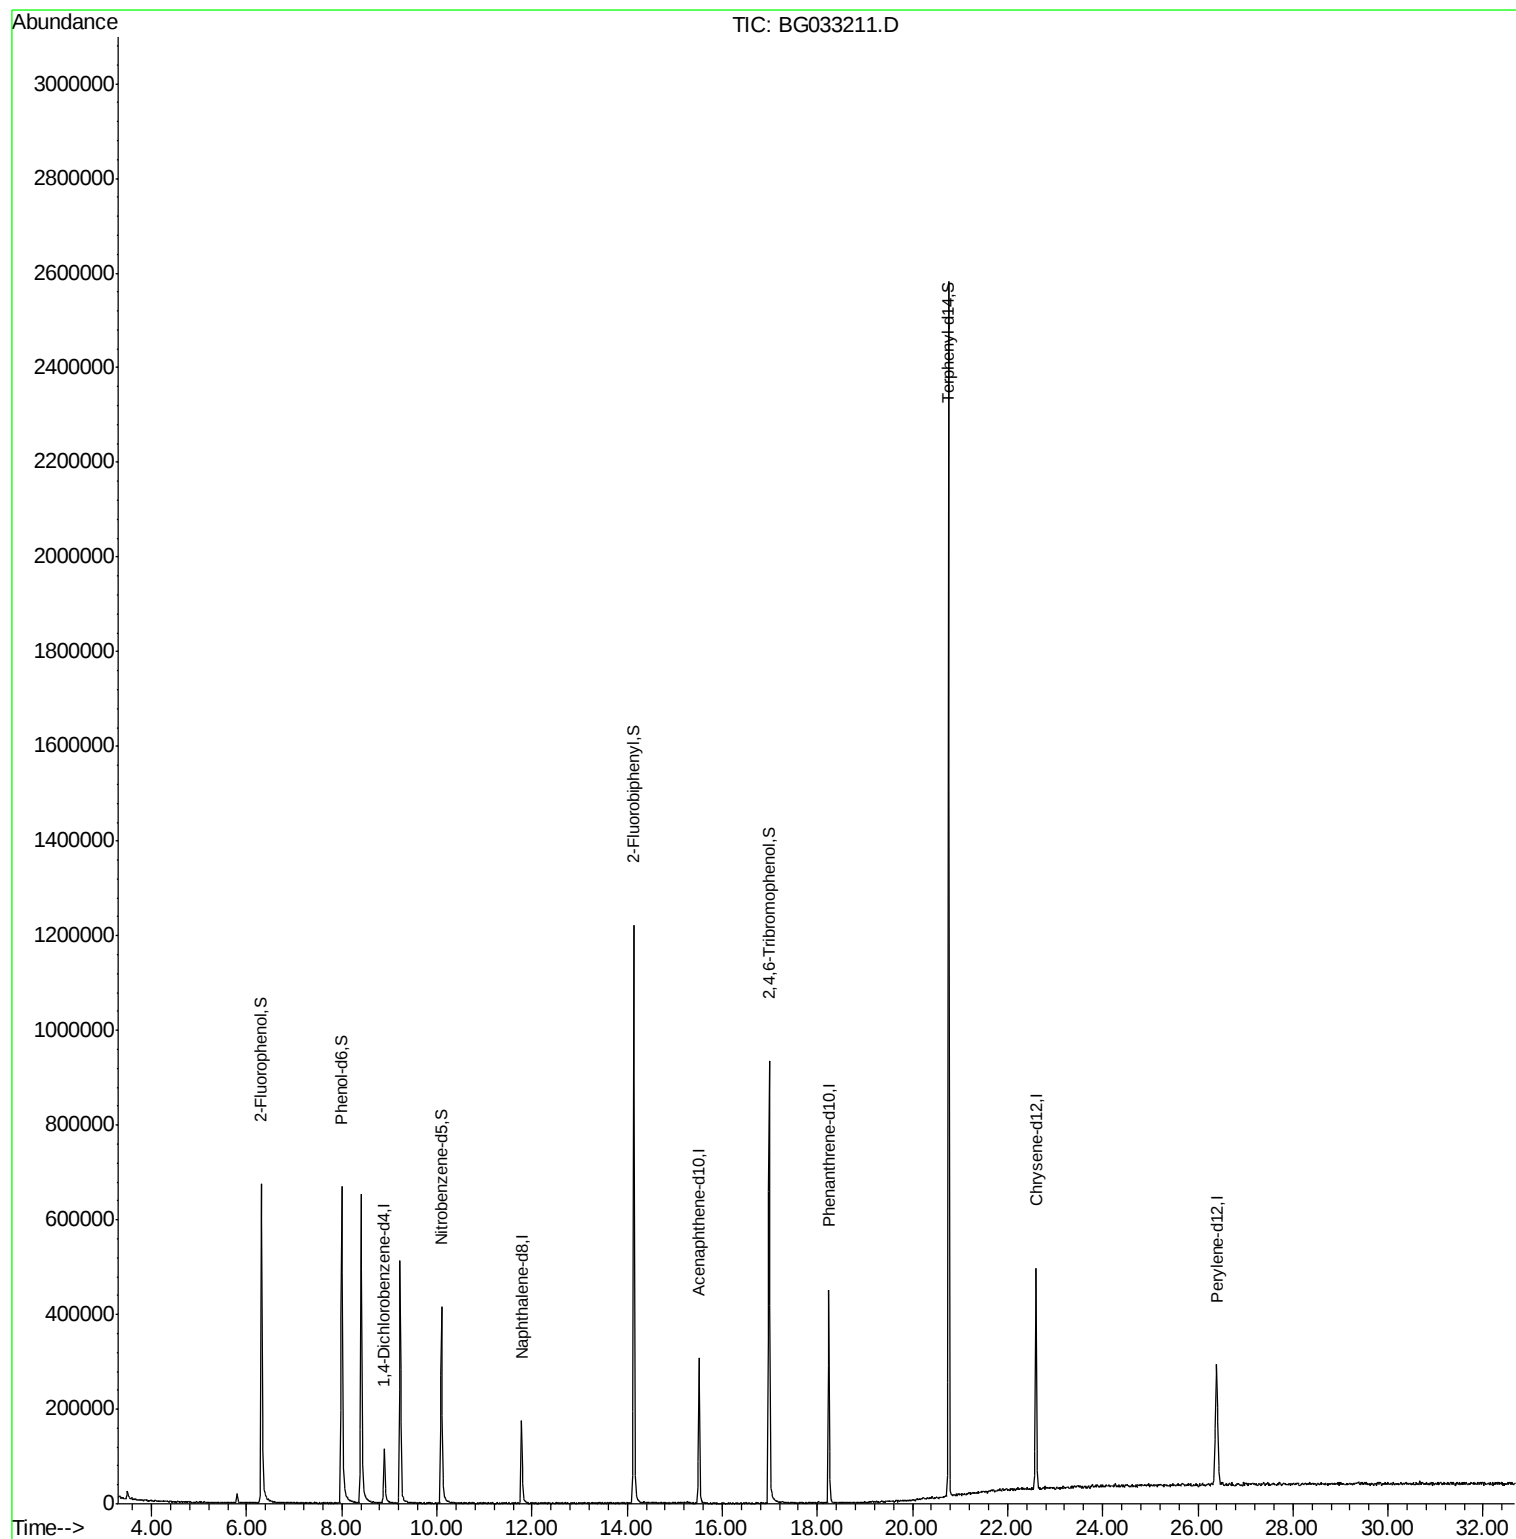

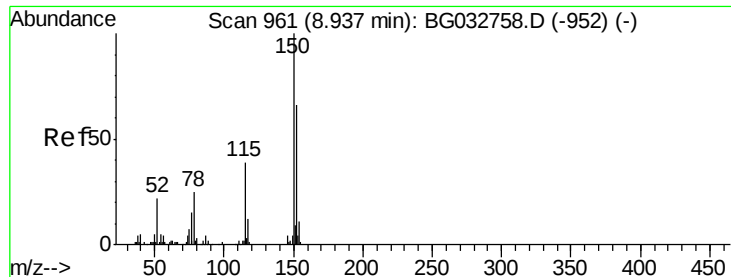


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.89 min Scan# 953
Delta R.T. -0.01 min
Lab File: BG033211.D
Acq: 16 Mar 2018 22:25

Instrument :
BNA_G
ClientSampleId :
PB107389BL

Tot Ion:152 Resp: 41149
Ion Ratio Lower Upper
152 100
150 155.7 126.6 189.8
115 63.1 53.0 79.4

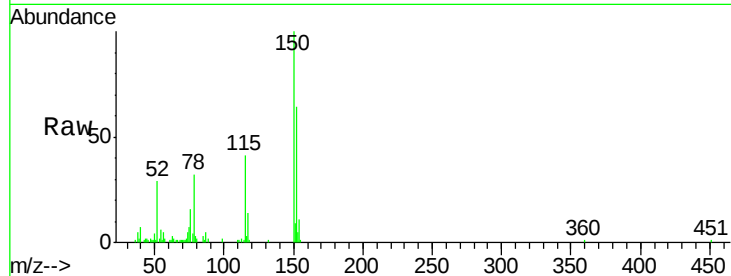


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

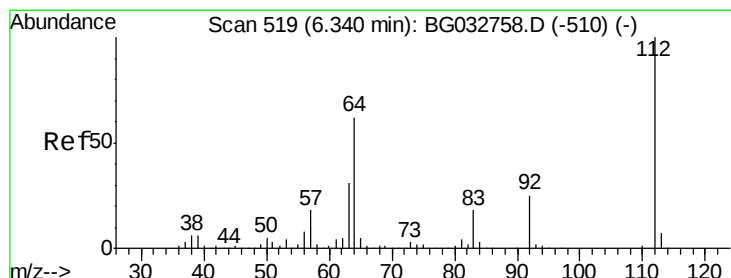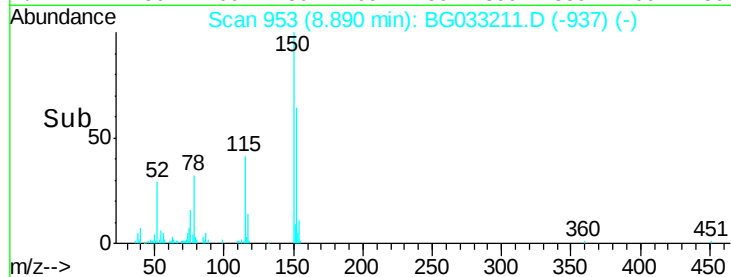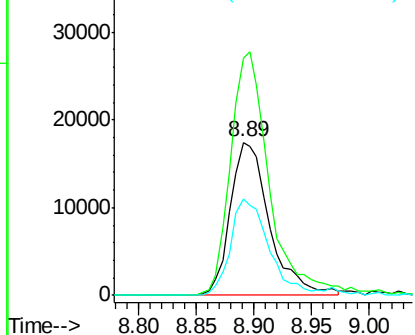



#5

2-Fluorophenol
Concen: 131.620 ng
RT: 6.31 min Scan# 514
Delta R.T. -0.01 min
Lab File: BG033211.D
Acq: 16 Mar 2018 22:25

Tgt Ion:112 Resp: 338533
Ion Ratio Lower Upper
112 100
64 74.1 56.3 84.5
63 42.6 30.1 45.1

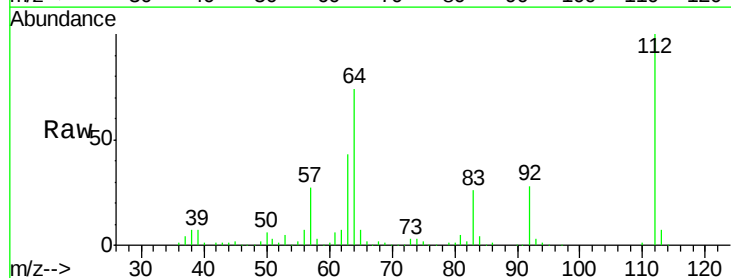

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

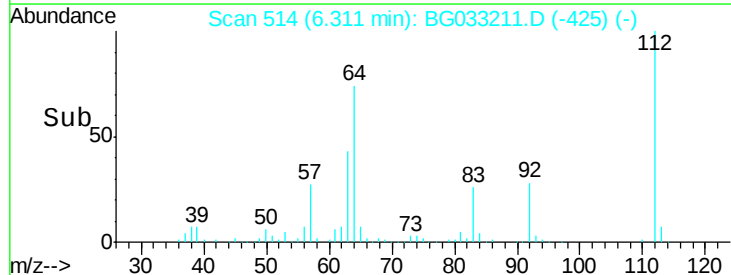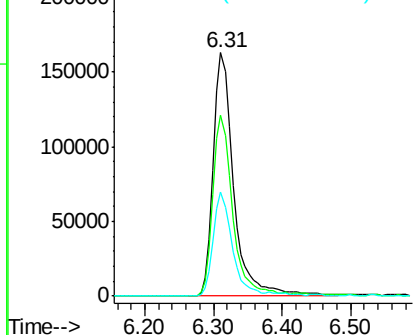



#7

Phenol-d6

Concen: 135.847 ng

RT: 8.00 min Scan# 801

Delta R.T. -0.01 min

Lab File: BG033211.D

Acq: 16 Mar 2018 22:25

Instrument :

BNA_G

ClientSampleId :

PB107389BL


Tot Ion: 99 Resp: 487022

Ion Ratio Lower Upper




99 100

42 20.6 14.1 21.1

71 39.9 26.1 39.1#

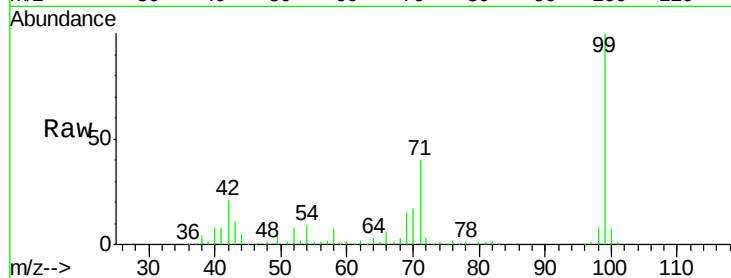

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

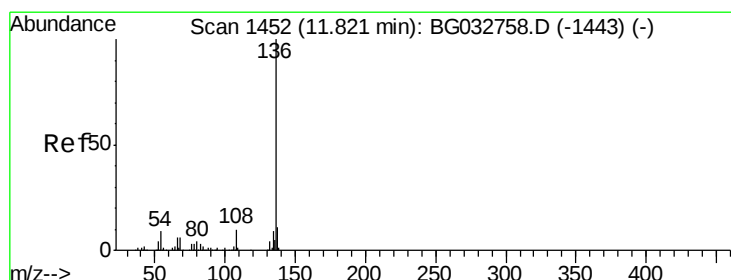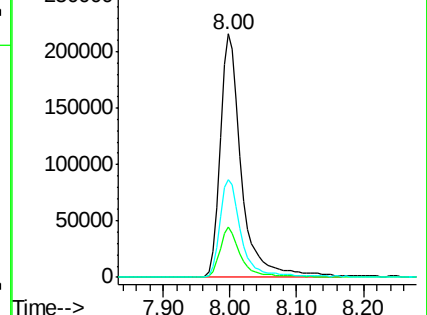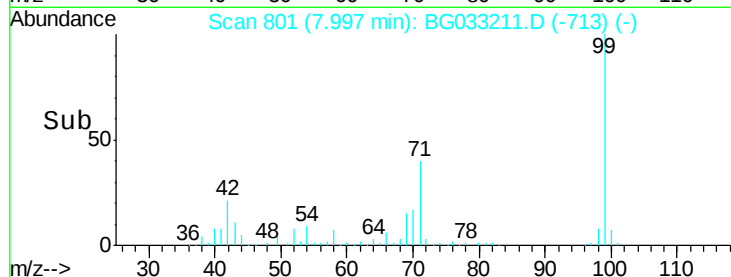

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.78 min Scan# 1445

Delta R.T. -0.01 min

Lab File: BG033211.D

Acq: 16 Mar 2018 22:25

Tgt Ion: 136 Resp: 168547


Ion Ratio Lower Upper

136 100



137 11.6 9.2 13.8


54 10.9 10.3 15.5

68 4.9 4.5 6.7

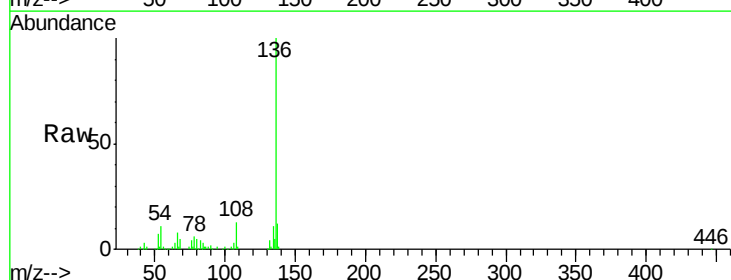

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

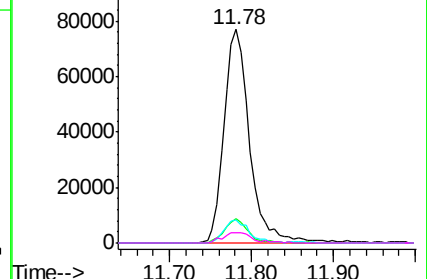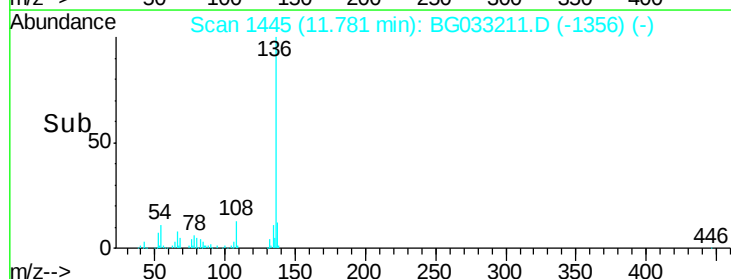

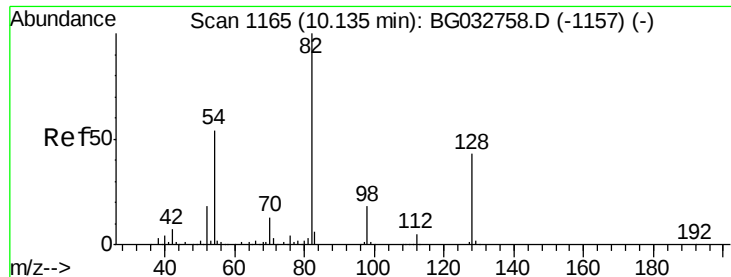

#23

Nitrobenzene-d5

Concen: 124.254 ng

RT: 10.09 min Scan# 1158

Delta R.T. -0.01 min

Lab File: BG033211.D

Acq: 16 Mar 2018 22:25

Instrument :

BNA_G

ClientSampleId :

PB107389BL





Tot Ion: 82 Resp: 314375

Ion Ratio Lower Upper

82 100

128 34.4 29.7 44.5

54 55.1 43.1 64.7

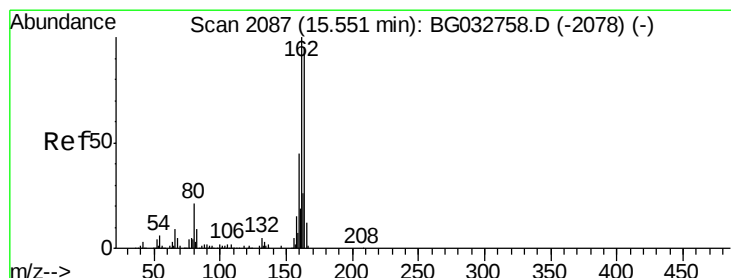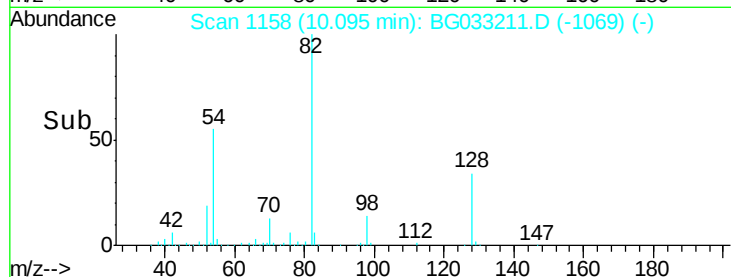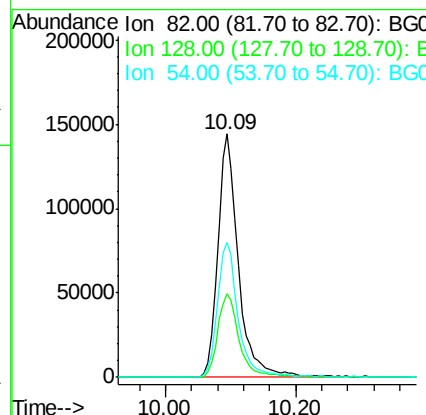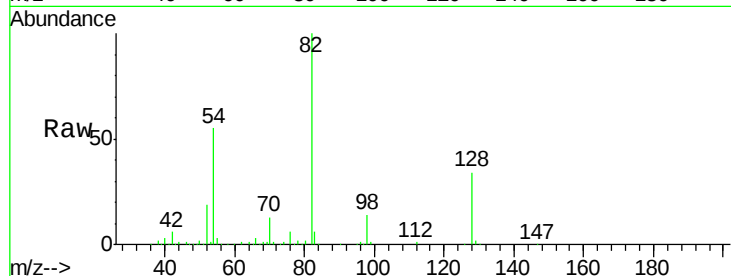

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.51 min Scan# 2080

Delta R.T. -0.01 min

Lab File: BG033211.D

Acq: 16 Mar 2018 22:25




Tgt Ion: 164 Resp: 116730


Ion Ratio Lower Upper

164 100

162 102.1 78.8 118.2

160 47.4 35.4 53.0

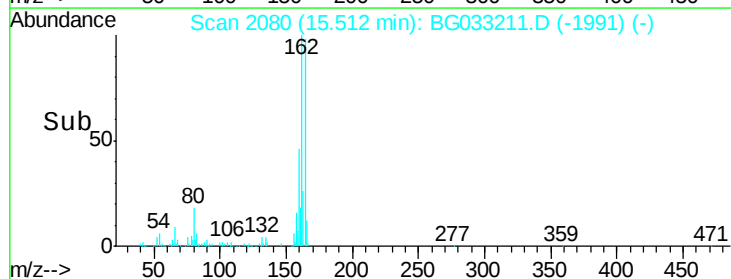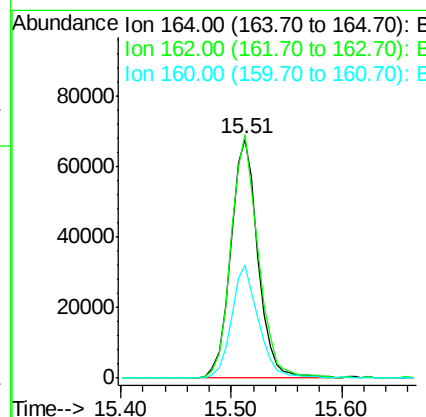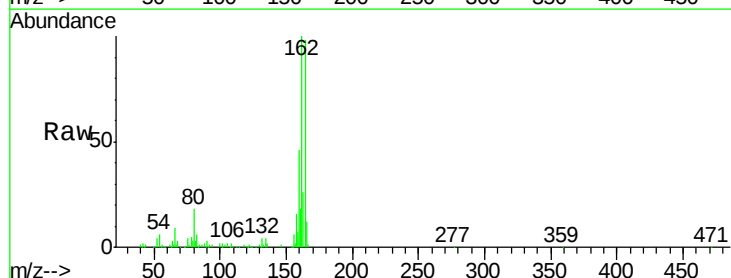


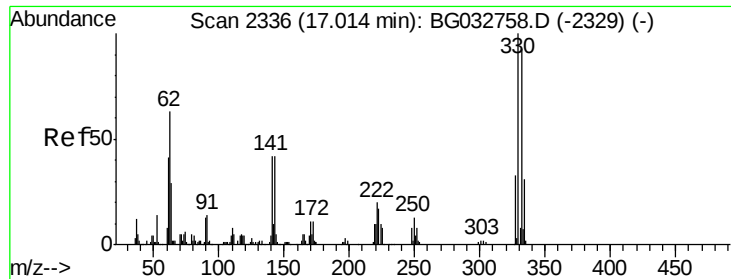

#41
 2,4,6-Tribromophenol
 Concen: 167.148 ng
 RT: 16.99 min Scan# 2331
 Delta R.T. -0.01 min
 Lab File: BG033211.D
 Acq: 16 Mar 2018 22:25

Instrument :
 BNA_G
 ClientSampleId :
 PB107389BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.0	115.6
141	36.2	25.2	37.8



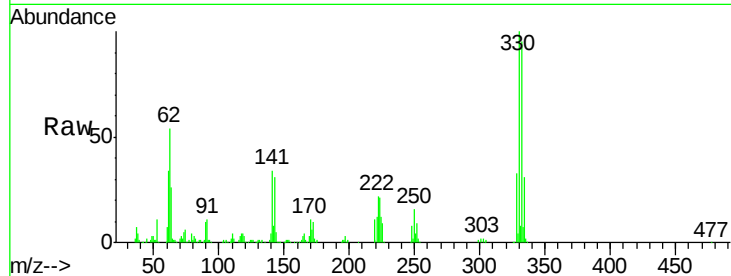


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

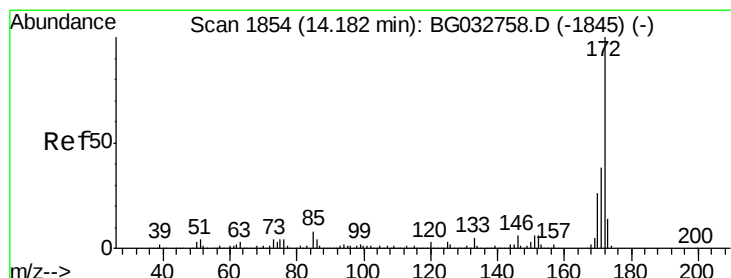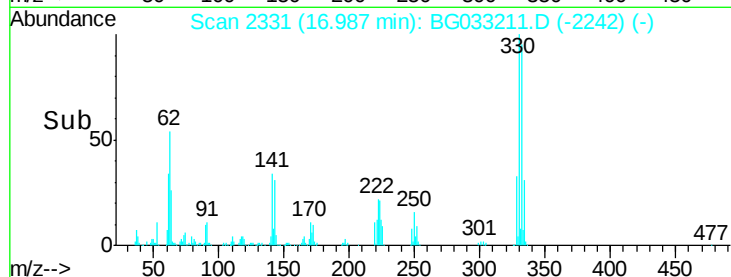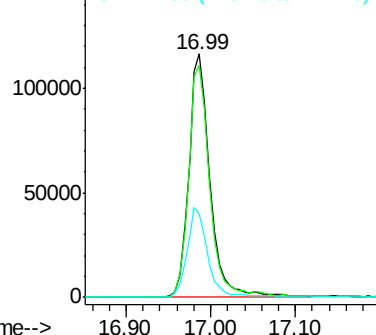

#44
 2-Fluorobiphenyl
 Concen: 89.239 ng
 RT: 14.14 min Scan# 1847
 Delta R.T. -0.00 min
 Lab File: BG033211.D
 Acq: 16 Mar 2018 22:25

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	30.0	45.0
170	25.1	19.5	29.3


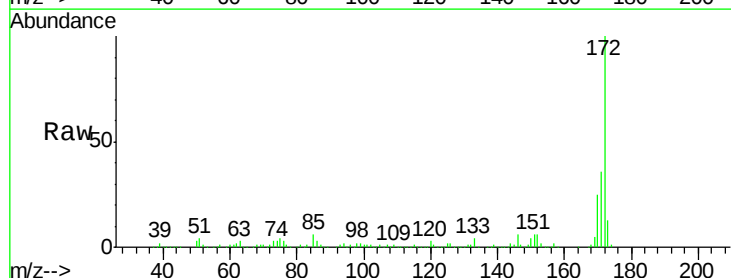



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



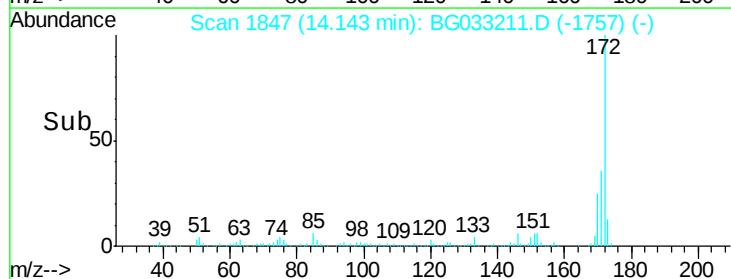
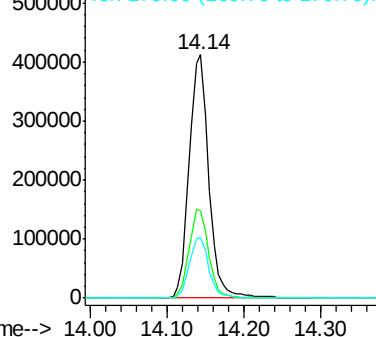


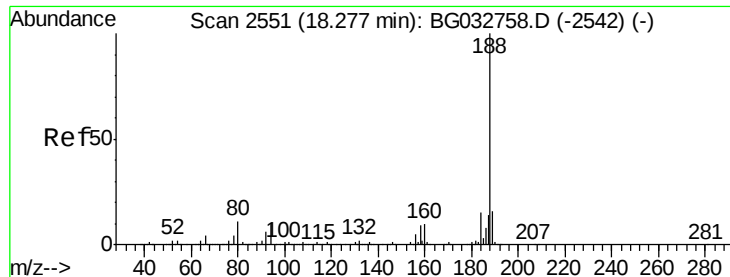

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.24 min Scan# 2545
Delta R.T. -0.01 min
Lab File: BG033211.D
Acq: 16 Mar 2018 22:25




Instrument :
BNA_G
ClientSampleId :
PB107389BL


Tot Ion:188 Resp: 313163
Ion Ratio Lower Upper
188 100
94 7.2 6.9 10.3
80 8.1 7.7 11.5

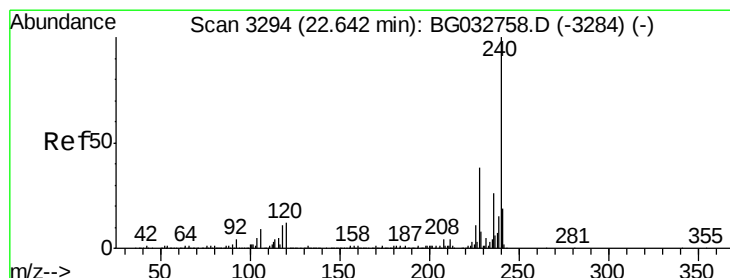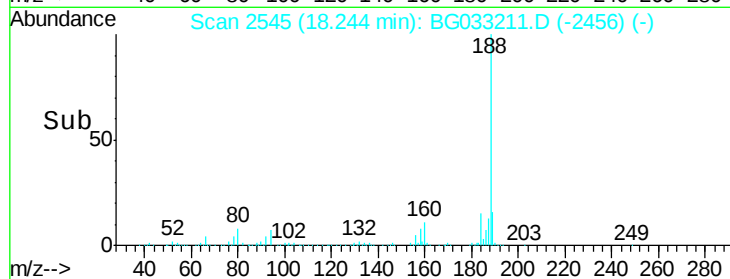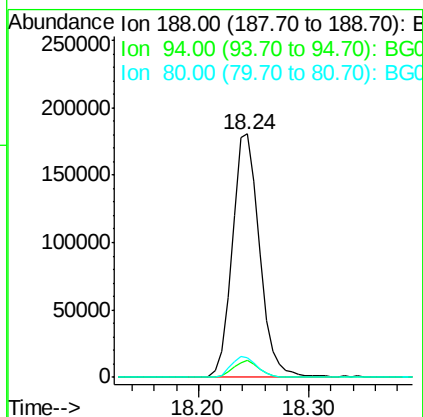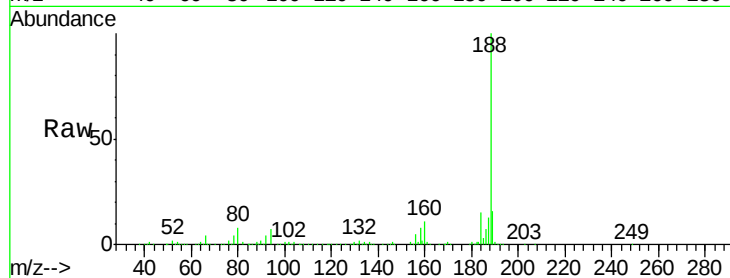

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.60 min Scan# 3286
Delta R.T. -0.01 min
Lab File: BG033211.D
Acq: 16 Mar 2018 22:25

Tgt Ion:240 Resp: 324848
Ion Ratio Lower Upper
240 100
120 6.8 6.8 10.2#
236 27.6 20.9 31.3

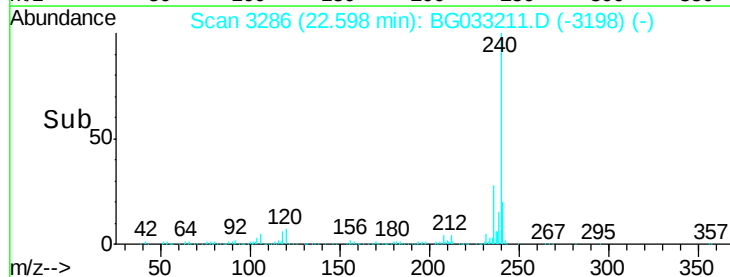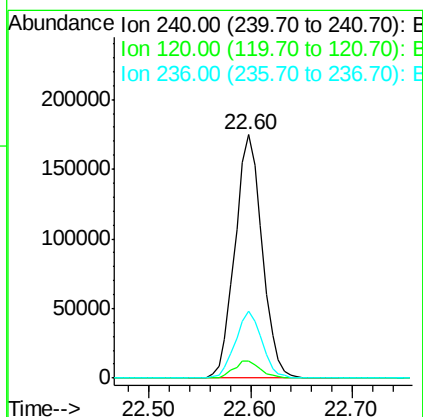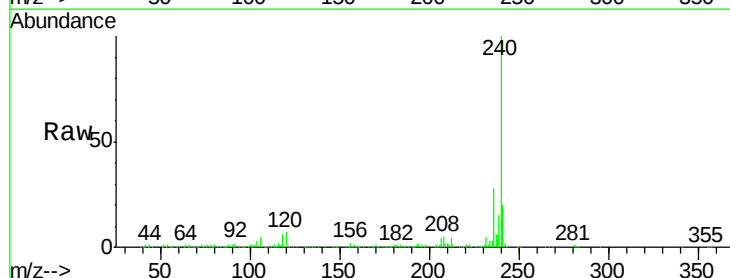

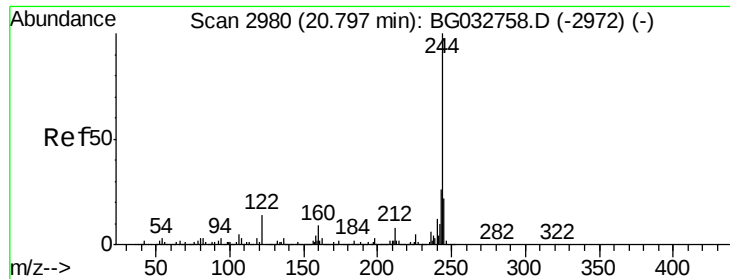

#78

Terphenyl-d14

Concen: 90.271 ng

RT: 20.76 min Scan# 2973

Delta R.T. -0.00 min

Lab File: BG033211.D

Acq: 16 Mar 2018 22:25

Instrument :

BNA_G

ClientSampleId :

PB107389BL


Tot Ion:244 Resp: 1305201

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#




122 7.7 7.0 10.4

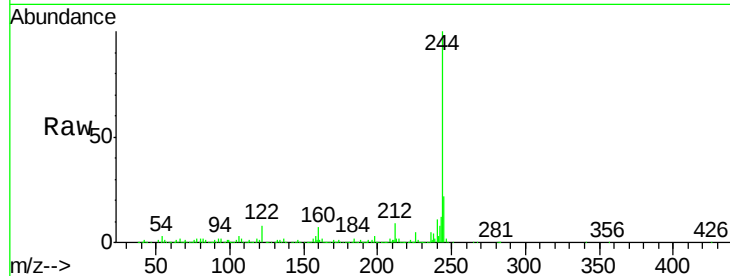

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

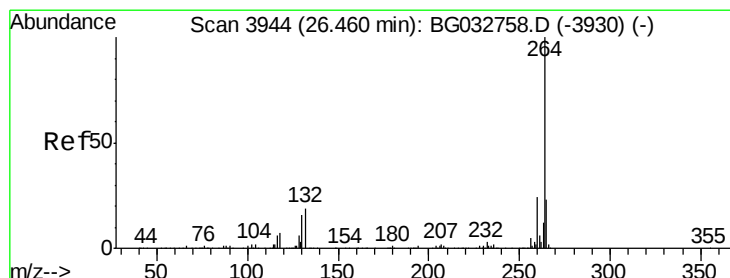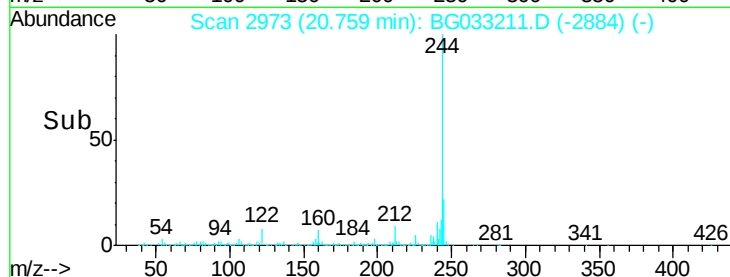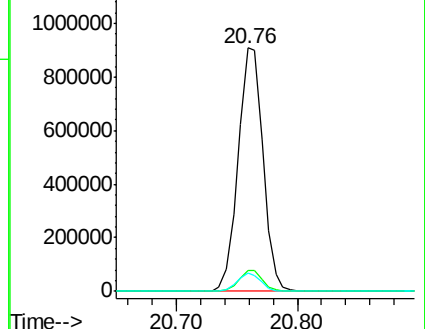

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.39 min Scan# 3932

Delta R.T. -0.02 min

Lab File: BG033211.D

Acq: 16 Mar 2018 22:25


Tgt Ion:264 Resp: 346943

Ion Ratio Lower Upper

264 100

260 21.8 17.4 26.0

265 22.2 17.7 26.5

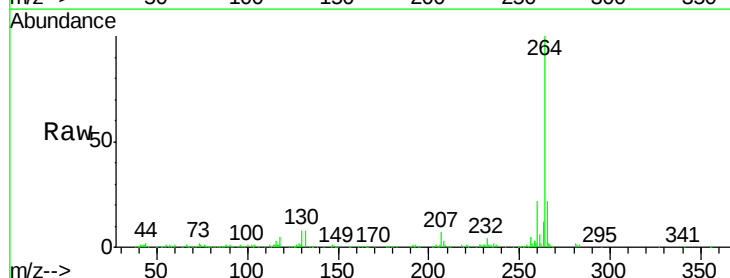

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

