

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031618\
 Data File : BG033211.D
 Acq On : 16 Mar 2018 22:25
 Operator : SJ/JU
 Sample : PB107389BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB107389BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.311	507	514	529	rBV	673779	1355326	37.59%	7.828%
2	7.997	794	801	819	rBV	667888	1472351	40.83%	8.504%
3	8.403	863	870	898	rBV	652533	1415428	39.25%	8.176%
4	8.890	946	953	964	rBV2	113851	256806	7.12%	1.483%
5	9.231	1003	1011	1026	rBV	511994	1044752	28.97%	6.035%
6	10.095	1149	1158	1177	rBV	415529	910447	25.25%	5.259%
7	11.781	1435	1445	1455	rBV	174173	369951	10.26%	2.137%
8	14.143	1839	1847	1861	rBV	1221637	2142914	59.43%	12.378%
9	15.512	2073	2080	2092	rBV2	307424	548341	15.21%	3.167%
10	16.987	2324	2331	2350	rBV	935183	1683894	46.70%	9.726%
11	18.244	2538	2545	2558	rBV2	449415	755020	20.94%	4.361%
12	20.759	2967	2973	2983	rBV	2566682	3605730	100.00%	20.827%
13	22.598	3279	3286	3294	rBV2	467975	881963	24.46%	5.094%
14	26.399	3920	3933	3946	rBV3	254799	869953	24.13%	5.025%


Sum of corrected areas: 17312876

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031618\
Data File : BG033211.D
Acq On : 16 Mar 2018 22:25
Operator : SJ/JU
Sample : PB107389BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB107389BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

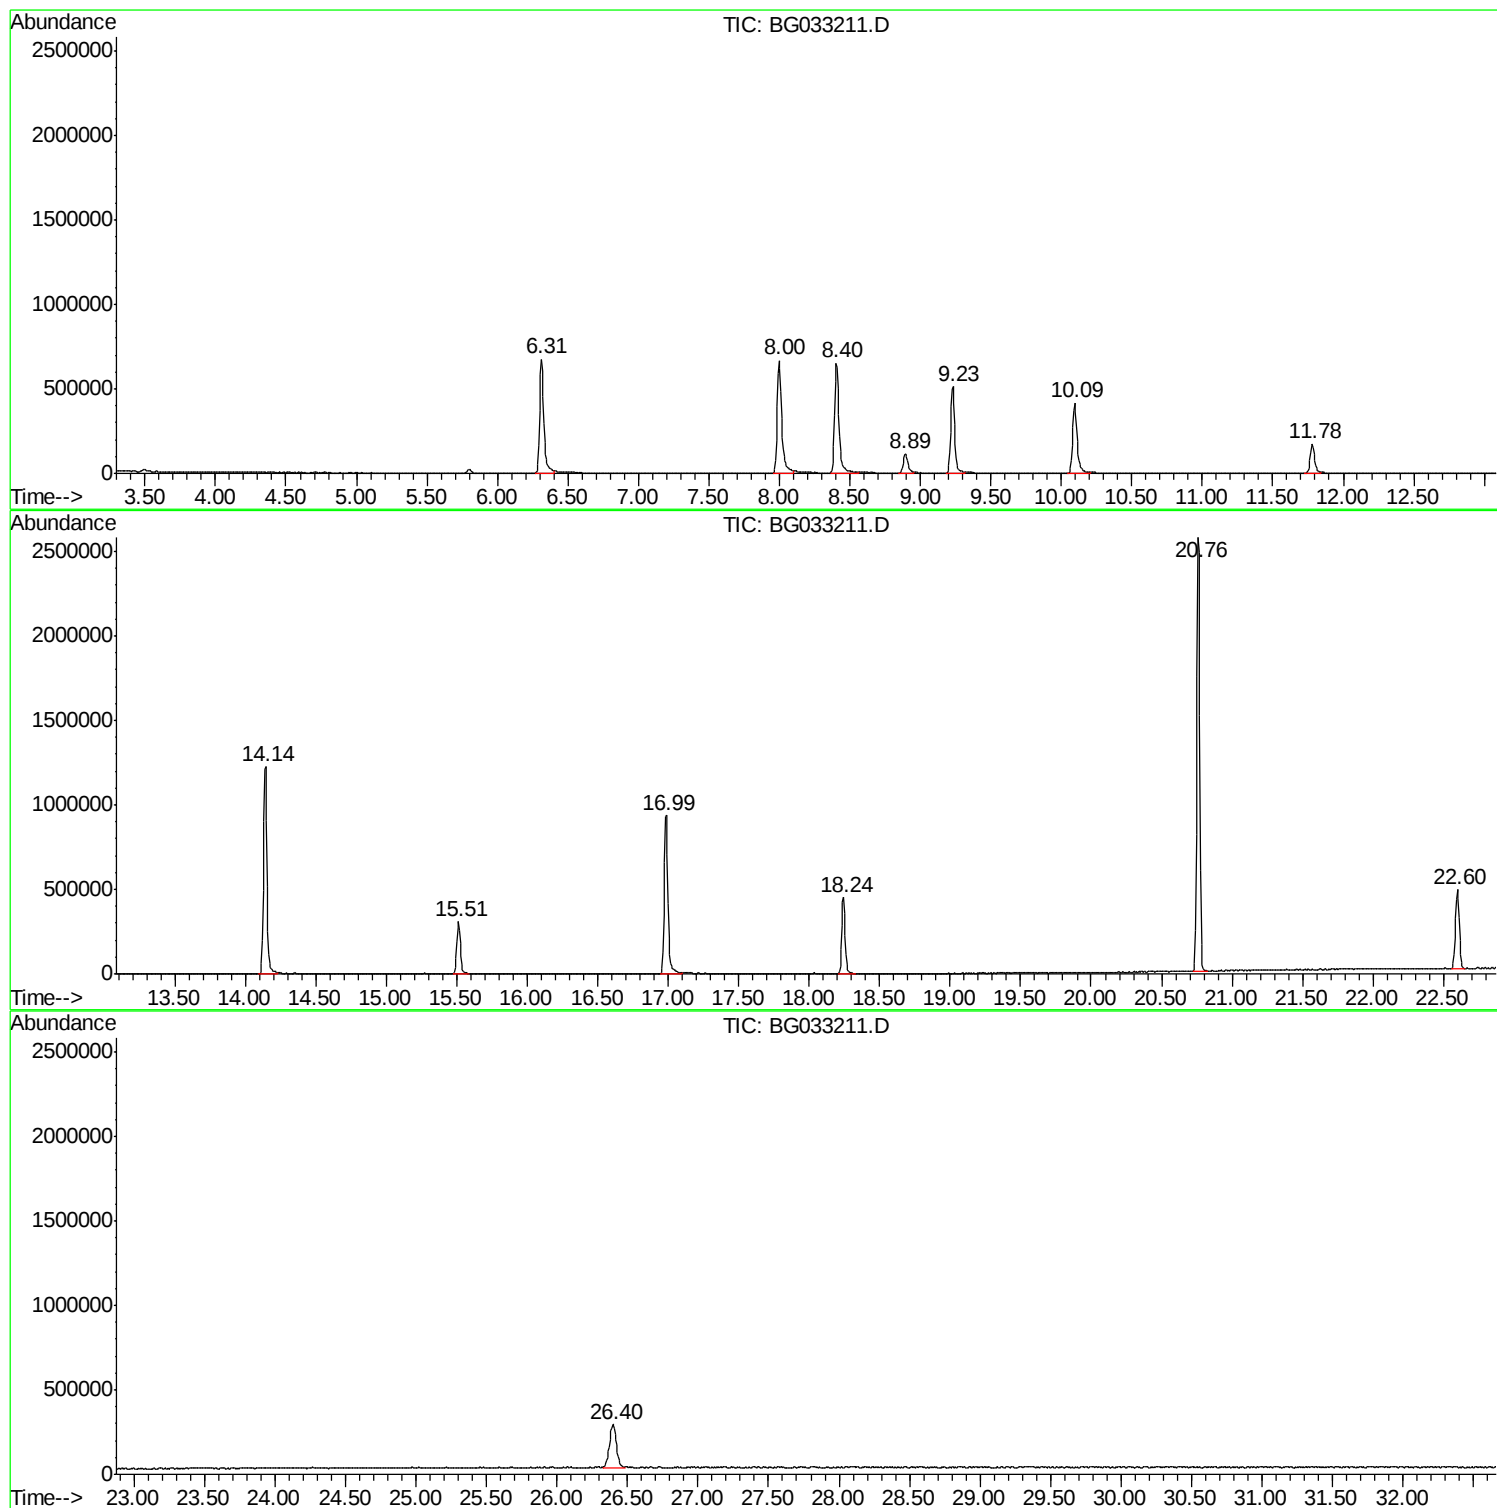

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031618\
Data File : BG033211.D
Acq On : 16 Mar 2018 22:25
Operator : SJ/JU
Sample : PB107389BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB107389BL










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown8.40 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.40	110.23 ng	1415430	1,4-Dichlorobenzene-d4	8.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	22
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

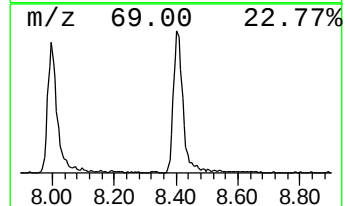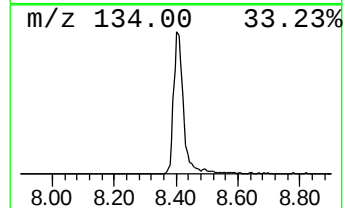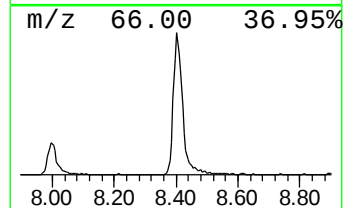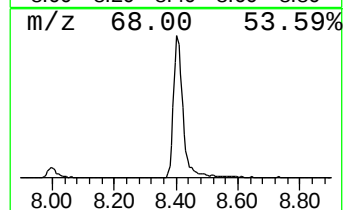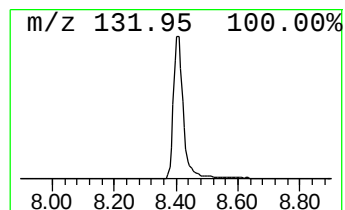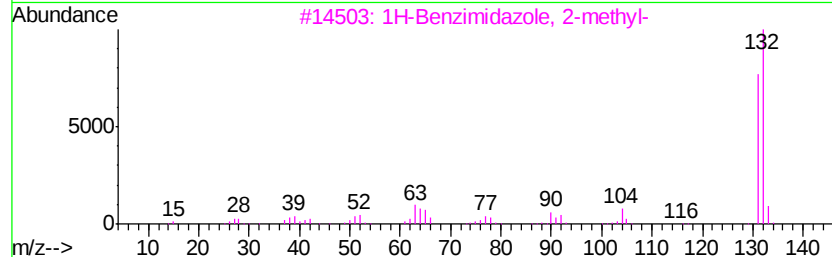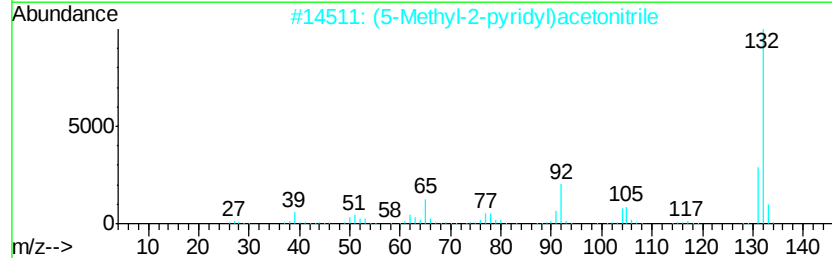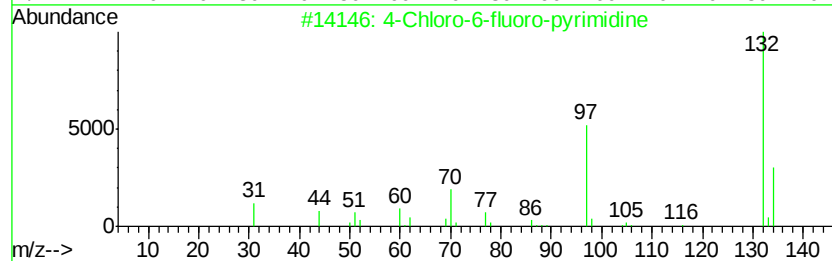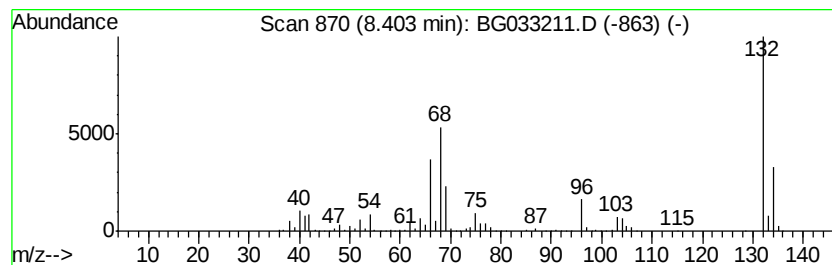

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031618\
Data File : BG033211.D
Acq On : 16 Mar 2018 22:25
Operator : SJ/JU
Sample : PB107389BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB107389BL

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.40	8.40	110.2	ng	1415430	1	8.89	256806	20.0