


Data Path : Z:\HPCHEM1\BNA G\Data\BG031618\
 Data File : BG033195.D
 Acq On : 16 Mar 2018 11:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 13:59:34 2018

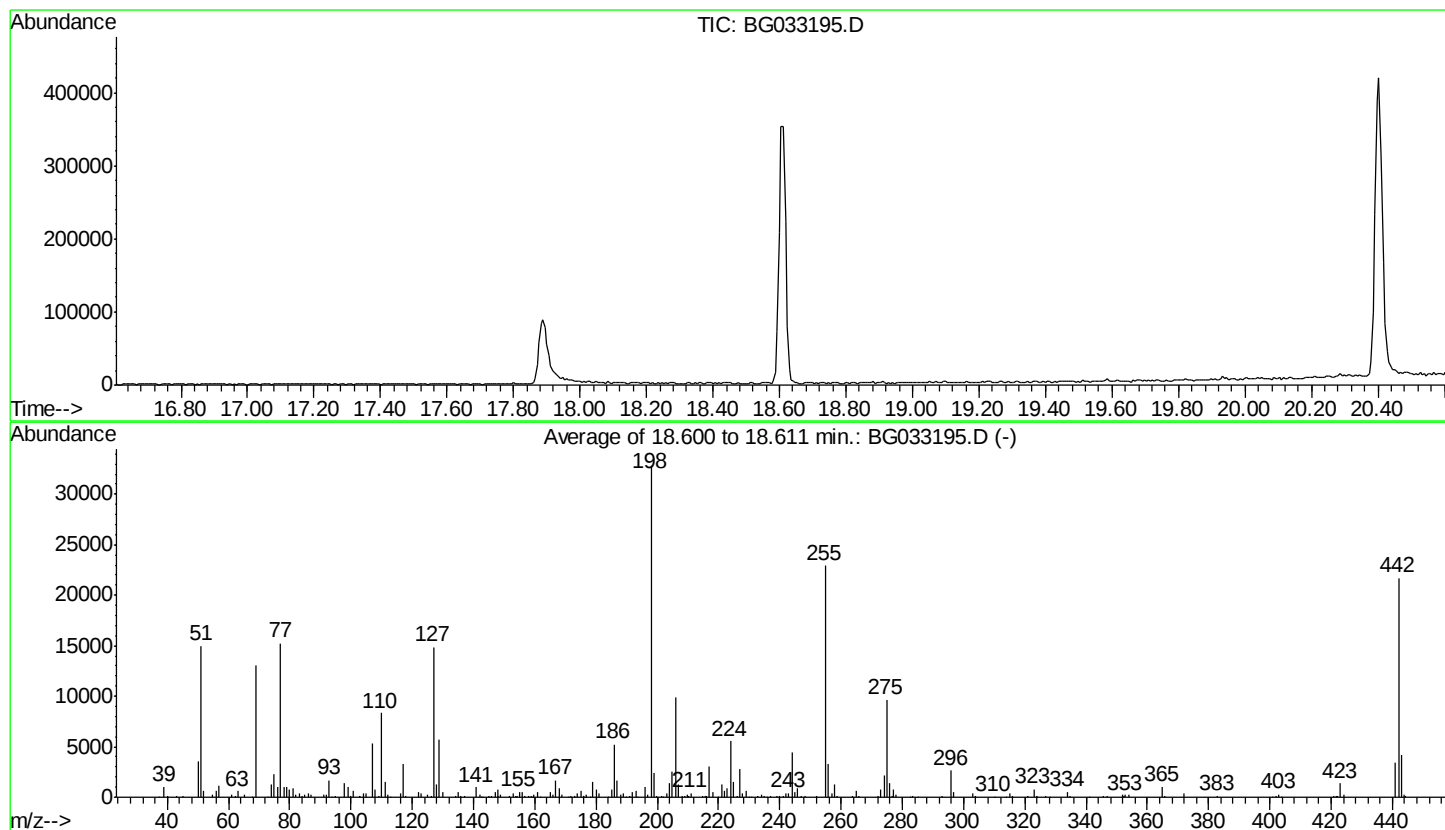

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	14976	PASS
68	69	0.00	2	0.5	61	PASS
69	198	0.00	100	39.6	13000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	14842	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32840	PASS
199	198	5	9	7.3	2382	PASS
275	198	10	60	29.5	9703	PASS
365	198	1	100	3.1	1032	PASS
441	442	0.01	24	15.8	3434	PASS
442	198	50	100	66.2	21741	PASS
443	442	15	24	19.4	4221	PASS