


Data Path : Z:\HPCHEM1\BNA G\Data\BG031618\
 Data File : BG033213.D
 Acq On : 17 Mar 2018 1:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 14 13:59:34 2018

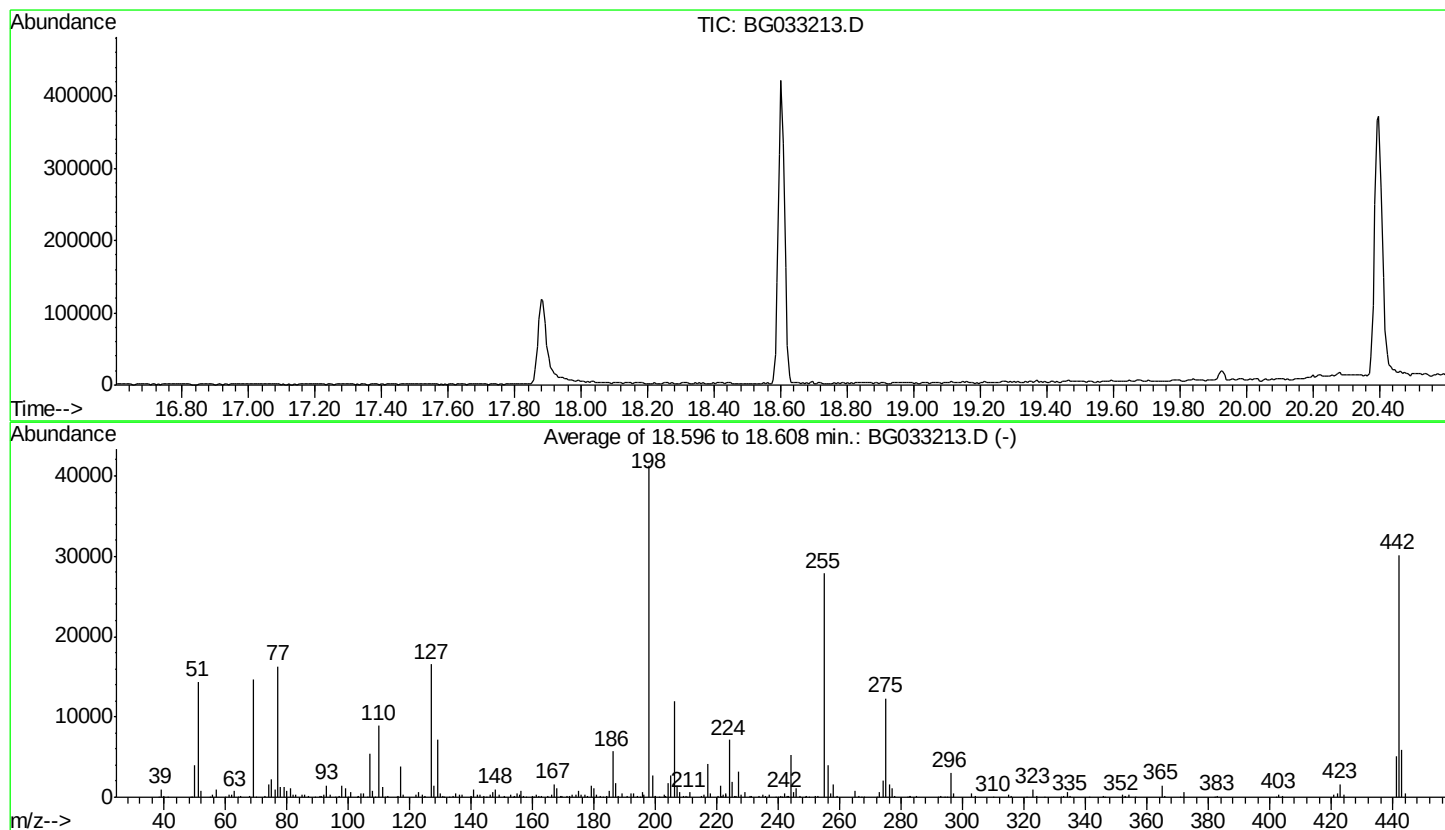

AutoFind: Scans 2605, 2606, 2607; Background Corrected with Scan 2599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	14379	PASS
68	69	0.00	2	1.2	178	PASS
69	198	0.00	100	35.7	14724	PASS
70	69	0.00	2	0.4	54	PASS
127	198	10	80	40.0	16524	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41274	PASS
199	198	5	9	6.4	2644	PASS
275	198	10	60	29.8	12281	PASS
365	198	1	100	3.6	1476	PASS
441	442	0.01	24	16.8	5074	PASS
442	198	50	100	73.1	30160	PASS
443	442	15	24	19.4	5845	PASS