
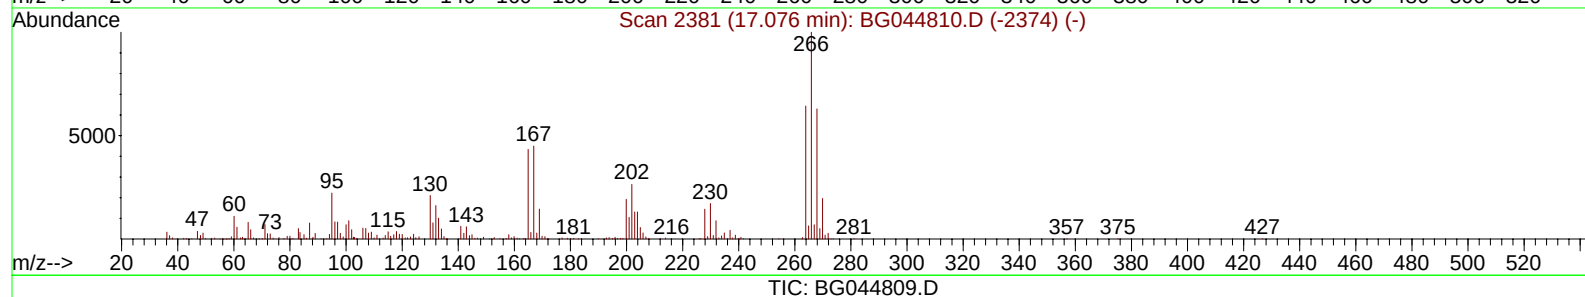
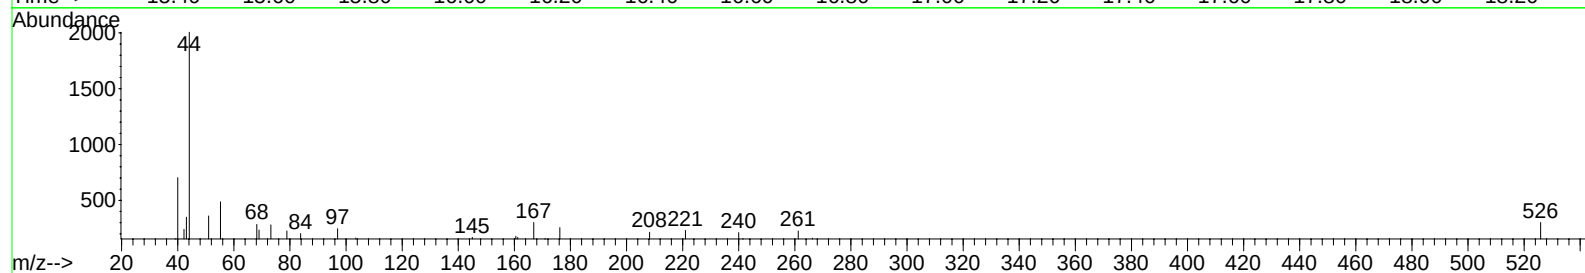


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031620\
Data File : BG044809.D
Acq On : 16 Mar 2020 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 18:27:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 17:37:15 2020
Response via : Initial Calibration

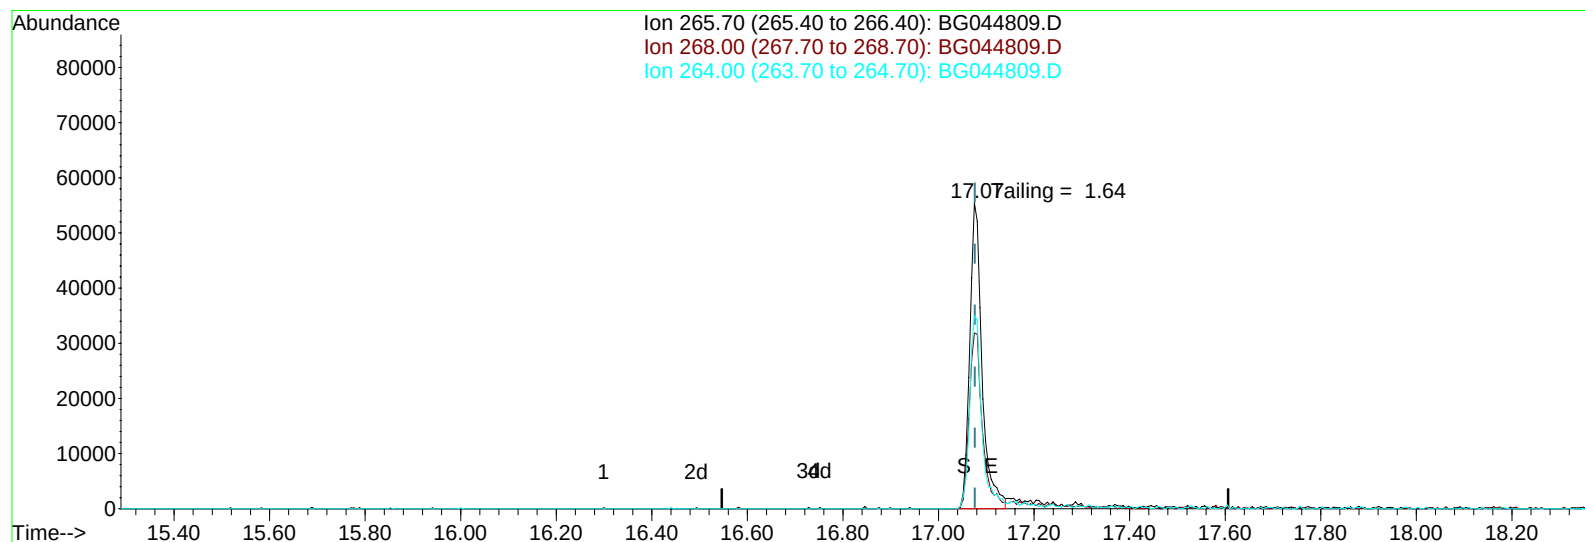

(70) Pentachlorophenol (C)




16.299min (-0.777) 134.01ng

response 57

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	0.00#
264.00	64.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031620\
 Data File : BG044809.D
 Acq On : 16 Mar 2020 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 18:27:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 17:37:15 2020
 Response via : Initial Calibration

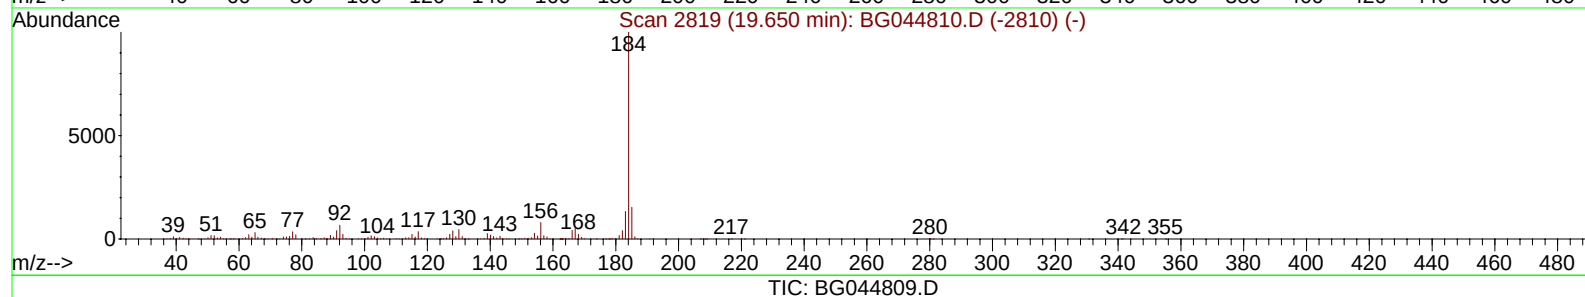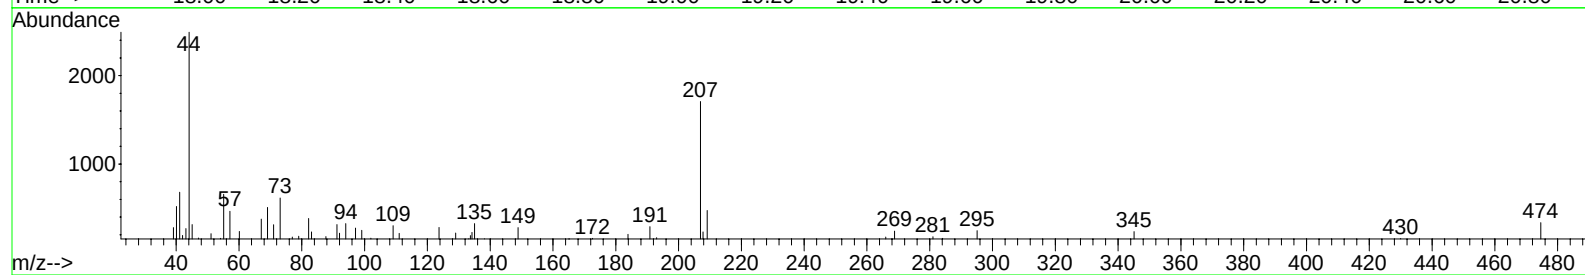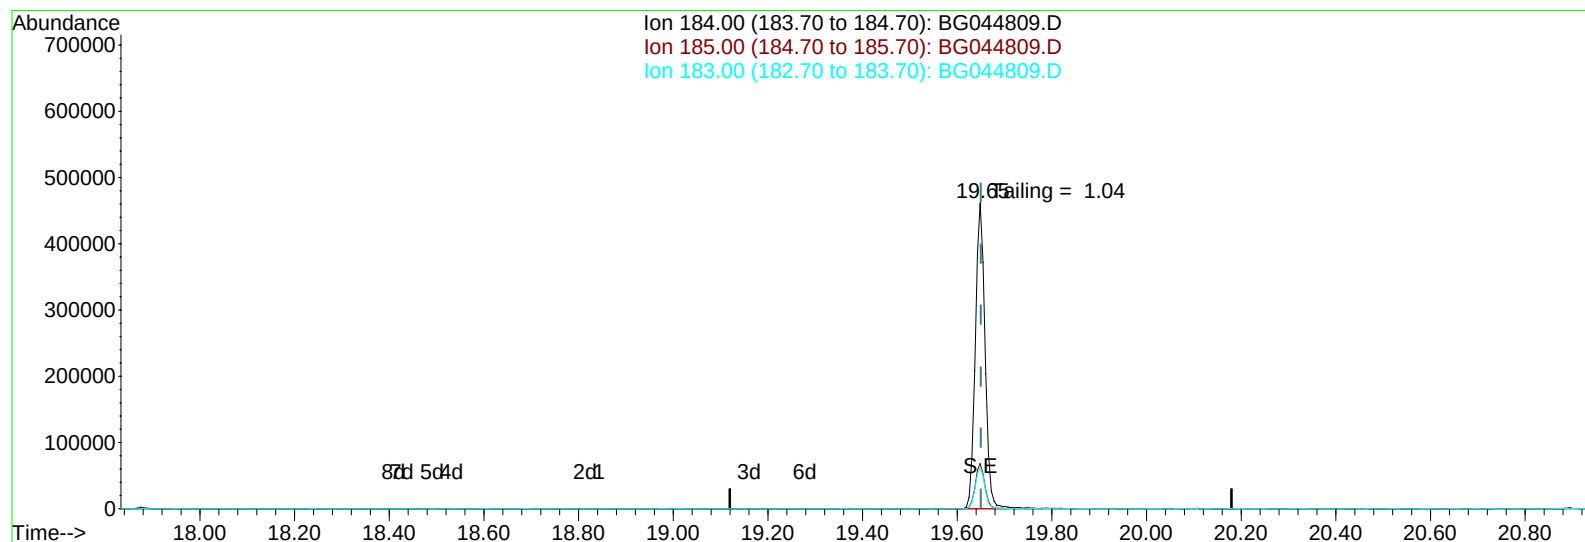

(77) Benzidine

18.844min (-0.806) 15.40ng

response 72

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00