


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031620\
 Data File : BG044809.D
 Acq On : 16 Mar 2020 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 17:37:15 2020

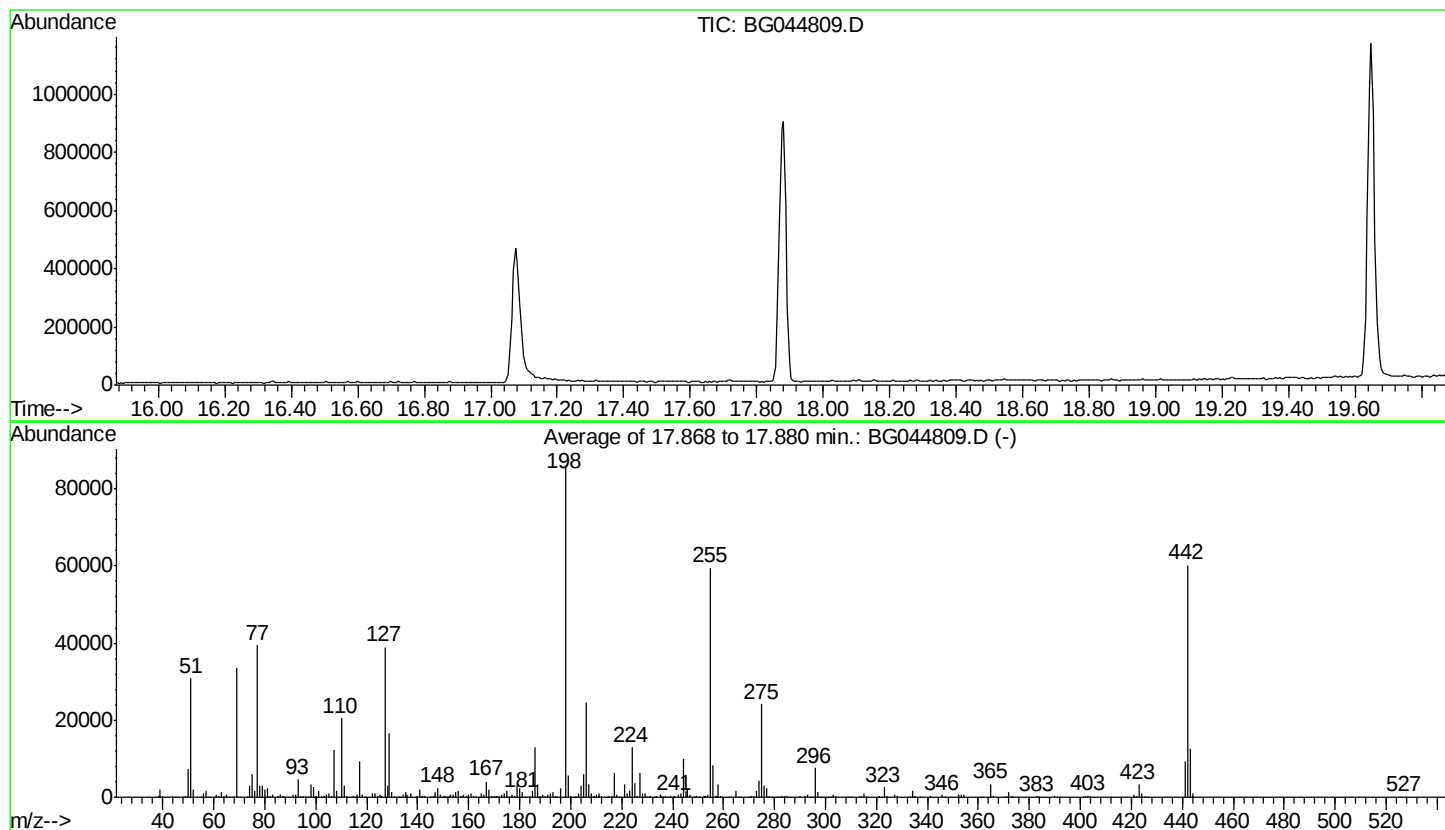

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	30850	PASS
68	69	0.00	2	1.4	471	PASS
69	198	0.00	100	38.9	33483	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	39008	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86005	PASS
199	198	5	9	6.5	5582	PASS
275	198	10	60	28.1	24154	PASS
365	198	1	100	4.0	3476	PASS
441	198	0.01	100	10.9	9410	PASS
442	198	50	100	69.9	60138	PASS
443	442	15	24	20.8	12488	PASS