


Data Path : Z:\HPCHEM1\BNA_G\Data\BG031915\
Data File : BG016065.D
Acq On : 19 Mar 2015 14:48
Operator : TP/IZ
Sample : DFTPP10
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-BG031715.M
Title : SVOA CALIBRATION
Last Update : Sat Mar 21 00:41:50 2015

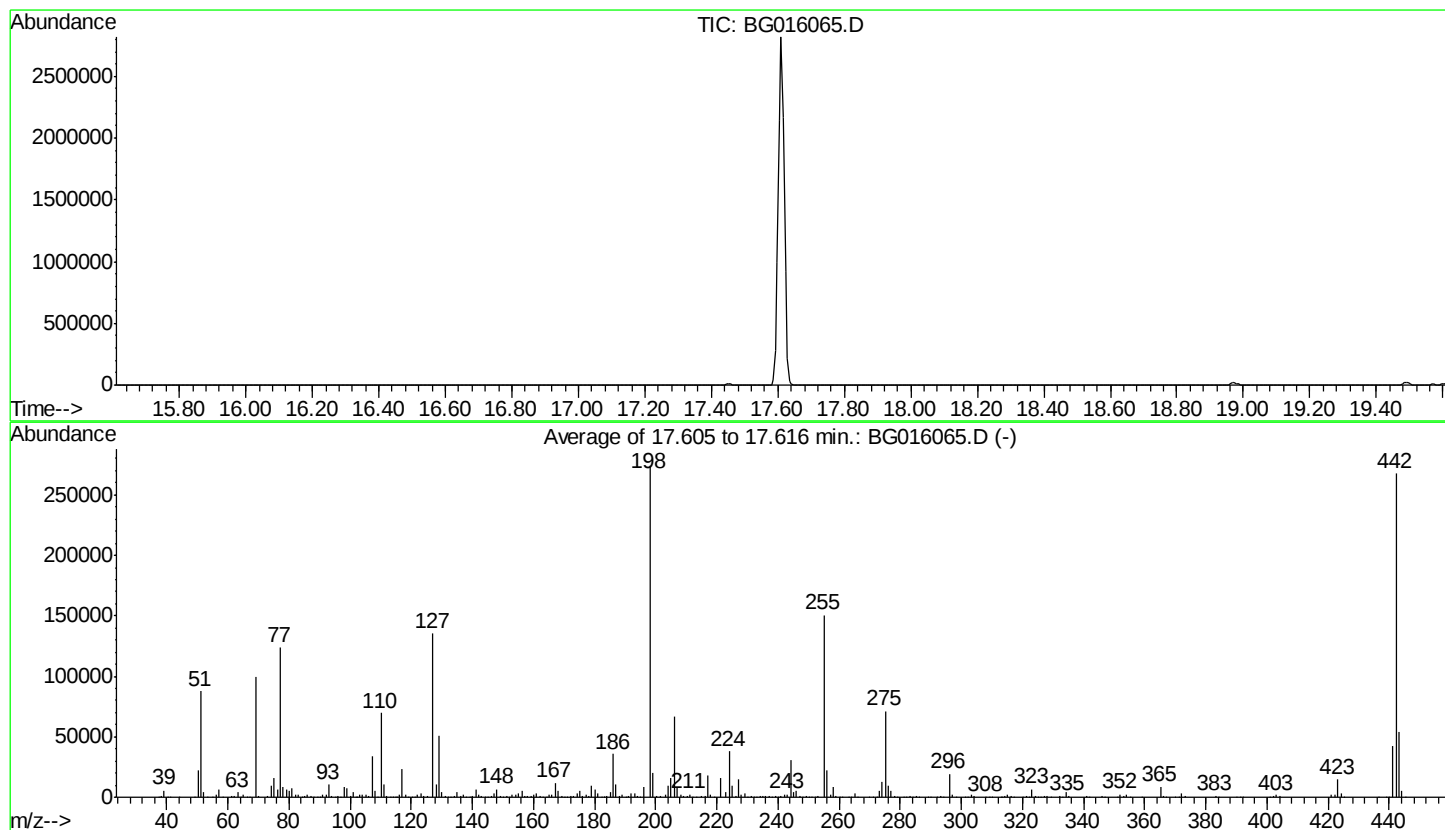

AutoFind: Scans 2539, 2540, 2541; Background Corrected with Scan 2533

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	87629	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	99400	PASS
70	69	0.00	2	0.6	585	PASS
127	198	10	80	49.4	135312	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	274176	PASS
199	198	5	9	7.2	19754	PASS
275	198	10	60	26.1	71466	PASS
365	198	1	100	3.3	8940	PASS
441	443	0.01	100	77.5	42066	PASS
442	198	50	100	97.8	268160	PASS
443	442	15	24	20.2	54264	PASS