

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031717\
 Data File : BG026303.D
 Acq On : 18 Mar 2017 5:07
 Operator : SJ/MA
 Sample : I2283-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB304

Quant Time: Mar 18 05:42:06 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 18 00:29:44 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	169217	20.00	ng/ul	0.00
2) Naphthalene-d8	10.85	136	803748	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.66	164	438432	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	865465	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	851807	20.00	ng/ul	0.00
23) Perylene-d12	24.83	264	802437	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.48	165	14021	1.18	ng/uL	0.00
7) Acenaphthylene-d8	14.35	160	541048	14.47	ng/ul	0.00
10) Fluorene-d10	15.64	176	399764	14.66	ng/ul	0.00
15) Anthracene-d10	17.49	188	533994	13.88	ng/ul	0.00
19) Pyrene-d10	19.76	212	546205	12.57	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.61	264	468549	13.54	ng/ul	0.00
Target Compounds				Qvalue		
4) Naphthalene	10.90	128	89432	2.27	ng/ul	99
5) 2-Methylnaphthalene	12.50	142	50702	1.74	ng/ul	96
9) Acenaphthene	14.72	153	117220	4.34	ng/ul	98
11) Fluorene	15.70	166	134445	4.41	ng/ul	97
14) Phenanthrene	17.44	178	1705803	37.19	ng/ul	97
16) Anthracene	17.52	178	340861	7.36	ng/ul	98
17) Fluoranthene	19.43	202	1871562	39.31	ng/ul	96
20) Pyrene	19.80	202	1663980	30.68	ng/ul	98
21) Benzo(a)anthracene	21.62	228	885118	18.67	ng/ul	98
22) Chrysene	21.68	228	868243	19.63	ng/ul	99
24) Benzo(b)fluoranthene	23.82	252	967620	21.24	ng/ul	98
25) Benzo(k)fluoranthene	23.82	252	967620	22.24	ng/ul	97
27) Benzo(a)pyrene	24.67	252	629011	14.86	ng/ul	96
28) Indeno(1,2,3-cd)pyrene	28.45	276	331003	7.08	ng/ul	95
29) Dibenzo(a,h)anthracene	28.48	278	44382	1.20	ng/ul	93
30) Benzo(g,h,i)perylene	29.59	276	224947	5.62	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031717\
Data File : BG026303.D
Acq On : 18 Mar 2017 5:07
Operator : SJ/MA
Sample : I2283-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB304

Quant Time: Mar 18 05:42:06 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 18 00:29:44 2017
Response via : Initial Calibration

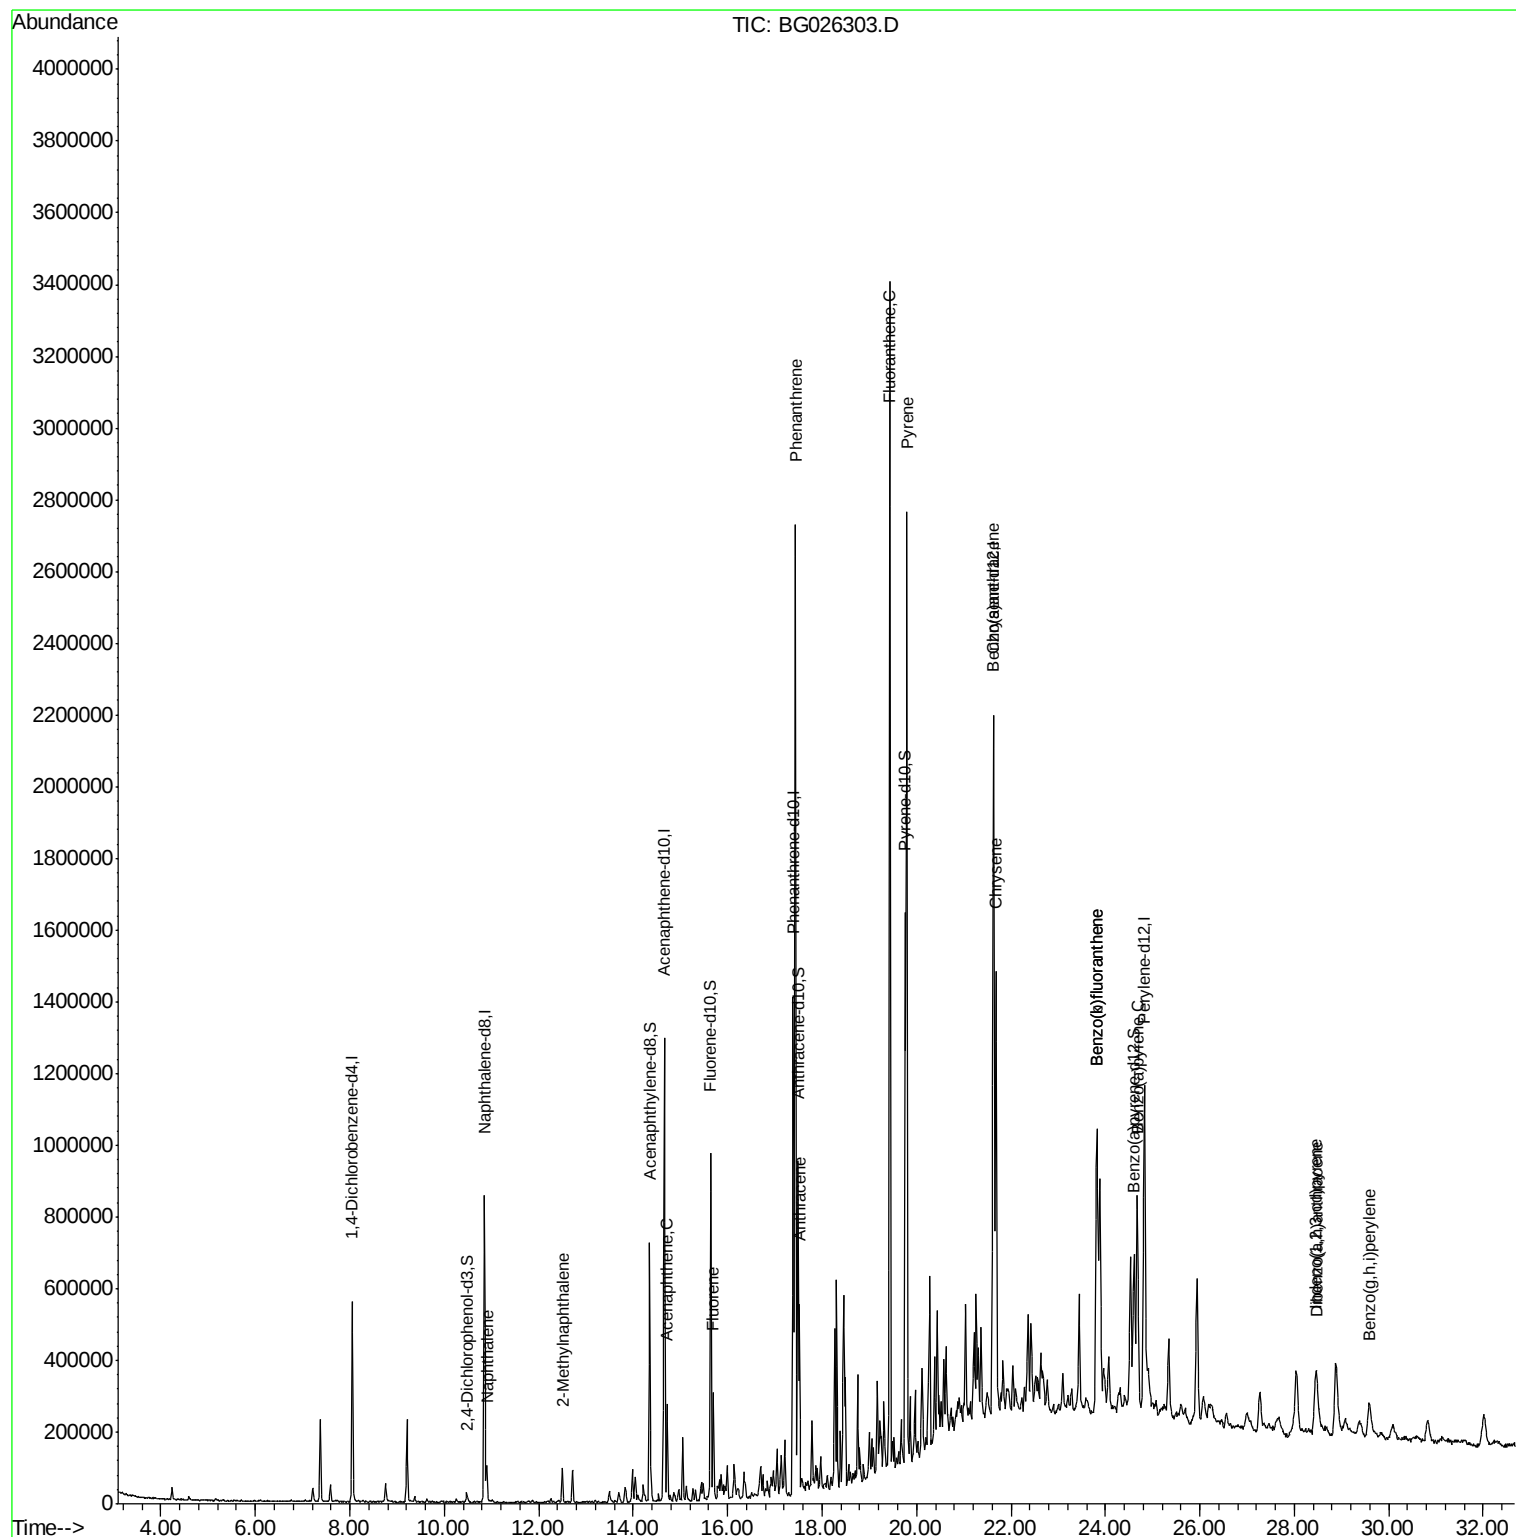

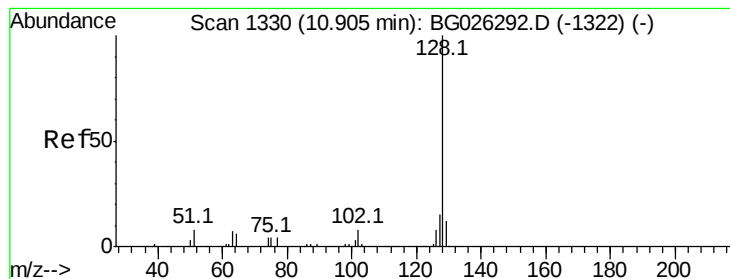

#4

Naphthalene

Concen: 2.27 ng/ul

RT: 10.90 min Scan# 1330

Delta R.T. -0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :

BNA_G

ClientSampleId :

CB304


Tot Ion:128 Resp: 89432

Ion Ratio Lower Upper

128 100

129 11.1 9.1 13.7




127 13.8 10.6 15.8

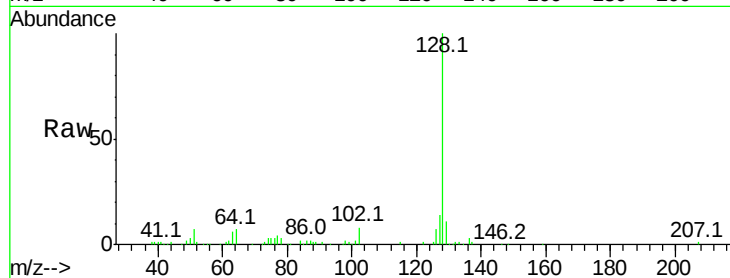

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

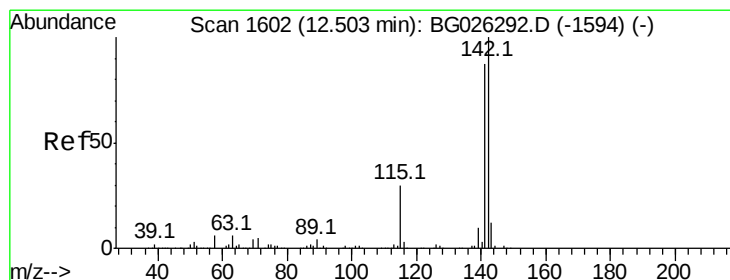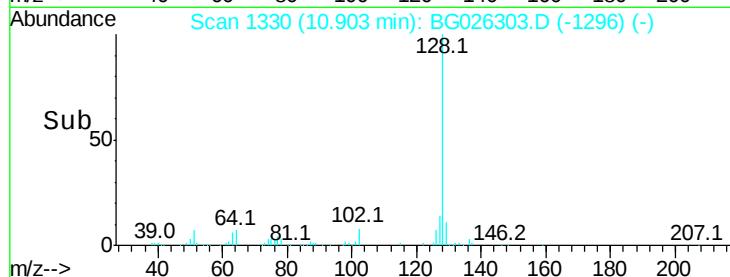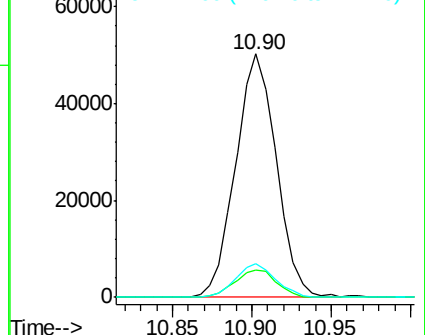

#5

2-Methylnaphthalene

Concen: 1.74 ng/ul

RT: 12.50 min Scan# 1602

Delta R.T. -0.00 min

Lab File: BG026303.D


Acq: 18 Mar 2017 5:07

Tgt Ion:142 Resp: 50702

Ion Ratio Lower Upper



142 100


141 90.6 69.8 104.8

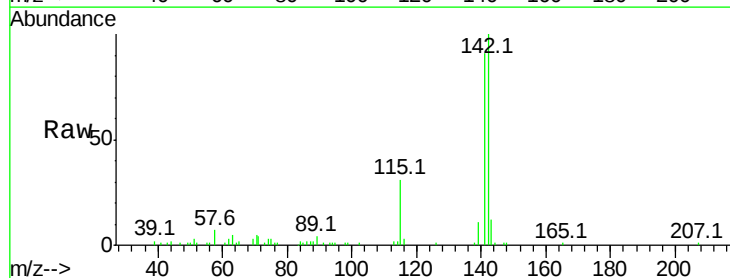

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

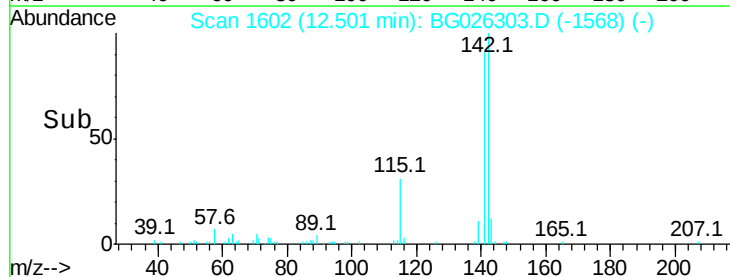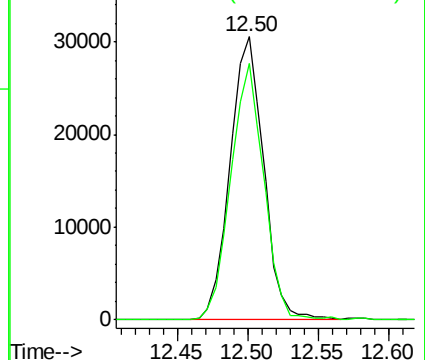

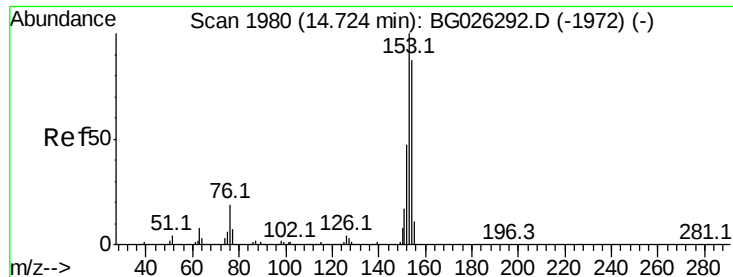

#9

Acenaphthene

Concen: 4.34 ng/ul

RT: 14.72 min Scan# 1980

Delta R.T. -0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :

BNA_G

ClientSampled :

CB304


Tot Ion:153 Resp: 117220

Ion Ratio Lower Upper

153 100

152 49.1 37.9 56.9




154 88.1 71.6 107.4

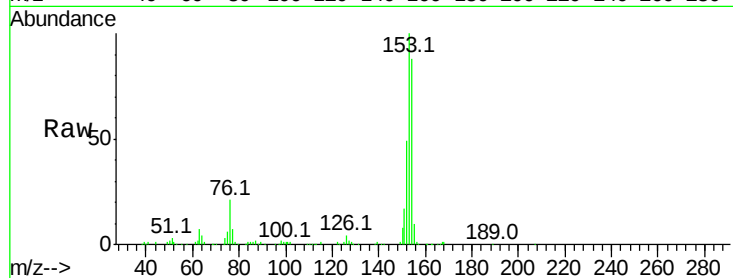

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

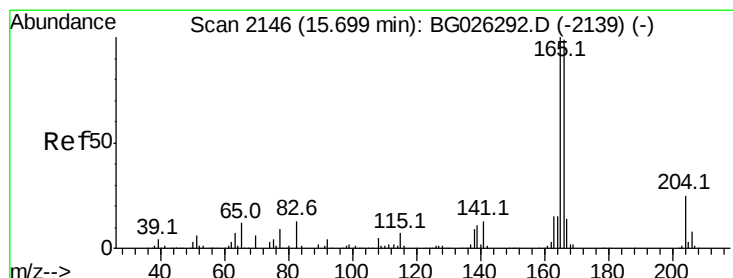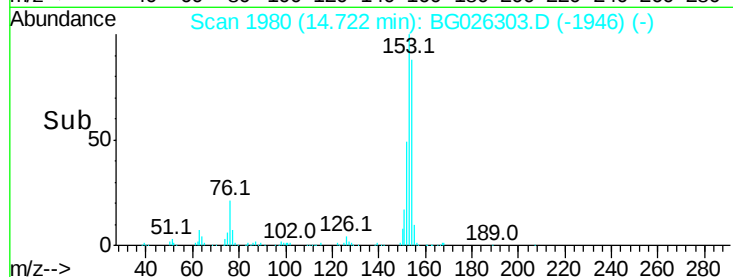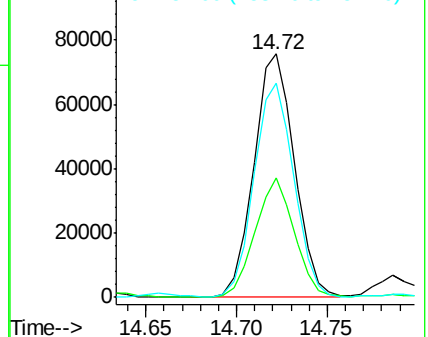

#11

Fluorene

Concen: 4.41 ng/ul

RT: 15.70 min Scan# 2146

Delta R.T. -0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07


Tgt Ion:166 Resp: 134445

Ion Ratio Lower Upper

166 100

165 96.2 80.0 120.0



167 14.3 11.6 17.4

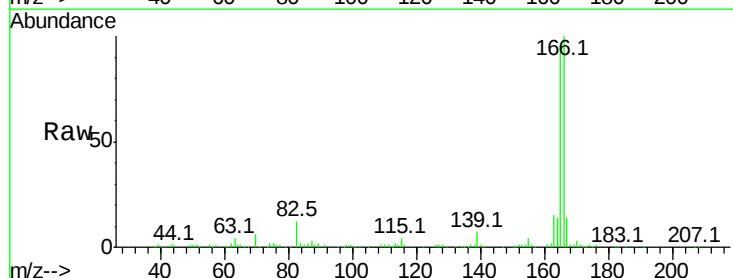


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

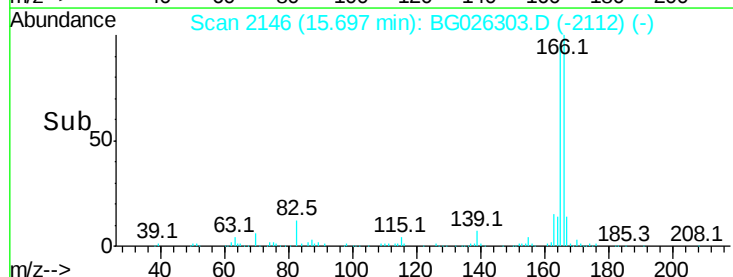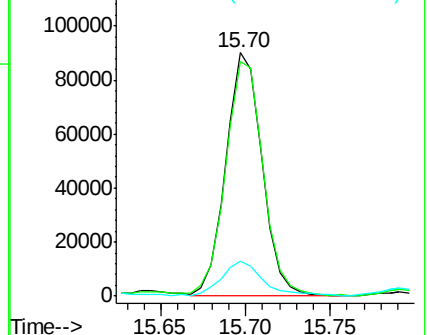

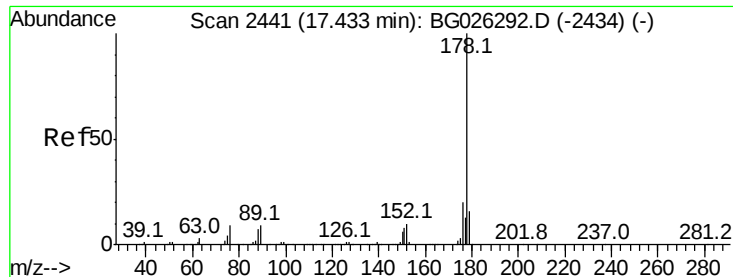

#14

Phenanthrene

Concen: 37.19 ng/ul

RT: 17.44 min Scan# 2442

Delta R.T. 0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :


BNA_G

ClientSampled :

CB304

Tot Ion:178 Resp: 1705803



Ion	Ratio	Lower	Upper
178	100		
179	17.2	12.2	18.4
176	21.4	16.4	24.6

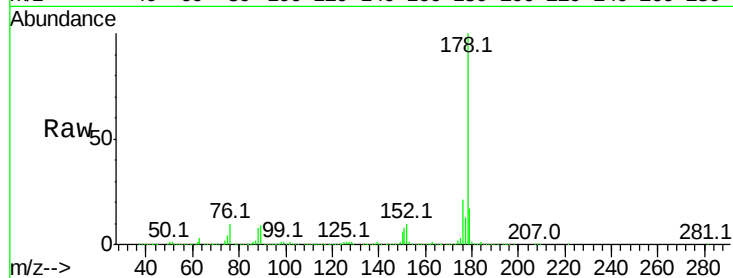


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

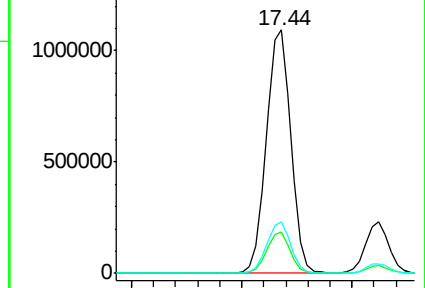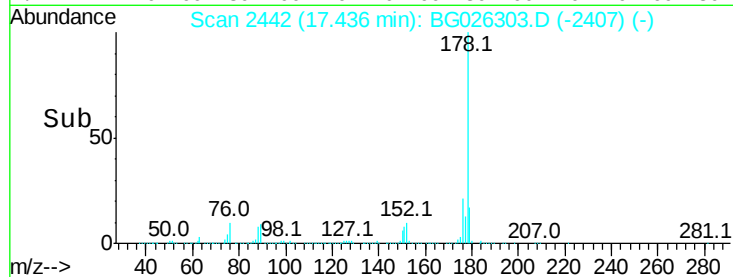

Time-->

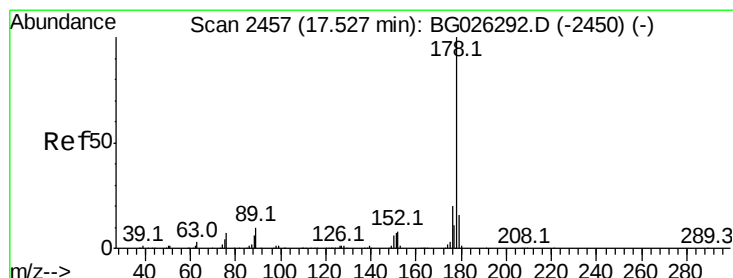

#16

Anthracene

Concen: 7.36 ng/ul

RT: 17.52 min Scan# 2457


Delta R.T. -0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Tgt Ion:178 Resp: 340861



Ion	Ratio	Lower	Upper
178	100		
179	15.9	12.7	19.1
176	18.5	15.8	23.8

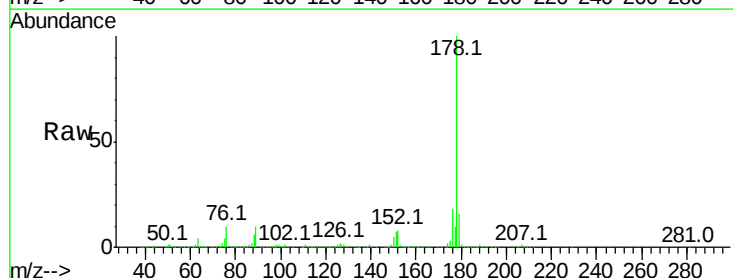


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

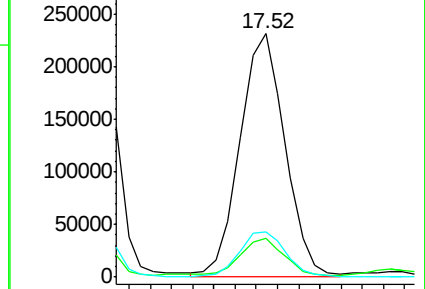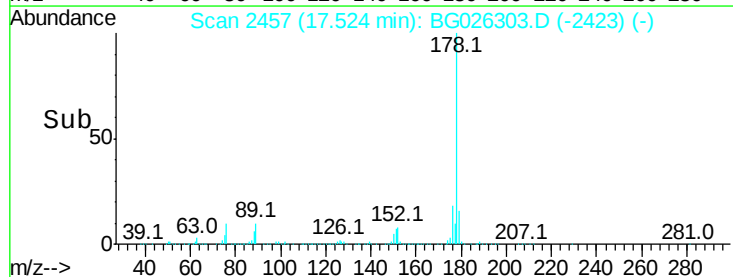

Time-->




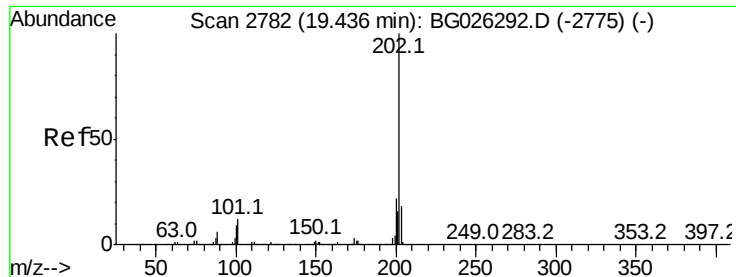


#17
Fluoranthene
 Concen: 39.31 ng/ul
 RT: 19.43 min Scan# 2782
 Delta R.T. -0.00 min
 Lab File: BG026303.D
 Acq: 18 Mar 2017 5:07

Instrument :
 BNA_G
 ClientSampleId :
 CB304

Tot Ion:202 Resp: 1871562




Ion	Ratio	Lower	Upper
202	100		
101	13.9	9.8	14.8
100	11.0	7.5	11.3

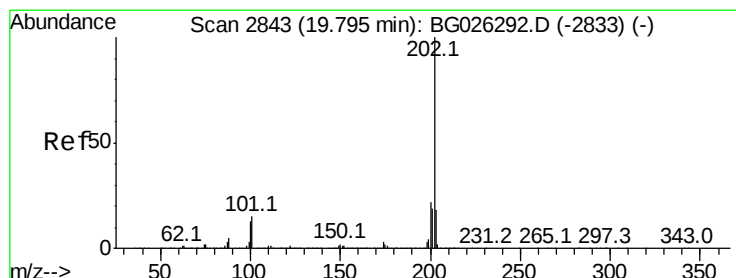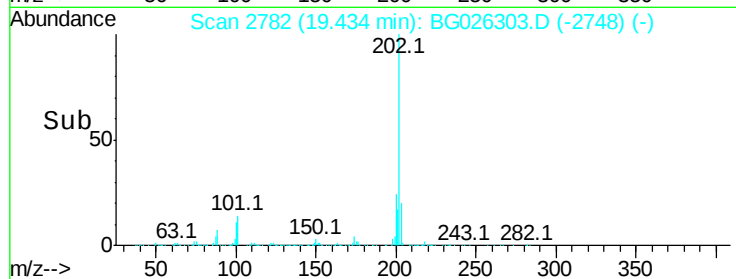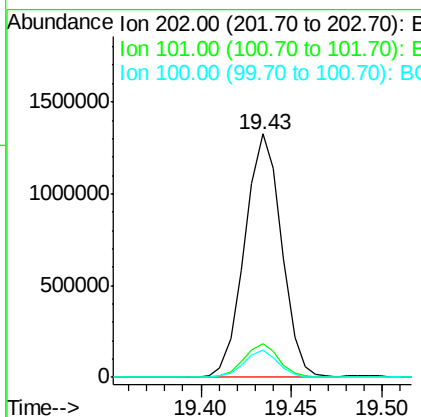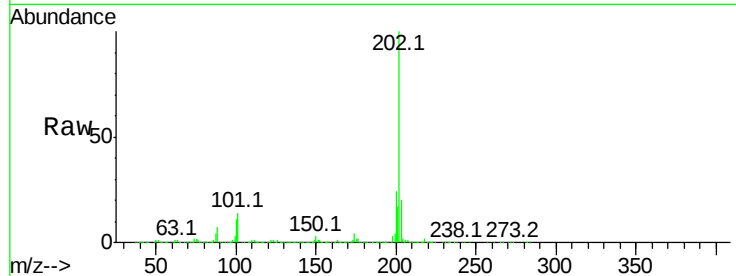


#20
Pyrene
 Concen: 30.68 ng/ul
 RT: 19.80 min Scan# 2844
 Delta R.T. 0.00 min
 Lab File: BG026303.D
 Acq: 18 Mar 2017 5:07

Tgt Ion:202 Resp: 1663980

Ion	Ratio	Lower	Upper
202	100		
101	15.2	11.2	16.8
100	13.0	9.8	14.6

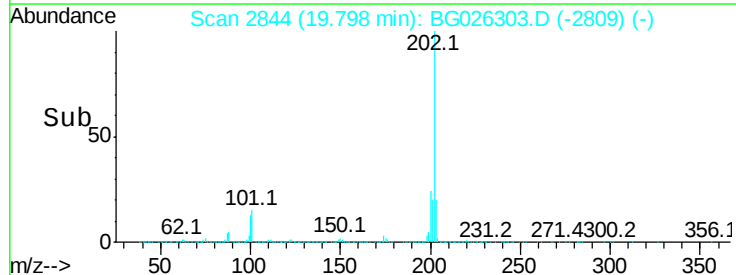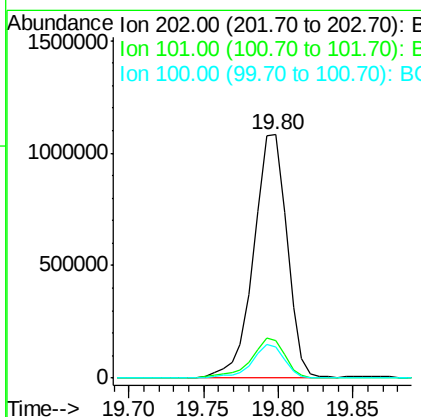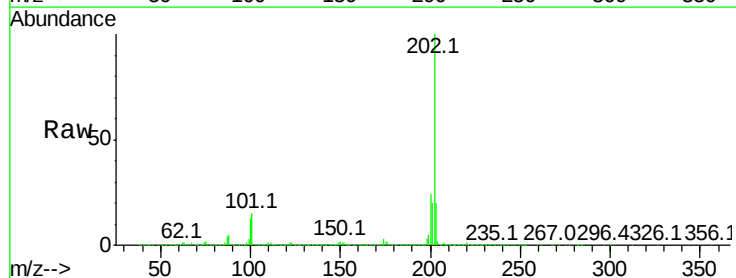

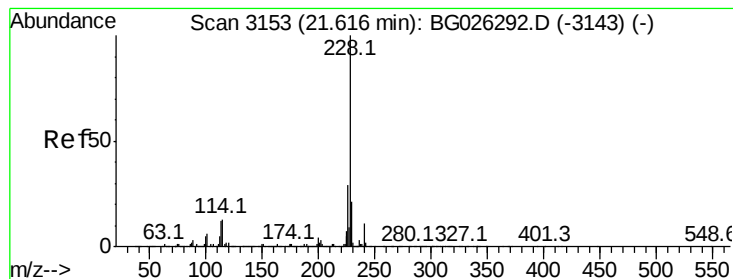

#21

Benzo(a)anthracene

Concen: 18.67 ng/ul

RT: 21.62 min Scan# 3154

Delta R.T. 0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :

BNA_G

ClientSampleId :

CB304


Tot Ion:228 Resp: 885118

Ion Ratio Lower Upper




228 100

229 21.1 15.9 23.9

226 28.6 22.1 33.1

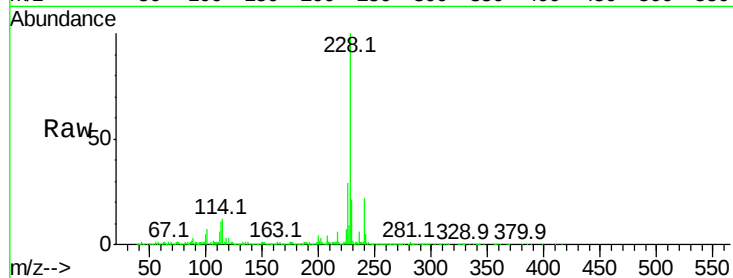

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

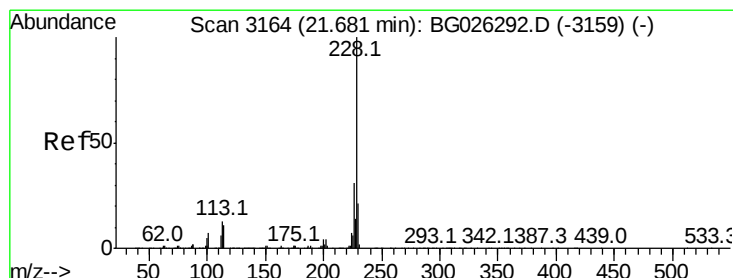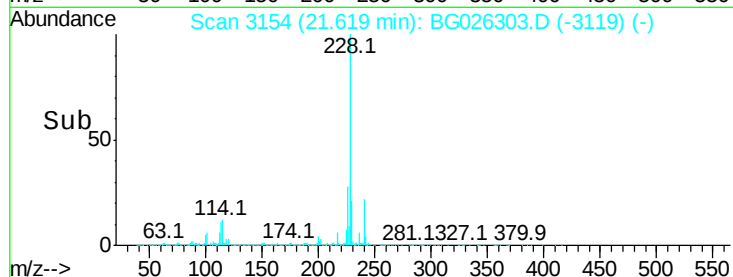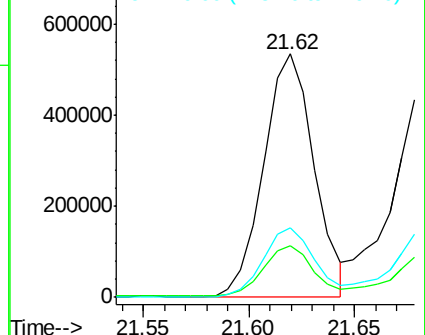

#22

Chrysene

Concen: 19.63 ng/ul

RT: 21.68 min Scan# 3165

Delta R.T. 0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07


Tgt Ion:228 Resp: 868243

Ion Ratio Lower Upper



228 100


226 31.6 25.0 37.6

229 20.6 16.6 25.0

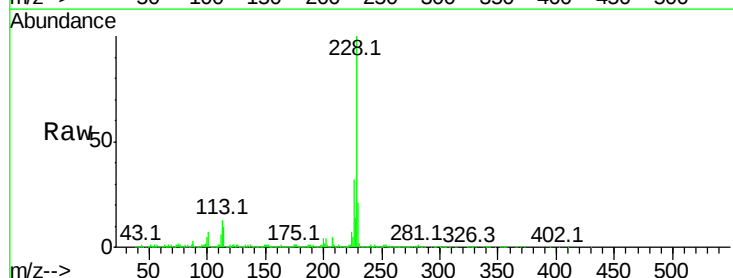

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

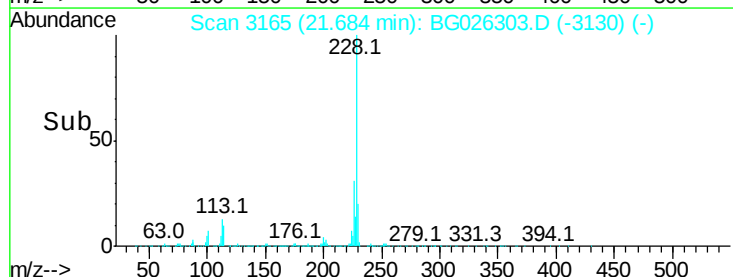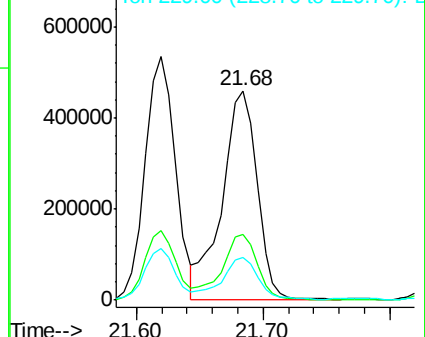

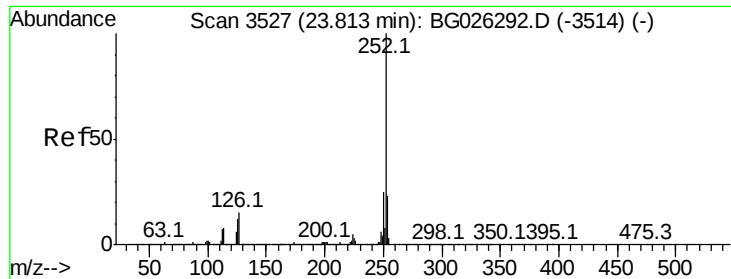

#24

Benzo(b)fluoranthene

Concen: 21.24 ng/ul

RT: 23.82 min Scan# 3528

Delta R.T. 0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :

BNA_G

ClientSampleId :

CB304


Tot Ion:252 Resp: 967620

Ion Ratio Lower Upper

252 100

253 23.7 17.8 26.6




125 11.9 9.4 14.0

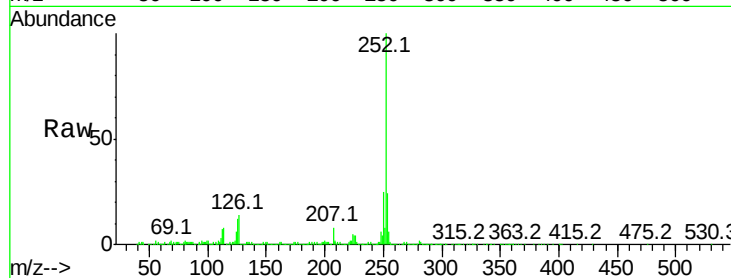

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

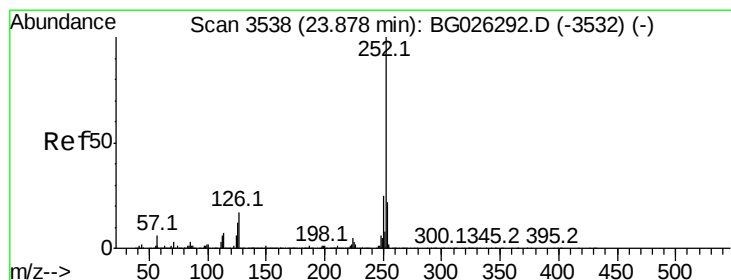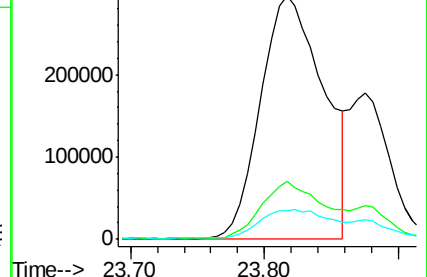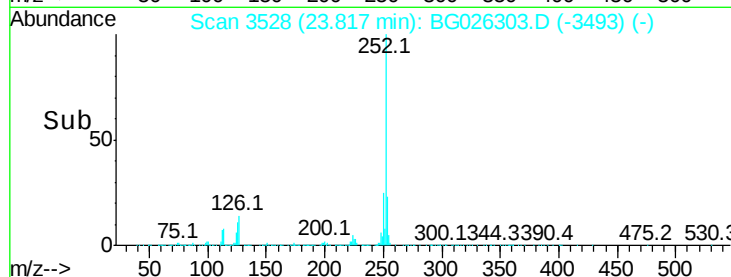

#25

Benzo(k)fluoranthene

Concen: 22.24 ng/ul

RT: 23.82 min Scan# 3528

Delta R.T. -0.06 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07


Tgt Ion:252 Resp: 967620

Ion Ratio Lower Upper

252 100

253 23.7 17.4 26.2



125 11.9 8.8 13.2

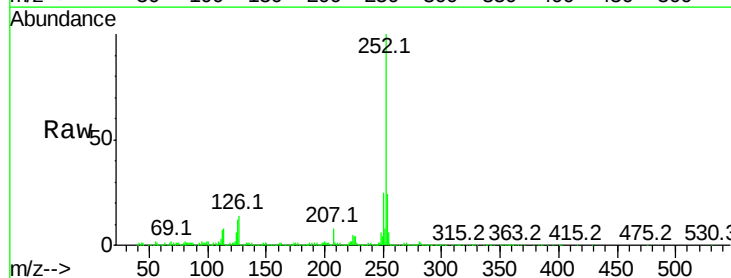


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

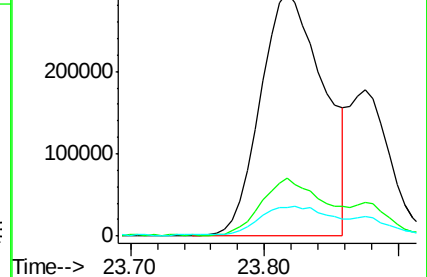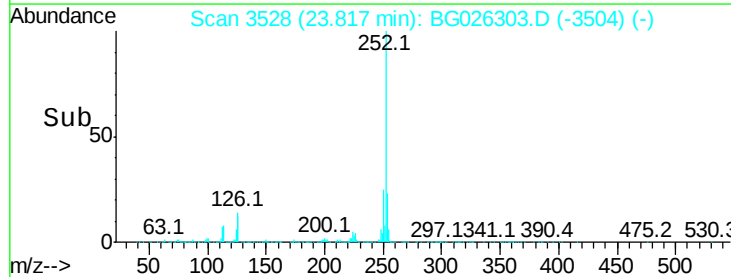

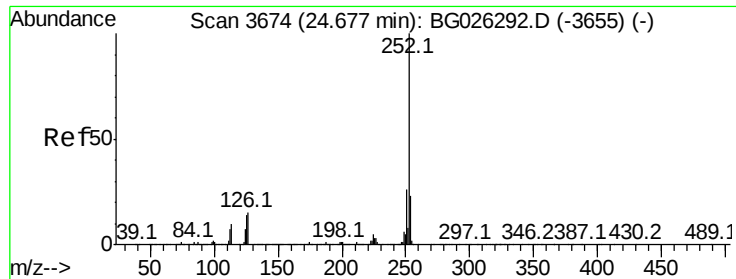

#27

Benzo(a)pyrene

Concen: 14.86 ng/ul

RT: 24.67 min Scan# 3674

Delta R.T. -0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :

BNA_G

ClientSampleId :

CB304


Tot Ion:252 Resp: 629011

Ion Ratio Lower Upper




252 100

253 23.1 17.1 25.7

125 13.6 9.4 14.2

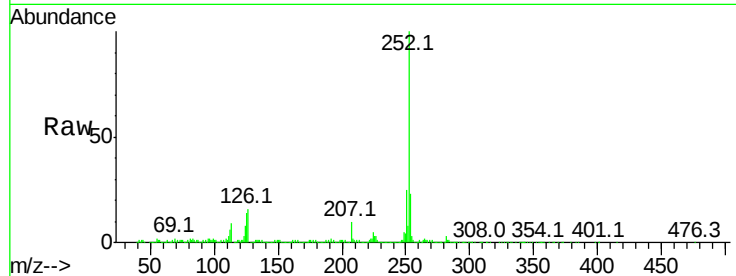

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

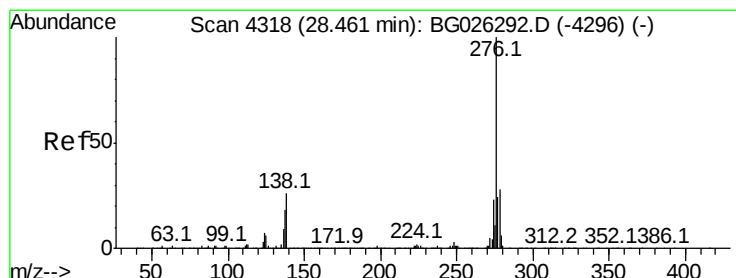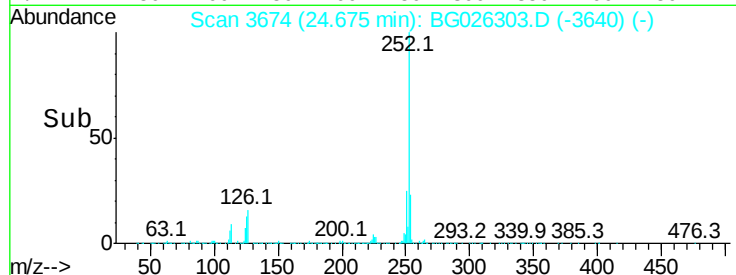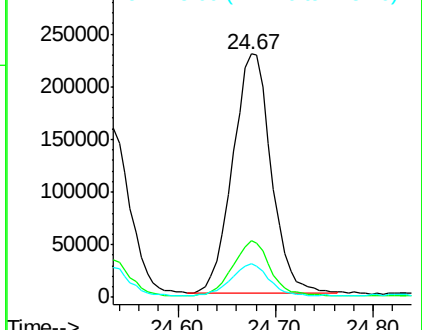

#28

Indeno(1,2,3-cd)pyrene

Concen: 7.08 ng/ul

RT: 28.45 min Scan# 4317

Delta R.T. -0.01 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07


Tgt Ion:276 Resp: 331003

Ion Ratio Lower Upper



276 100


138 25.7 17.8 26.6

277 25.9 19.4 29.0

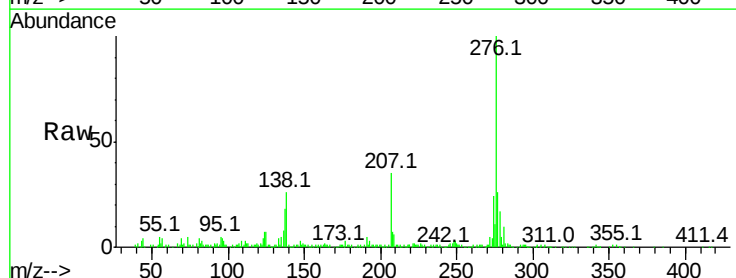

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

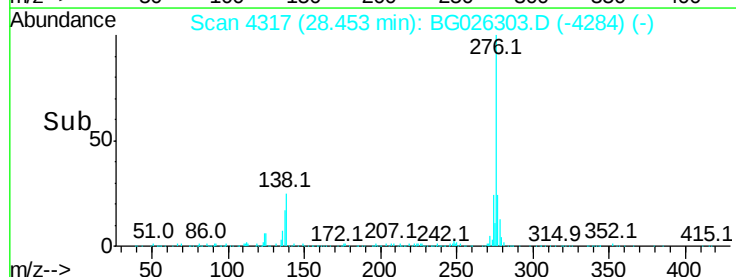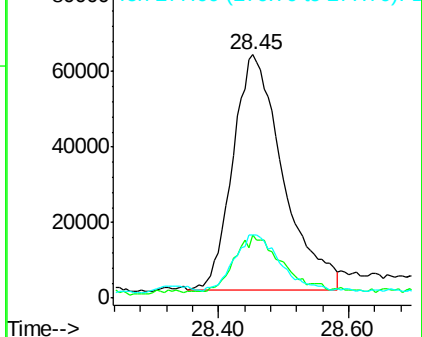

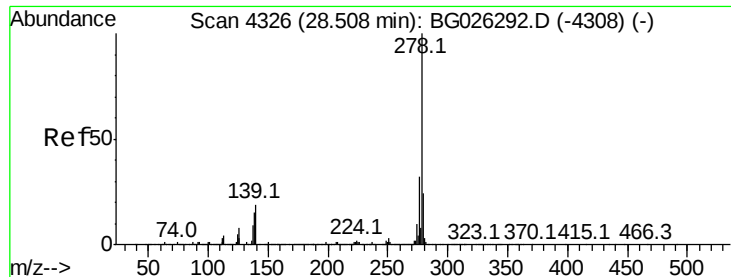

#29

Dibenzo(a,h)anthracene

Concen: 1.20 ng/ul

RT: 28.48 min Scan# 4322

Delta R.T. -0.03 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07

Instrument :

BNA_G

ClientSampleId :

CB304


Tot Ion:278 Resp: 44382

Ion Ratio Lower Upper

278 100

139 20.7 14.0 21.0




279 22.1 20.6 31.0

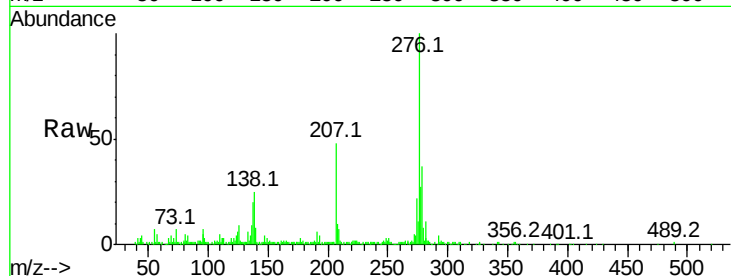

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

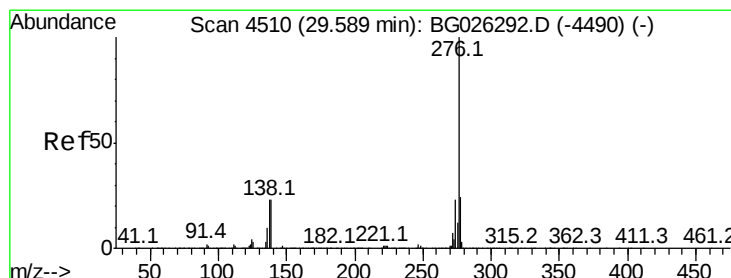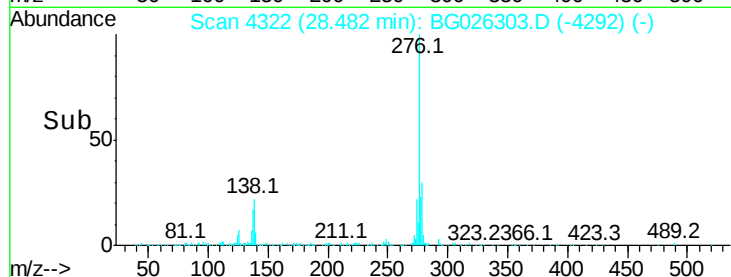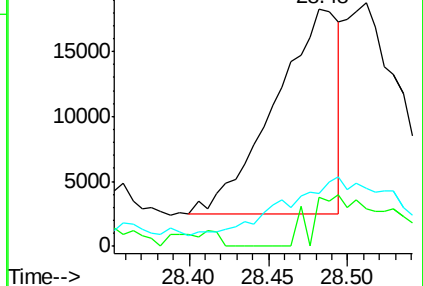

#30

Benzo(g,h,i)perylene

Concen: 5.62 ng/ul

RT: 29.59 min Scan# 4510

Delta R.T. -0.00 min

Lab File: BG026303.D

Acq: 18 Mar 2017 5:07


Tgt Ion:276 Resp: 224947

Ion Ratio Lower Upper

276 100

138 23.7 19.0 28.4

277 24.6 19.7 29.5

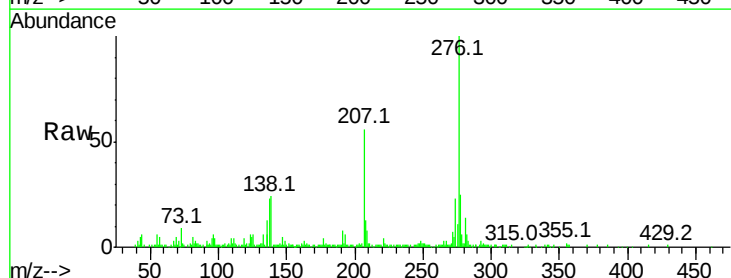

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

