

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031717\
 Data File : BG026284.D
 Acq On : 17 Mar 2017 16:01
 Operator : SJ/MA
 Sample : I2218-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB2Y3

Quant Time: Mar 17 16:53:58 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 17 14:43:33 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	118171	20.00	ng/ul	0.00
2) Naphthalene-d8	10.85	136	550822	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.66	164	298419	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	596040	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	574450	20.00	ng/ul	0.00
23) Perylene-d12	24.83	264	534351	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.48	165	18013	2.21	ng/uL	0.00
7) Acenaphthylene-d8	14.35	160	504336	19.82	ng/ul	0.00
10) Fluorene-d10	15.64	176	353589	19.05	ng/ul	0.00
15) Anthracene-d10	17.49	188	501555	18.93	ng/ul	0.00
19) Pyrene-d10	19.76	212	522453	17.82	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.61	264	439551	19.07	ng/ul	0.00
Target Compounds						
17) Fluoranthene	19.43	202	38417	1.17	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031717\
Data File : BG026284.D
Acq On : 17 Mar 2017 16:01
Operator : SJ/MA
Sample : I2218-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB2Y3

Quant Time: Mar 17 16:53:58 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 14:43:33 2017
Response via : Initial Calibration

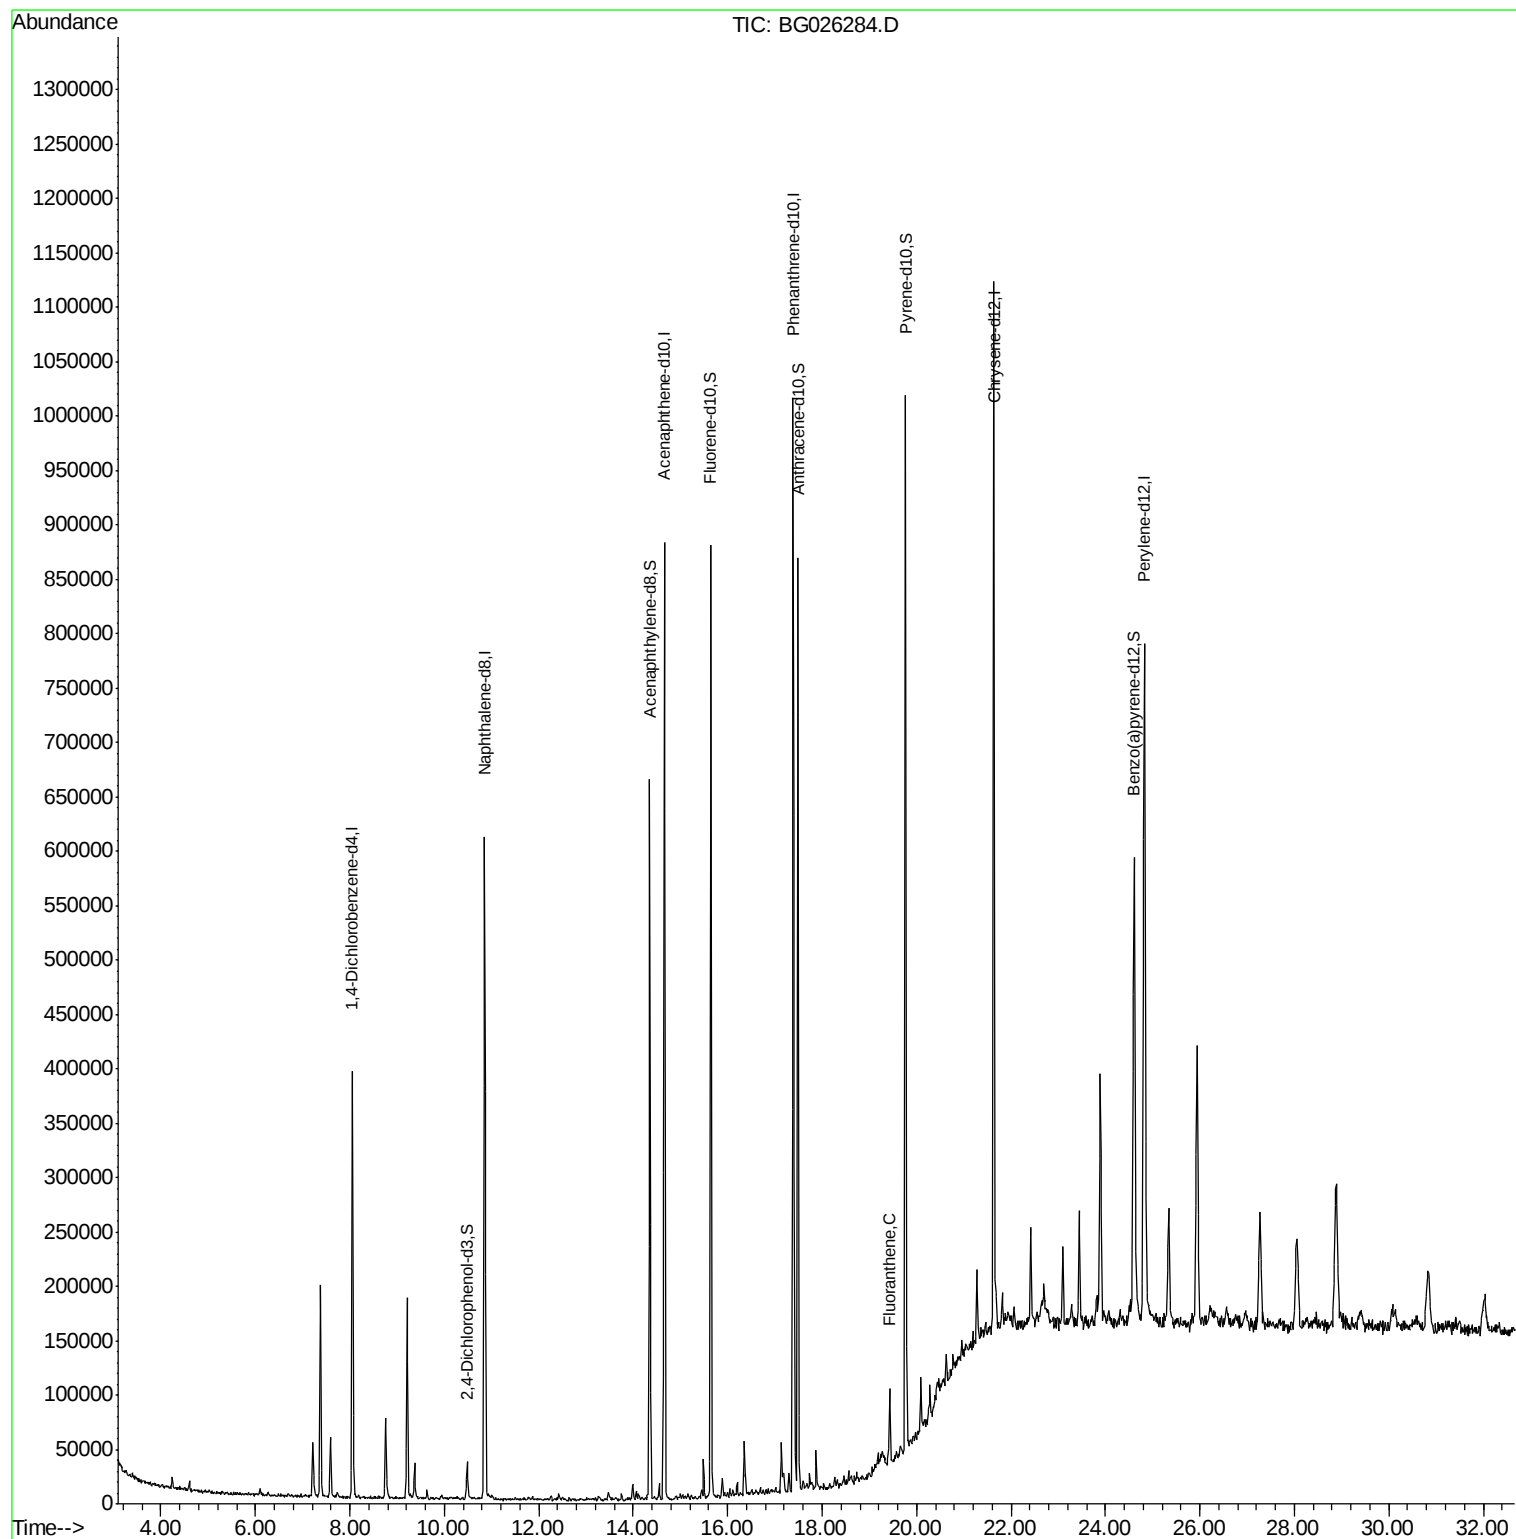


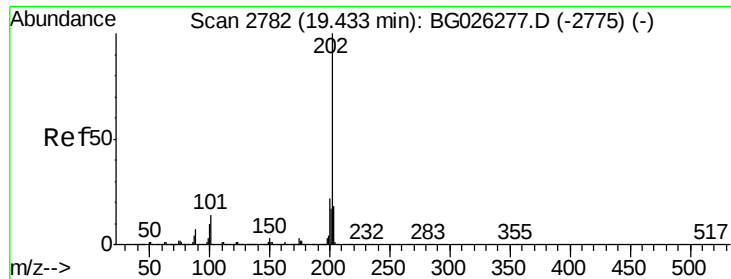

#17
 Fluoranthene
 Concen: 1.17 ng/ul
 RT: 19.43 min Scan# 2782
 Delta R.T. -0.00 min
 Lab File: BG026284.D
 Acq: 17 Mar 2017 16:01

Instrument :
 BNA_G
 ClientSampleId :
 CB2Y3

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.6	9.8	14.8#
100	10.3	7.5	11.3

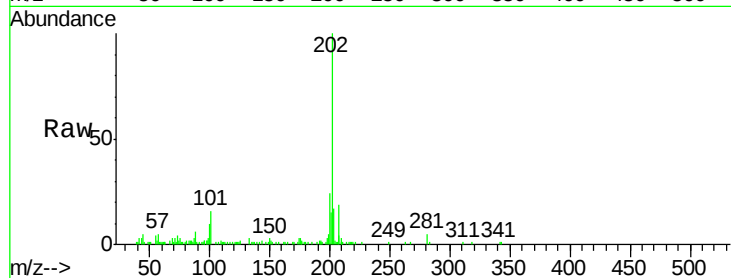

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

