

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031717\
 Data File : BG026293.D
 Acq On : 17 Mar 2017 22:34
 Operator : SJ/MA
 Sample : I2218-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB2Z5

Manual Integrations
 APPROVED

mohammad
 3/20/2017 12:54:59 PM

Quant Time: Mar 18 00:34:31 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 18 00:29:44 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	129874	20.00	ng/ul	0.00
2) Naphthalene-d8	10.86	136	617179	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.66	164	336208	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	665818	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	648314	20.00	ng/ul	0.00
23) Perylene-d12	24.82	264	604835	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.47	165	111211	12.17	ng/uL	0.00
7) Acenaphthylene-d8	14.35	160	731827	25.53	ng/ul	0.00
10) Fluorene-d10	15.64	176	505200	24.16	ng/ul	0.00
15) Anthracene-d10	17.49	188	687877	23.25	ng/ul	0.00
19) Pyrene-d10	19.76	212	764985	23.12	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.60	264	695438	26.66	ng/ul	0.00
Target Compounds						
4) Naphthalene	10.90	128	45141	1.50	ng/ul	Qvalue 97
5) 2-Methylnaphthalene	12.50	142	26522	1.18	ng/ul	100
9) Acenaphthene	14.72	153	39957	1.93	ng/ul	99
11) Fluorene	15.70	166	43908	1.88	ng/ul	98
14) Phenanthrene	17.43	178	662002	18.76	ng/ul	98
16) Anthracene	17.52	178	132401	3.71	ng/ul	98
17) Fluoranthene	19.43	202	958301	26.16	ng/ul	98
20) Pyrene	19.79	202	826884	20.03	ng/ul	97
21) Benzo(a)anthracene	21.61	228	451774	12.52	ng/ul	98
22) Chrysene	21.68	228	443021	13.16	ng/ul	99
24) Benzo(b)fluoranthene	23.81	252	564284	16.43	ng/ul	98
25) Benzo(k)fluoranthene	23.87	252	193753m	5.91	ng/ul	
27) Benzo(a)pyrene	24.67	252	333152	10.44	ng/ul#	95
28) Indeno(1,2,3-cd)pyrene	28.45	276	191466	5.43	ng/ul#	95
29) Dibenzo(a,h)anthracene	28.49	278	59658m	2.13	ng/ul	
30) Benzo(g,h,i)perylene	29.58	276	154159m	5.11	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031717\
Data File : BG026293.D
Acq On : 17 Mar 2017 22:34
Operator : SJ/MA
Sample : I2218-11
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
CB2Z5

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

Quant Time: Mar 18 00:34:31 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 18 00:29:44 2017
Response via : Initial Calibration

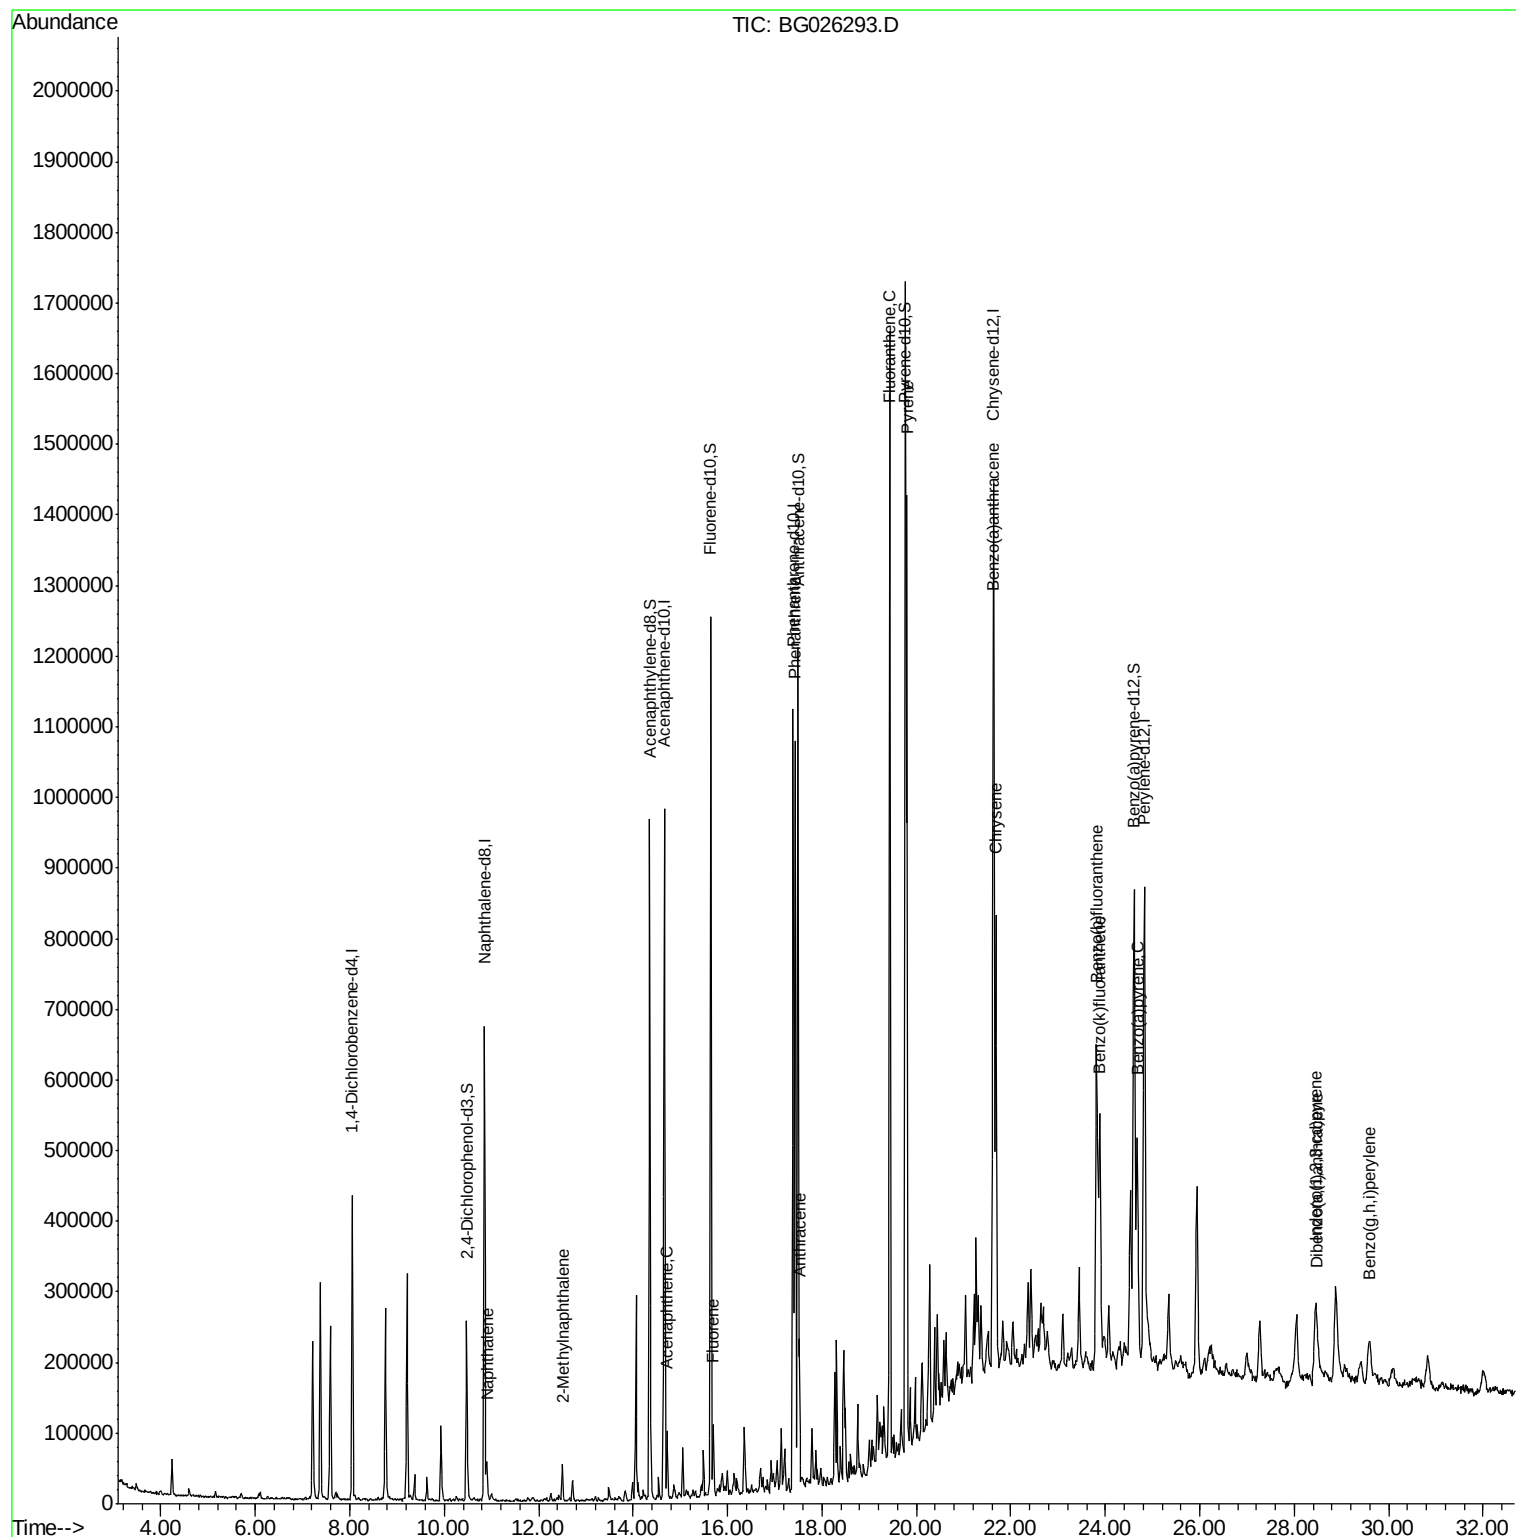

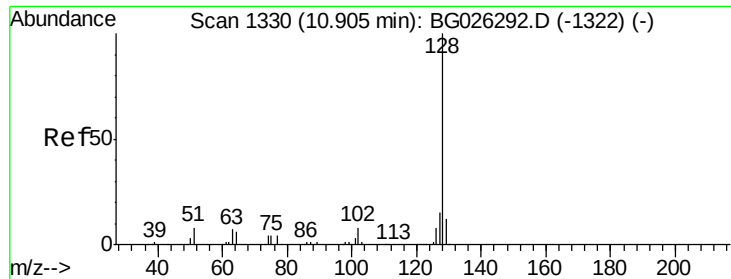

#4

Naphthalene

Concen: 1.50 ng/ul

RT: 10.90 min Scan# 1330

Delta R.T. -0.00 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Instrument :

BNA_G





ClientSampleId :

CB2Z5

Tgt Ion:	128	Resp:	45141
Ion Ratio	Lower	Upper	
128	100		
129	10.4	9.1	13.7
127	14.4	10.6	15.8

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

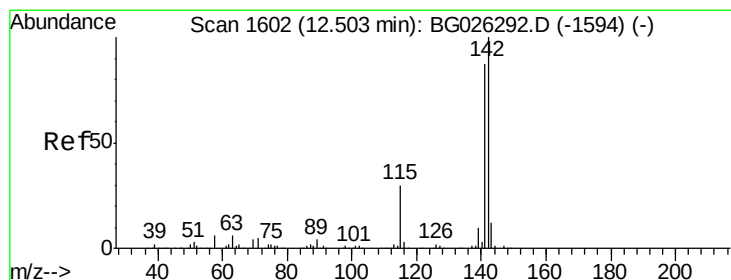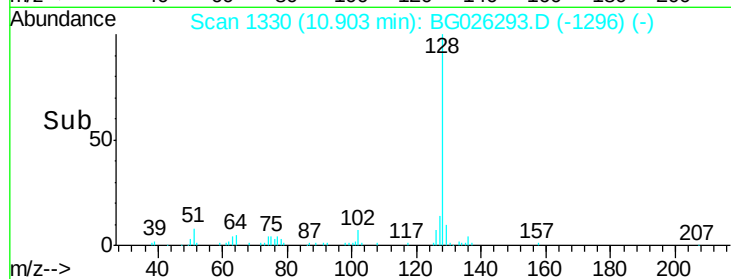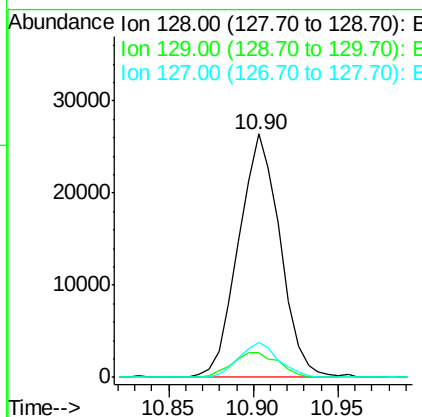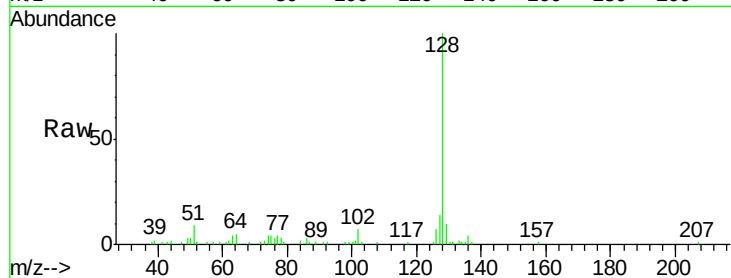

#5

2-Methylnaphthalene

Concen: 1.18 ng/ul




RT: 12.50 min Scan# 1602


Delta R.T. -0.00 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Tgt Ion:	142	Resp:	26522
Ion Ratio	Lower	Upper	
142	100		
141	87.5	69.8	104.8

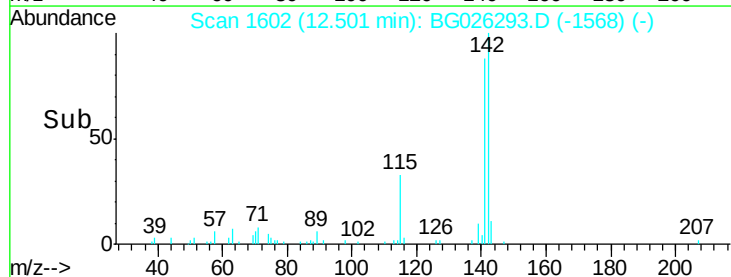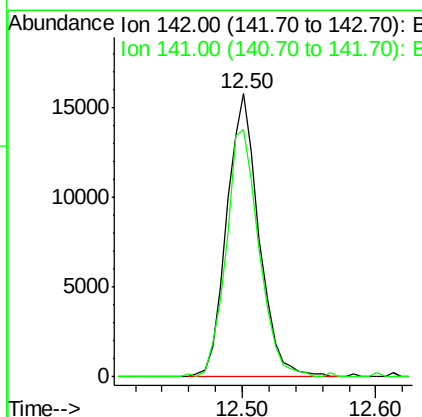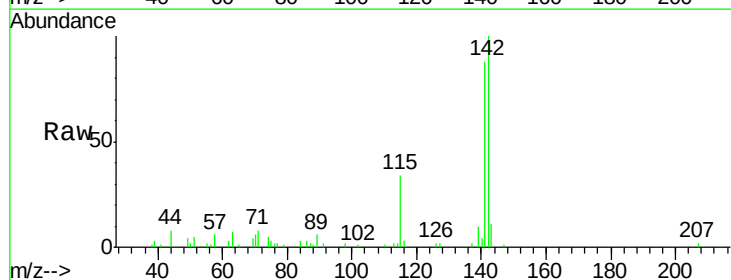

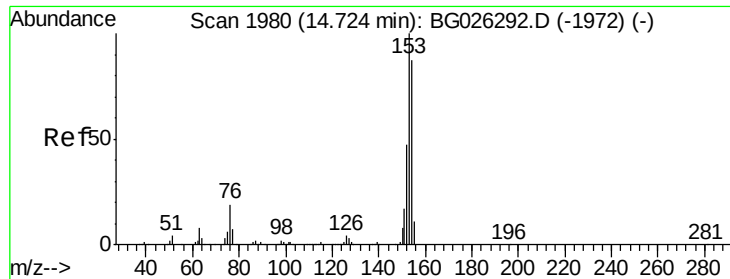

#9

Acenaphthene

Concen: 1.93 ng/ul

RT: 14.72 min Scan# 1980

Delta R.T. -0.00 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Instrument :

BNA_G


ClientSampleId :

CB2Z5




Tgt Ion:	153	Resp:	39957
Ion Ratio	Lower	Upper	
153	100		
152	46.3	37.9	56.9
154	88.7	71.6	107.4

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

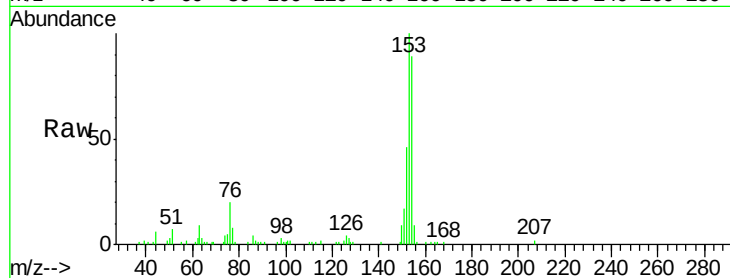

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

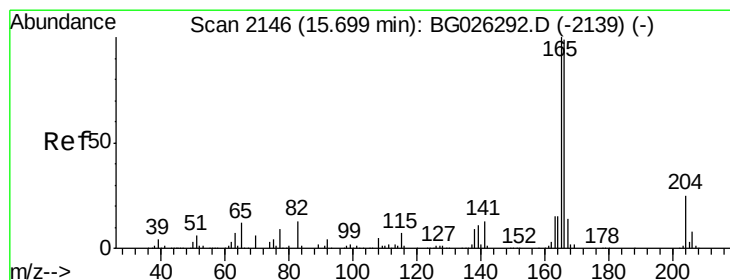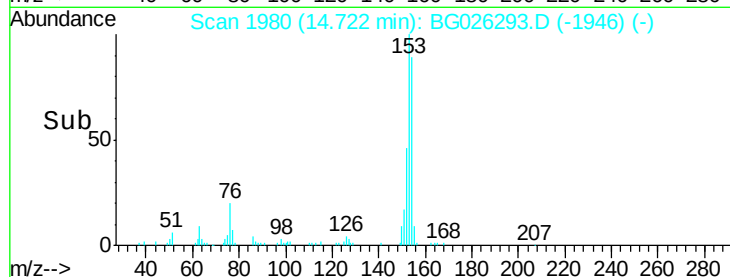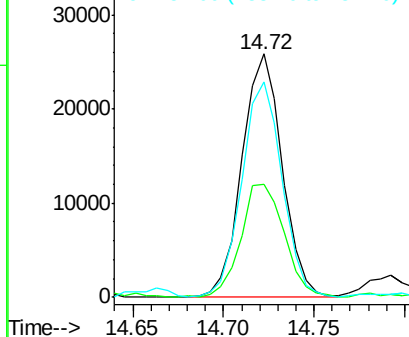

#11

Fluorene

Concen: 1.88 ng/ul

RT: 15.70 min Scan# 2146




Delta R.T. -0.00 min


Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Tgt Ion:	166	Resp:	43908
Ion Ratio	Lower	Upper	
166	100		
165	102.0	80.0	120.0
167	14.9	11.6	17.4

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

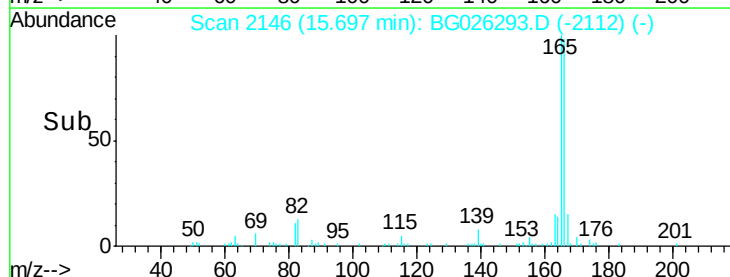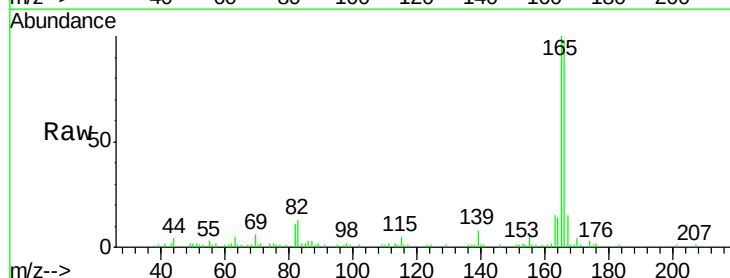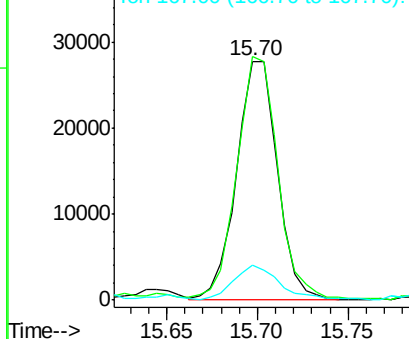

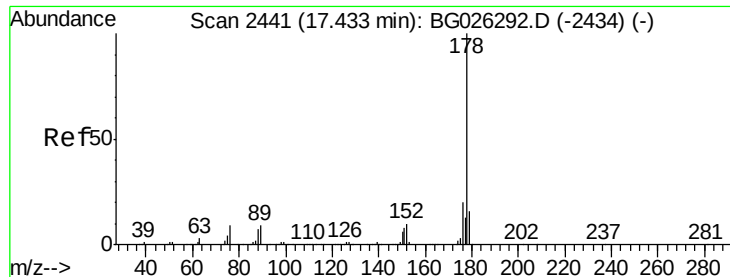





#14
Phenanthrene
Concen: 18.76 ng/ul
RT: 17.43 min Scan# 2441
Delta R.T. -0.00 min
Lab File: BG026293.D
Acq: 17 Mar 2017 22:34

Instrument :
BNA_G
ClientSampled :
CB2Z5

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.1	12.2	18.4
176	19.9	16.4	24.6




Manual Integrations
APPROVED


mohammad
3/20/2017 12:54:59 PM

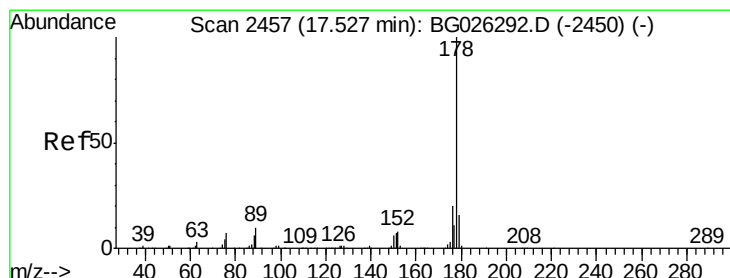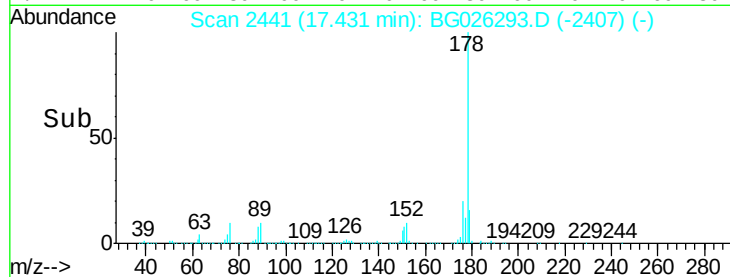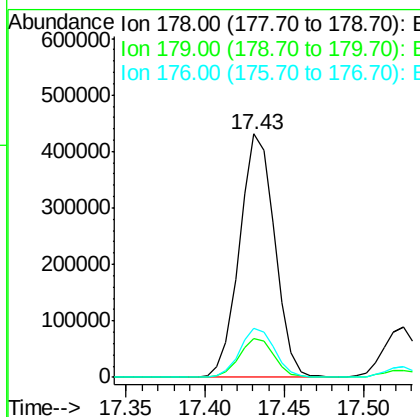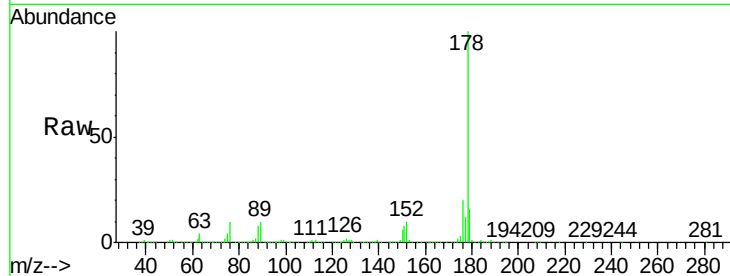

#16
Anthracene
Concen: 3.71 ng/ul
RT: 17.52 min Scan# 2457
Delta R.T. -0.00 min
Lab File: BG026293.D
Acq: 17 Mar 2017 22:34

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.5	12.7	19.1
176	20.2	15.8	23.8

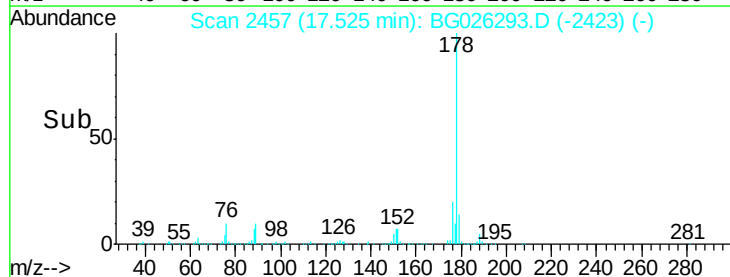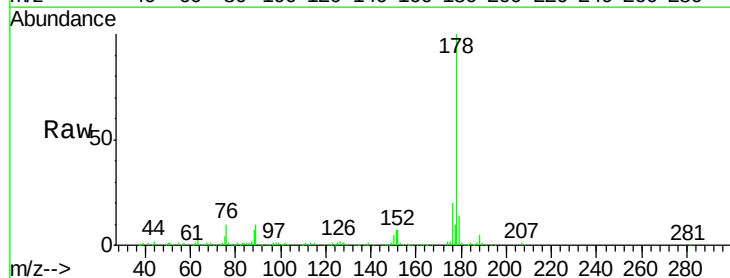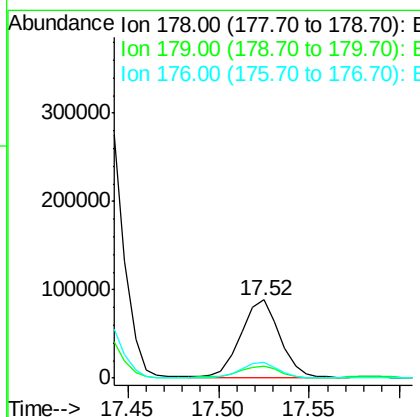

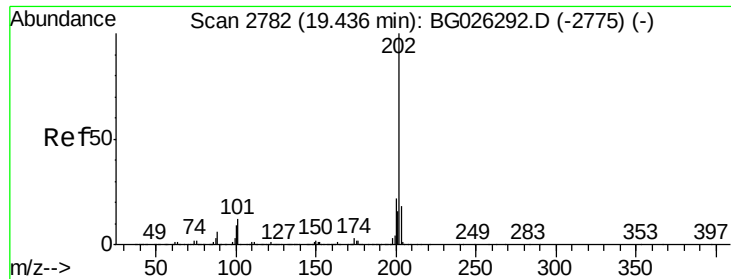





#17
Fluoranthene
Concen: 26.16 ng/ul
RT: 19.43 min Scan# 2782
Delta R.T. -0.00 min
Lab File: BG026293.D
Acq: 17 Mar 2017 22:34

Instrument :
BNA_G
ClientSampleId :
CB2Z5

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		958301		
101	12.9	9.8	14.8		
100	10.0	7.5	11.3		




Manual Integrations
APPROVED


mohammad
3/20/2017 12:54:59 PM

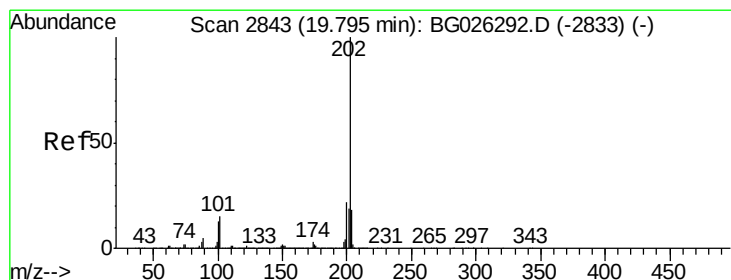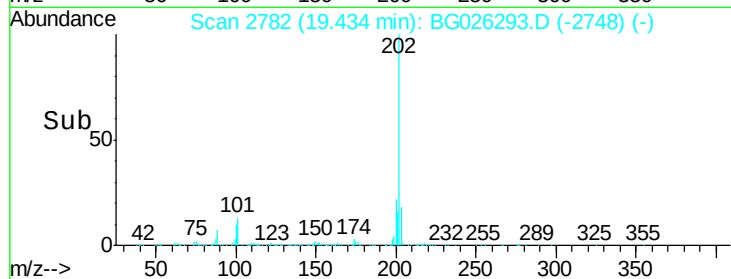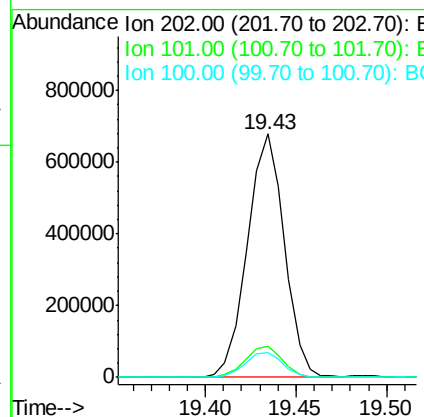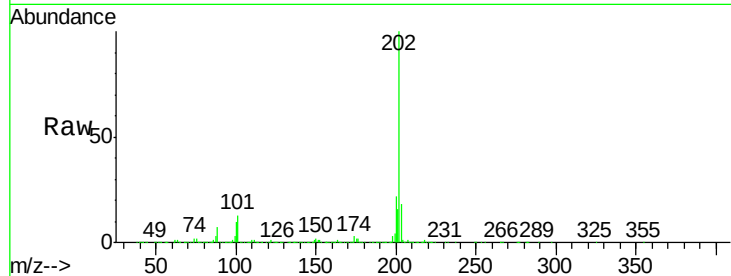

#20
Pyrene
Concen: 20.03 ng/ul
RT: 19.79 min Scan# 2843
Delta R.T. -0.00 min
Lab File: BG026293.D
Acq: 17 Mar 2017 22:34

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		826884		
101	15.5	11.2	16.8		
100	13.0	9.8	14.6		

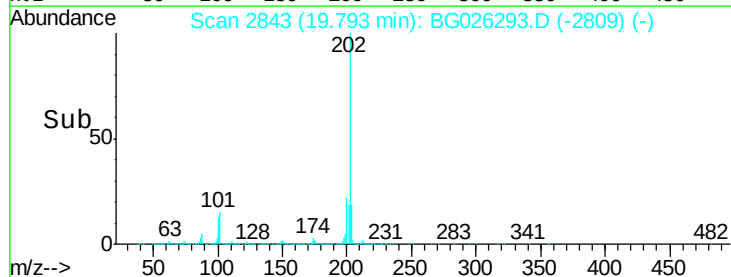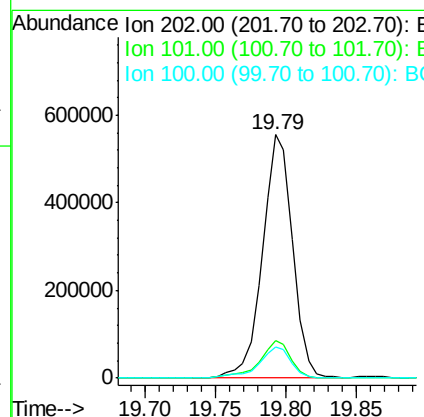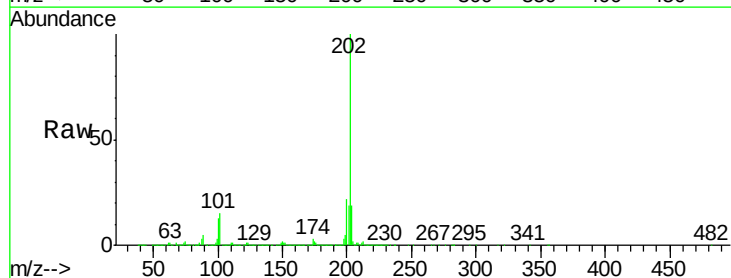

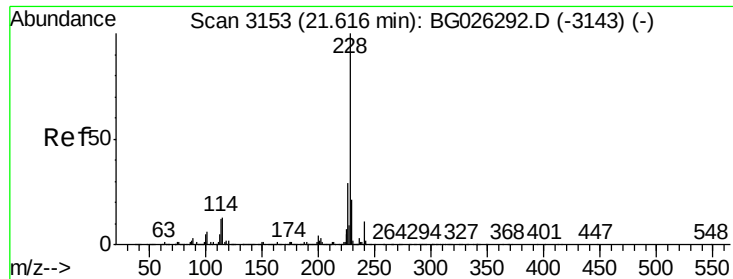

#21

Benzo(a)anthracene

Concen: 12.52 ng/ul

RT: 21.61 min Scan# 3153

Delta R.T. -0.00 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Instrument :

BNA_G





ClientSampleId :

CB2Z5

Tgt	Ion:228	Resp:	451774
Ion	Ratio	Lower	Upper
228	100		
229	20.3	15.9	23.9
226	28.9	22.1	33.1

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

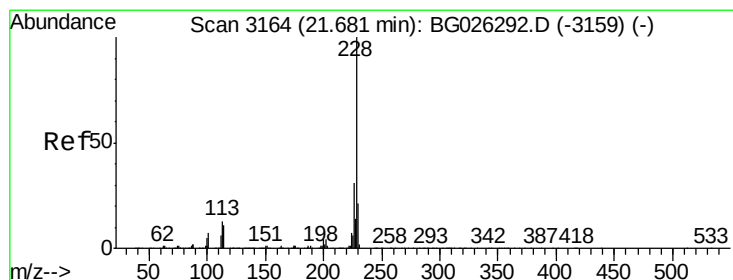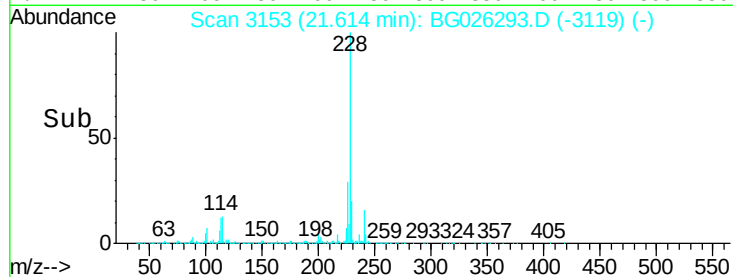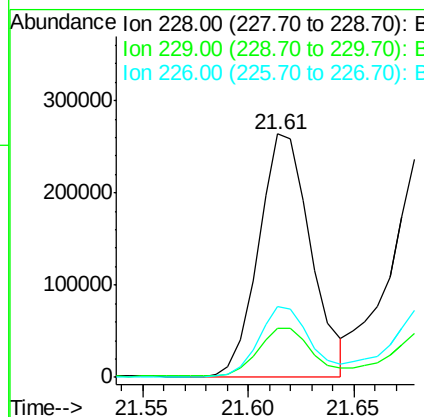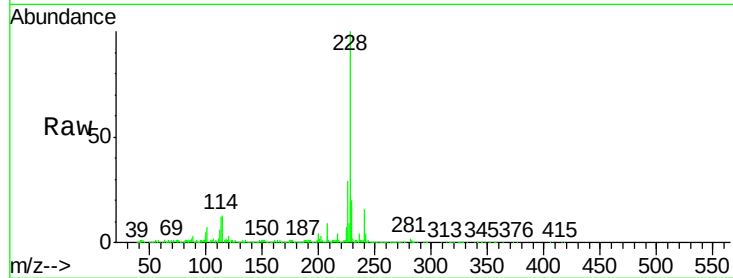

#22

Chrysene

Concen: 13.16 ng/ul




RT: 21.68 min Scan# 3165


Delta R.T. 0.00 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Tgt	Ion:228	Resp:	443021
Ion	Ratio	Lower	Upper
228	100		
226	30.8	25.0	37.6
229	20.4	16.6	25.0

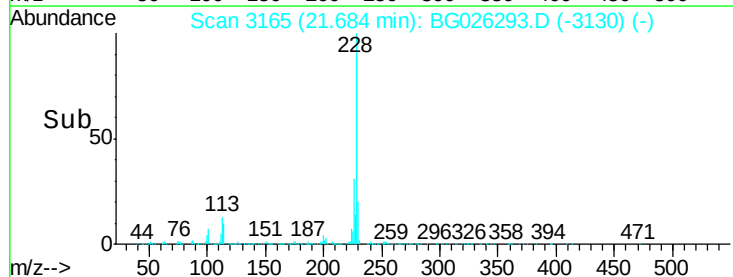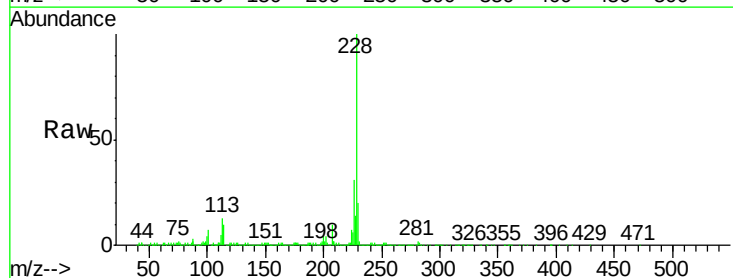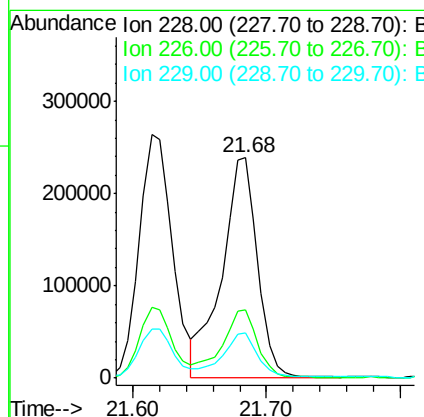

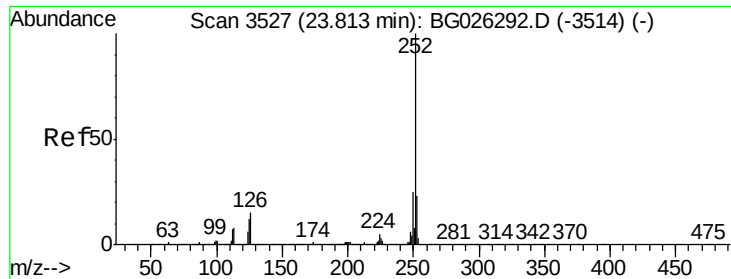

#24

Benzo(b)fluoranthene

Concen: 16.43 ng/ul

RT: 23.81 min Scan# 3527

Delta R.T. -0.00 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Instrument :

BNA_G





ClientSampled :

CB2Z5

Tgt Ion:	252	Resp:	564284
Ion Ratio	Lower	Upper	
252	100		
253	21.4	17.8	26.6
125	13.1	9.4	14.0

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

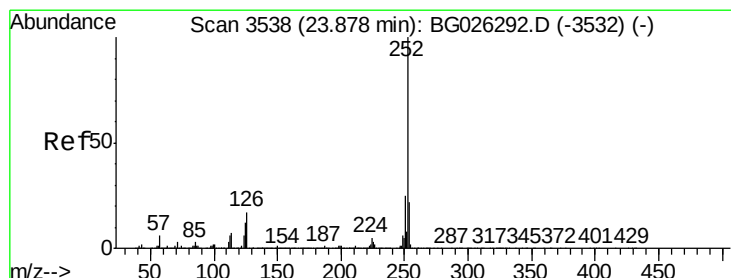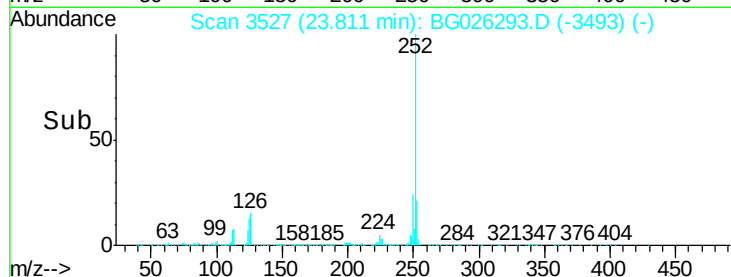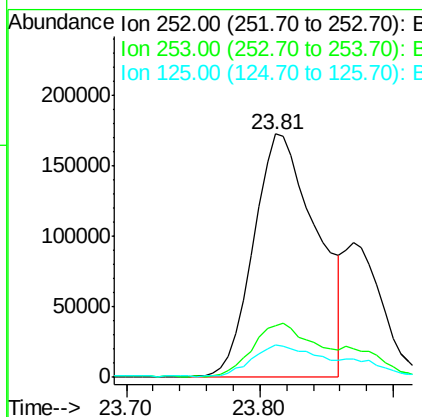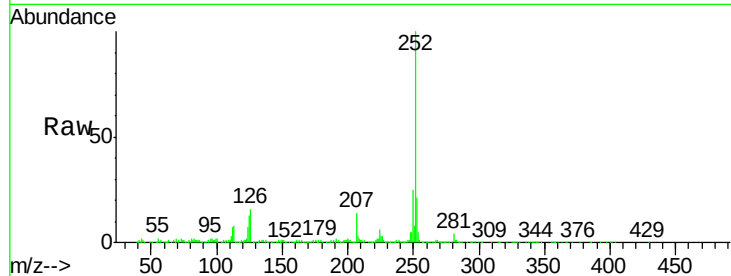

#25

Benzo(k)fluoranthene

Concen: 5.91 ng/ul m




RT: 23.87 min Scan# 3537


Delta R.T. -0.01 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Tgt Ion:	252	Resp:	193753
Ion Ratio	Lower	Upper	
252	100		
253	21.4	17.4	26.2
125	13.7	8.8	13.2#

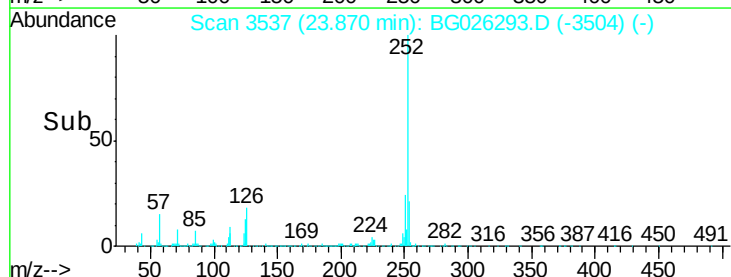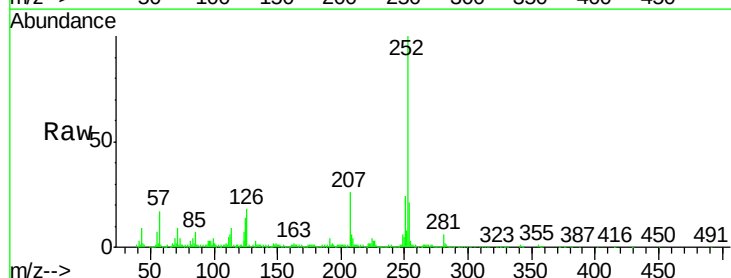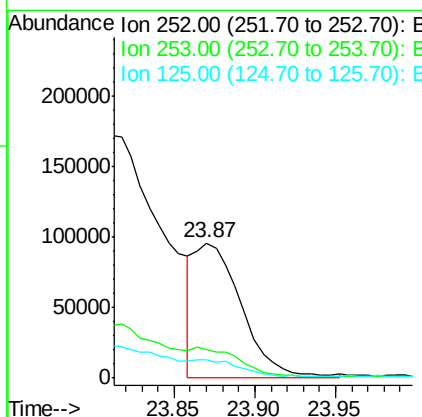

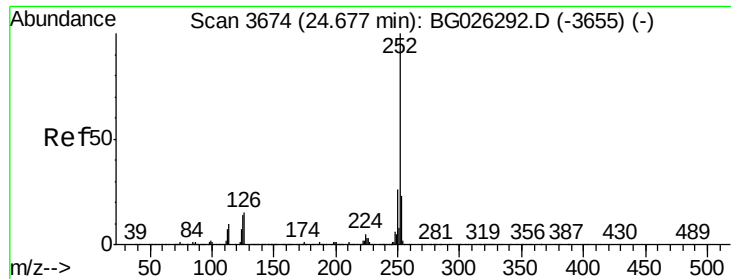

#27

Benzo(a)pyrene

Concen: 10.44 ng/ul

RT: 24.67 min Scan# 3673

Delta R.T. -0.01 min

Lab File: BG026293.D





Acq: 17 Mar 2017 22:34

Instrument :
BNA_G
ClientSampleId :
CB2Z5

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	23.3	17.1	25.7
125	14.4	9.4	14.2

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

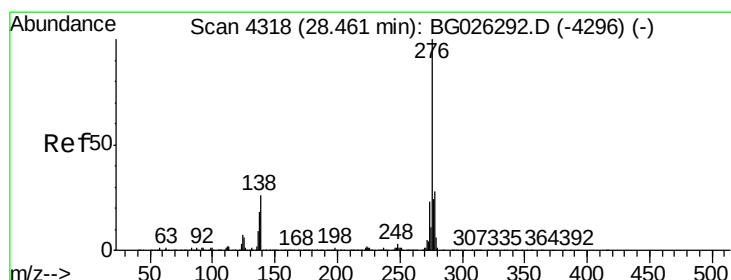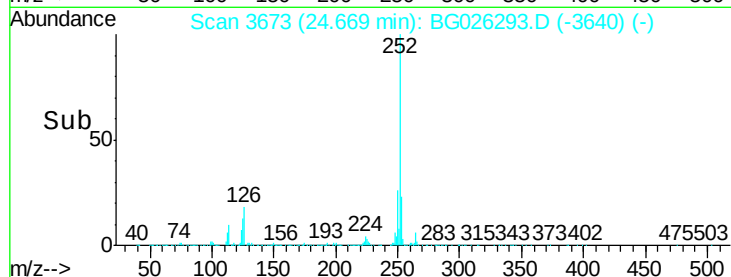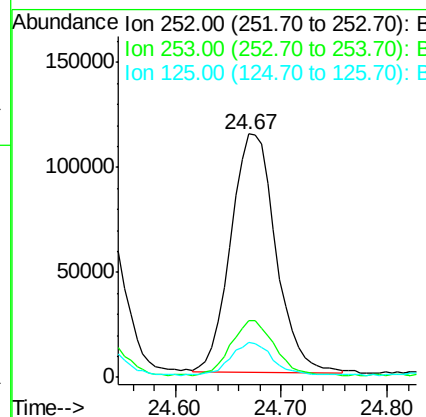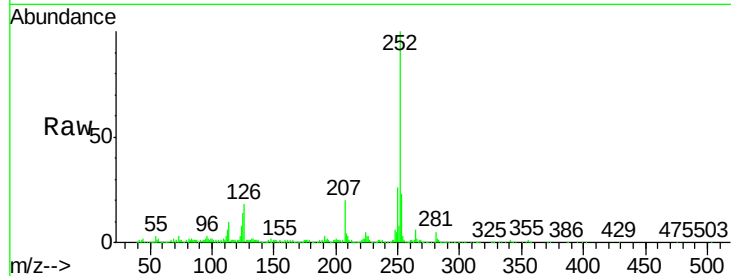

#28

Indeno(1,2,3-cd)pyrene

Concen: 5.43 ng/ul




RT: 28.45 min Scan# 4317


Delta R.T. -0.01 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	26.9	17.8	26.6
277	23.8	19.4	29.0

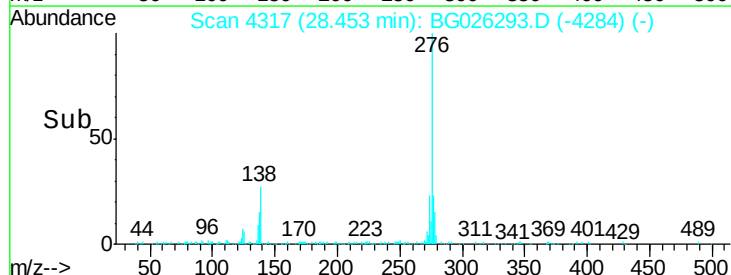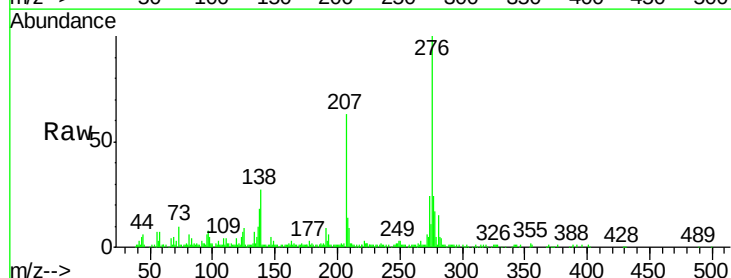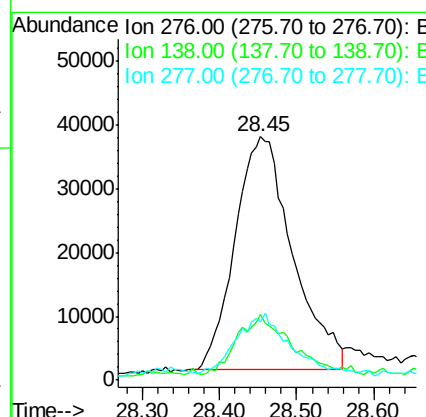

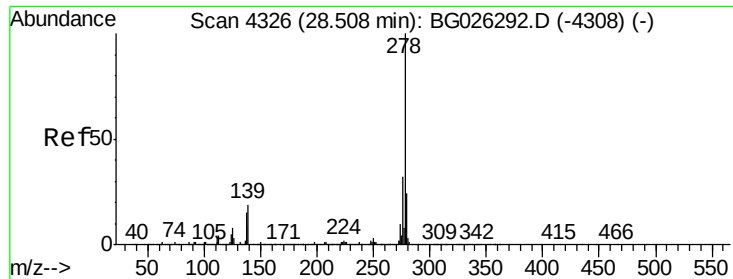

#29

Dibenzo(a,h)anthracene

Concen: 2.13 ng/ul m

RT: 28.49 min Scan# 4324

Delta R.T. -0.01 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Instrument :

BNA_G





ClientSampleId :

CB2Z5

Tgt Ion:	278	Resp:	59658
Ion Ratio	Lower	Upper	
278	100		
139	22.1	14.0	21.0#
279	26.2	20.6	31.0

Manual Integrations
APPROVED

mohammad
3/20/2017 12:54:59 PM

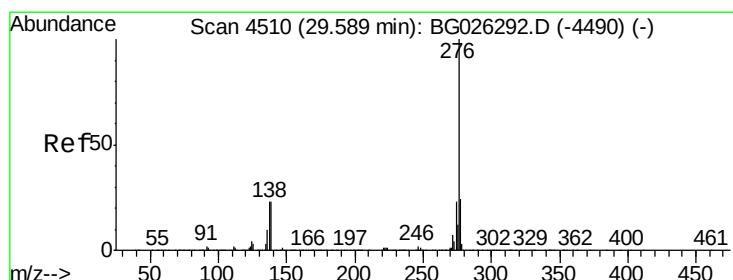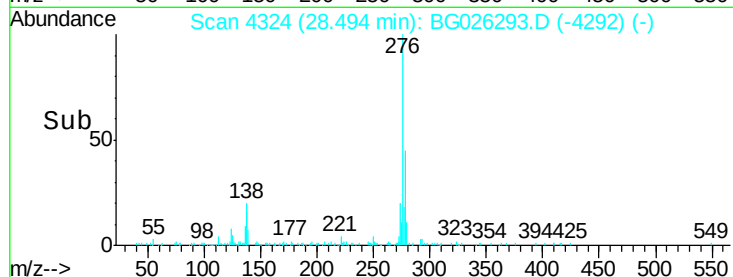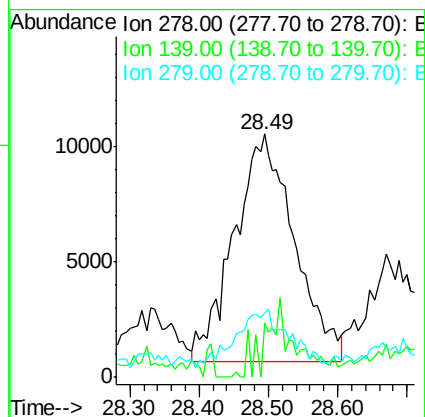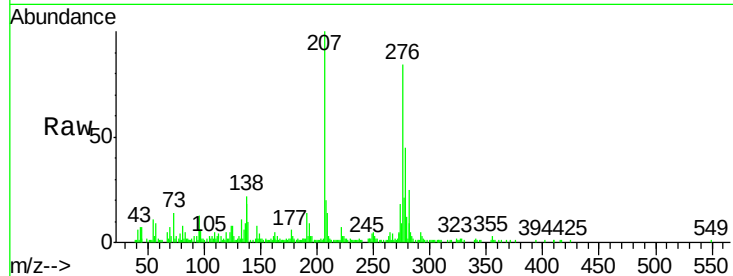

#30

Benzo(g,h,i)perylene

Concen: 5.11 ng/ul m

RT: 29.58 min Scan# 4509

Delta R.T. -0.01 min

Lab File: BG026293.D

Acq: 17 Mar 2017 22:34

Tgt Ion:	276	Resp:	154159
Ion Ratio	Lower	Upper	
276	100		
138	25.6	19.0	28.4
277	23.6	19.7	29.5

