

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031717\
 Data File : BG026304.D
 Acq On : 18 Mar 2017 5:46
 Operator : SJ/MA
 Sample : I2283-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB305

Manual Integrations
 APPROVED

mohammad
 3/20/2017 12:55:26 PM

Quant Time: Mar 18 06:31:09 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 18 00:29:44 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	160495	20.00	ng/ul	0.00
2) Naphthalene-d8	10.85	136	751900	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.66	164	412757	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	813030	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	803361	20.00	ng/ul	0.00
23) Perylene-d12	24.83	264	764756	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.47	165	20057	1.80	ng/uL	0.00
7) Acenaphthylene-d8	14.35	160	621916	17.67	ng/ul	0.00
10) Fluorene-d10	15.64	176	459903	17.91	ng/ul	0.00
15) Anthracene-d10	17.49	188	619327	17.14	ng/ul	0.00
19) Pyrene-d10	19.76	212	644649	15.73	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.60	264	563069	17.07	ng/ul	0.00
Target Compounds						
						Qvalue
4) Naphthalene	10.90	128	71995	1.96	ng/ul	98
5) 2-Methylnaphthalene	12.50	142	46457	1.70	ng/ul	98
9) Acenaphthene	14.72	153	102061	4.02	ng/ul	100
11) Fluorene	15.70	166	122045	4.26	ng/ul	98
14) Phenanthrene	17.44	178	1570823	36.46	ng/ul	97
16) Anthracene	17.52	178	333799	7.67	ng/ul	99
17) Fluoranthene	19.43	202	1779116	39.77	ng/ul	97
20) Pyrene	19.80	202	1531834	29.95	ng/ul	99
21) Benzo(a)anthracene	21.62	228	816954	18.27	ng/ul	97
22) Chrysene	21.68	228	777459	18.64	ng/ul	98
24) Benzo(b)fluoranthene	23.82	252	952388	21.93	ng/ul	98
25) Benzo(k)fluoranthene	23.87	252	284870m	6.87	ng/ul	
27) Benzo(a)pyrene	24.67	252	597119	14.80	ng/ul	98
28) Indeno(1,2,3-cd)pyrene	28.46	276	309765	6.95	ng/ul	97
29) Dibenzo(a,h)anthracene	28.49	278	85530m	2.42	ng/ul	
30) Benzo(g,h,i)perylene	29.59	276	238948m	6.27	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG031717\
Data File : BG026304.D
Acq On : 18 Mar 2017 5:46
Operator : SJ/MA
Sample : I2283-06
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
CB305

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

Quant Time: Mar 18 06:31:09 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 18 00:29:44 2017
Response via : Initial Calibration

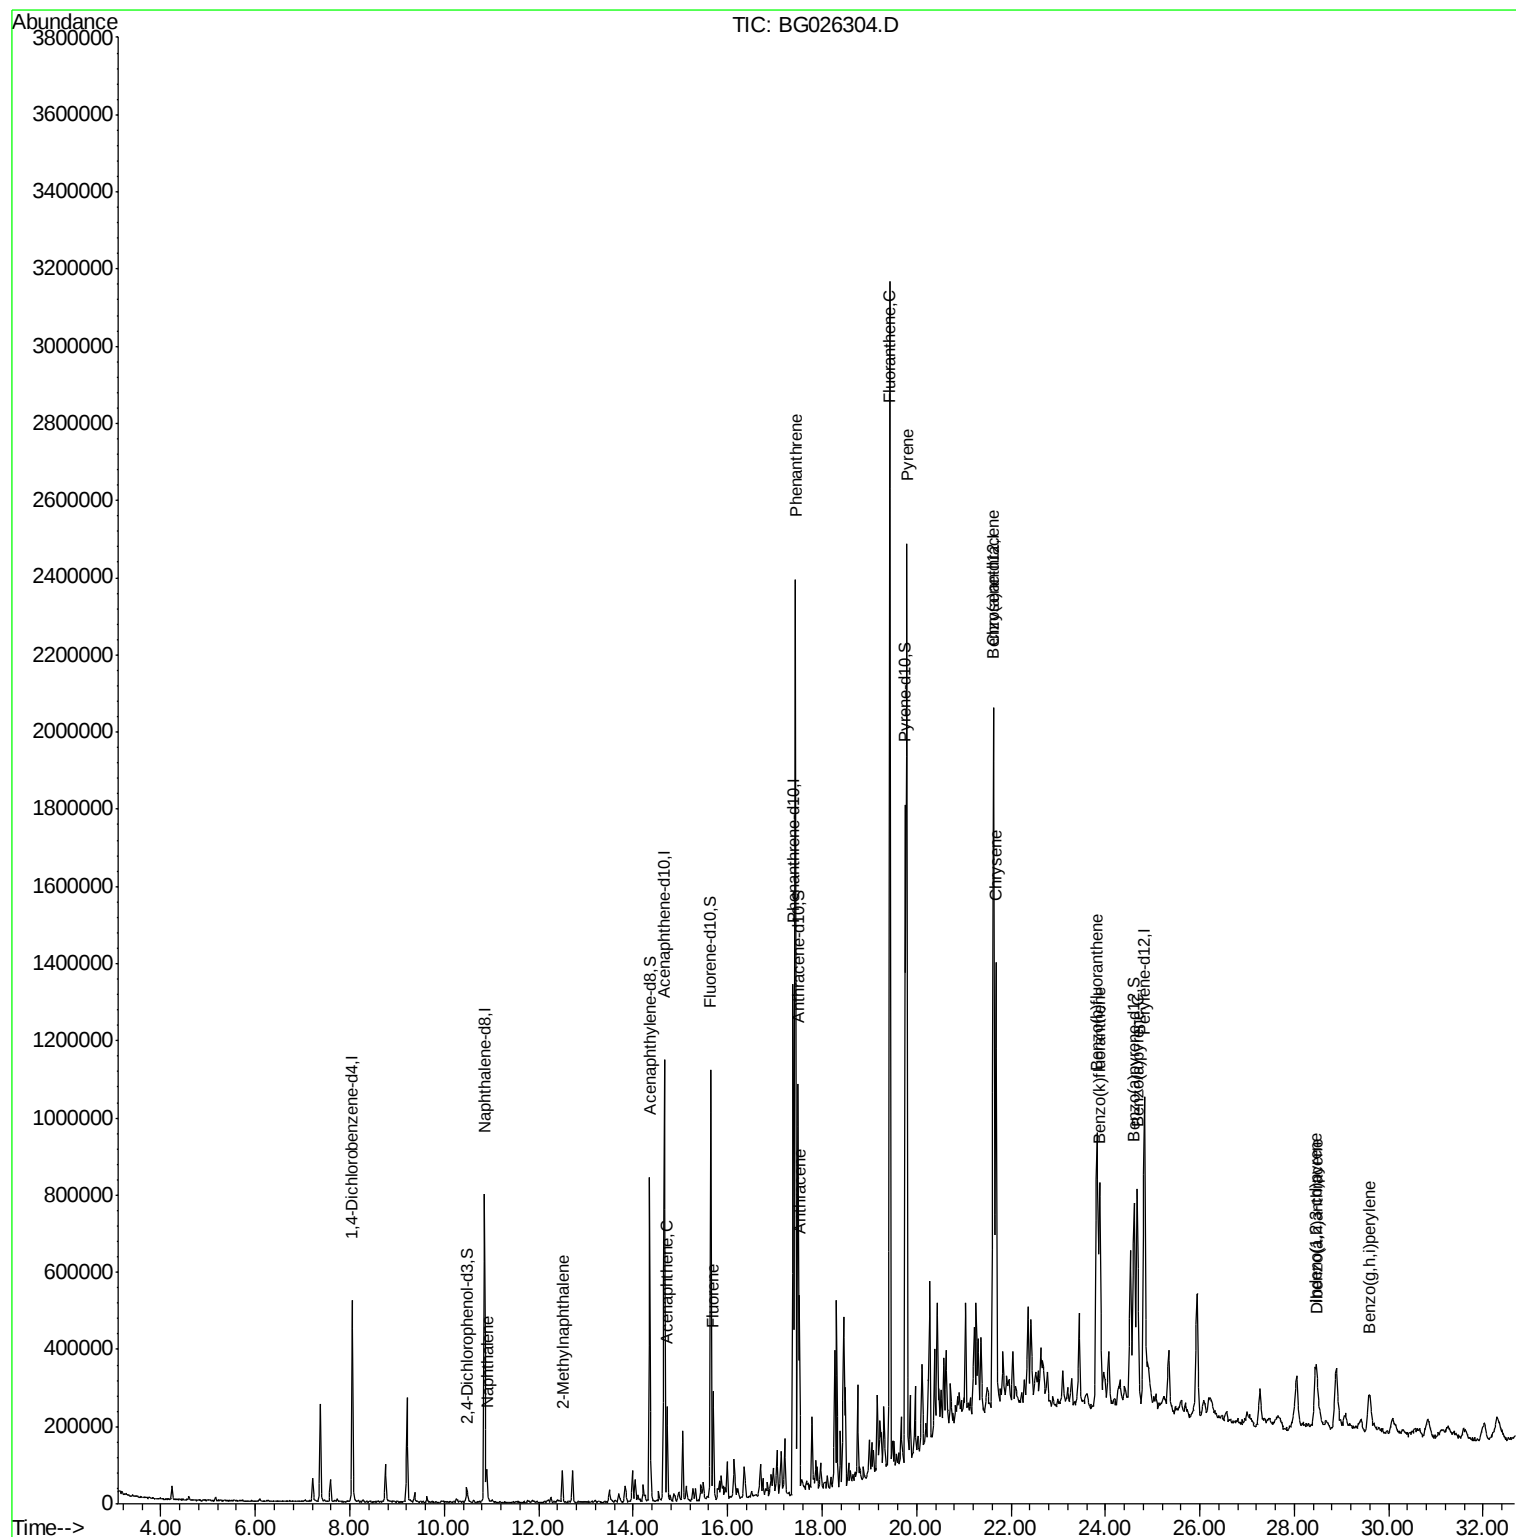

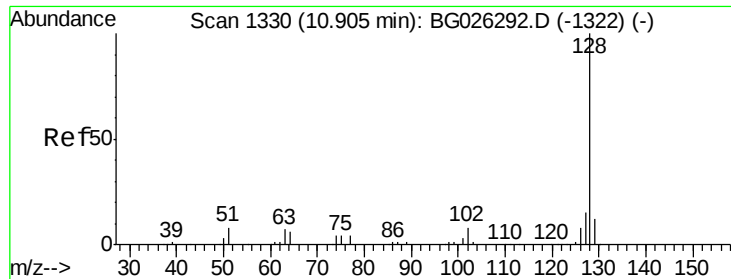

#4

Naphthalene

Concen: 1.96 ng/ul

RT: 10.90 min Scan# 1330

Delta R.T. -0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Instrument :

BNA_G





ClientSampled :

CB305

Tgt Ion:	128	Resp:	71995
Ion Ratio	Lower	Upper	
128	100		
129	10.2	9.1	13.7
127	13.9	10.6	15.8

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

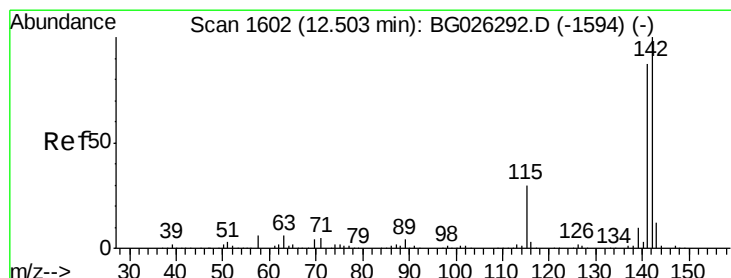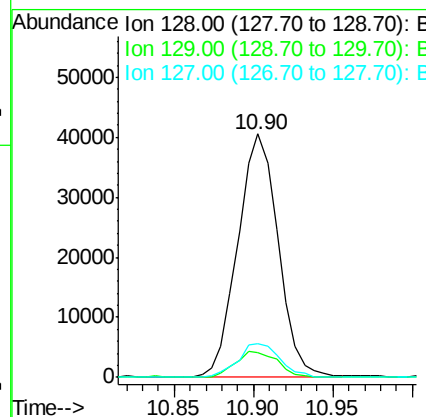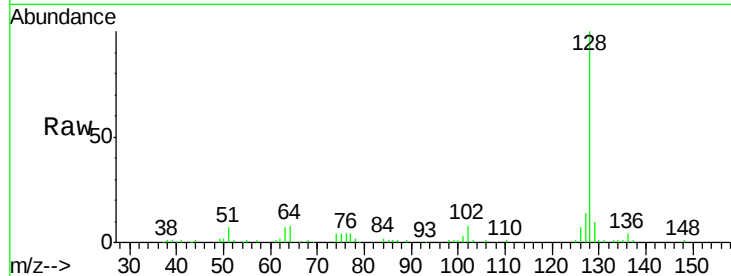

#5

2-Methylnaphthalene

Concen: 1.70 ng/ul




RT: 12.50 min Scan# 1602


Delta R.T. -0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Tgt Ion:	142	Resp:	46457
Ion Ratio	Lower	Upper	
142	100		
141	88.7	69.8	104.8

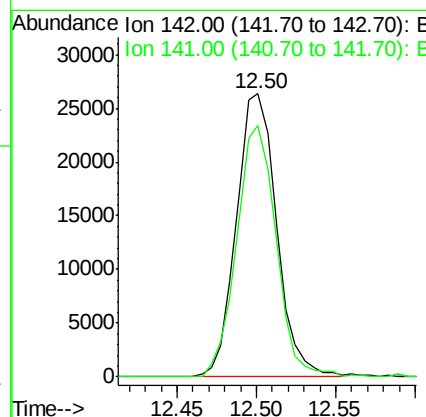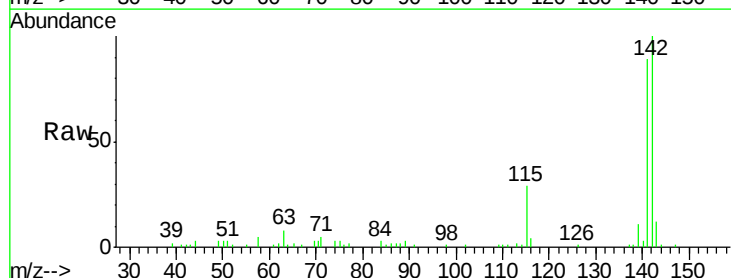

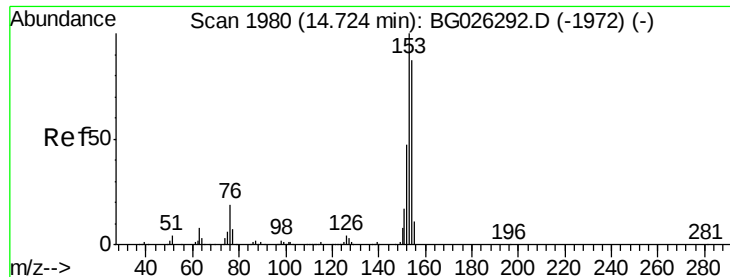

#9

Acenaphthene

Concen: 4.02 ng/ul

RT: 14.72 min Scan# 1980

Delta R.T. -0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Instrument :

BNA_G


ClientSampleId :

CB305




Tgt Ion:	153	Resp:	102061
Ion Ratio	Lower	Upper	
153	100		
152	46.7	37.9	56.9
154	89.7	71.6	107.4

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

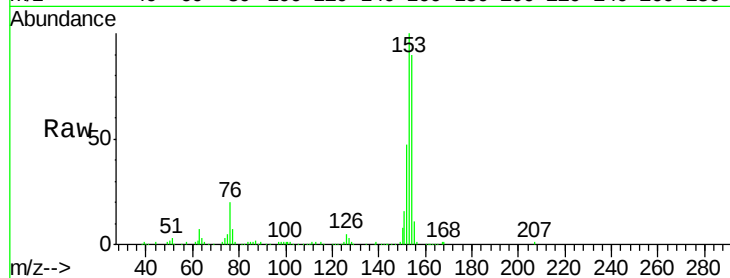

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

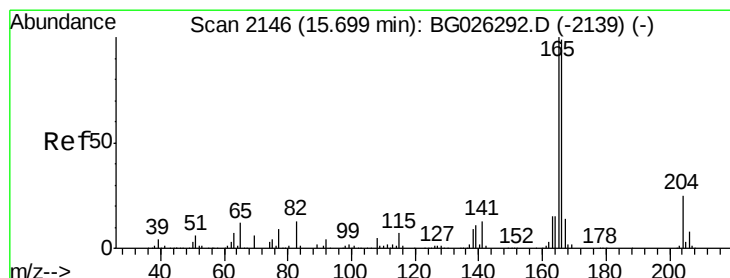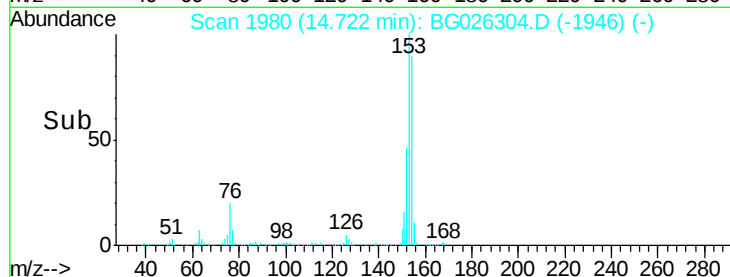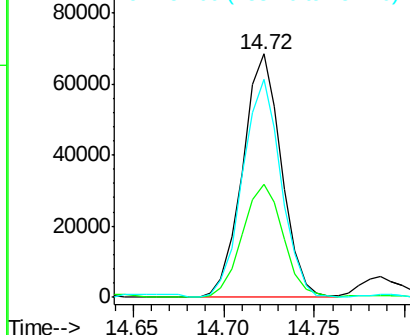

#11

Fluorene

Concen: 4.26 ng/ul

RT: 15.70 min Scan# 2146




Delta R.T. -0.00 min


Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Tgt Ion:	166	Resp:	122045
Ion Ratio	Lower	Upper	
166	100		
165	97.9	80.0	120.0
167	14.4	11.6	17.4

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

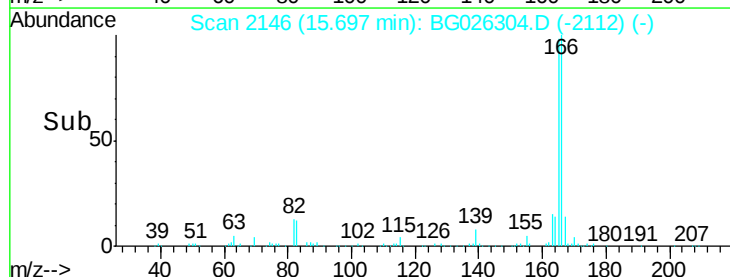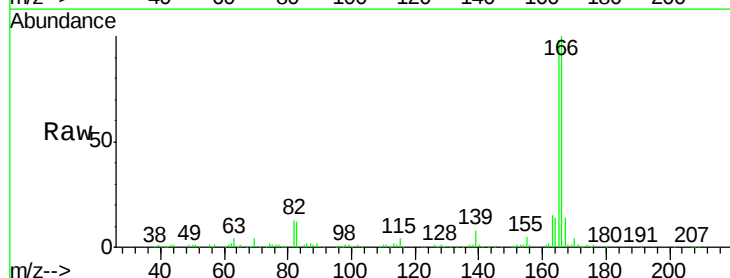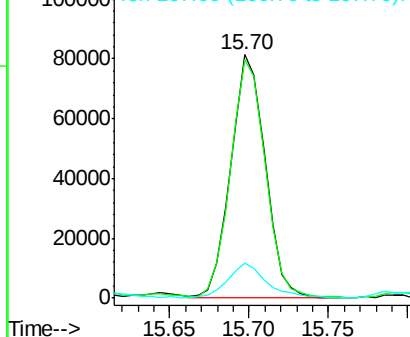

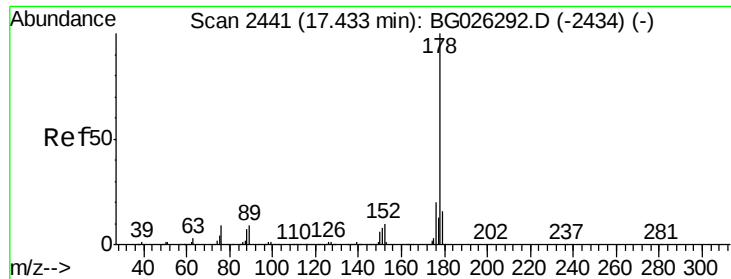





#14
Phenanthrene
Concen: 36.46 ng/ul
RT: 17.44 min Scan# 2442
Delta R.T. 0.00 min
Lab File: BG026304.D
Acq: 18 Mar 2017 5:46

Instrument :
BNA_G
ClientSampleId :
CB305

Tgt Ion:178 Resp: 1570823
Ion Ratio Lower Upper
178 100
179 17.0 12.2 18.4
176 21.3 16.4 24.6




Manual Integrations
APPROVED


mohammad
3/20/2017 12:55:26 PM

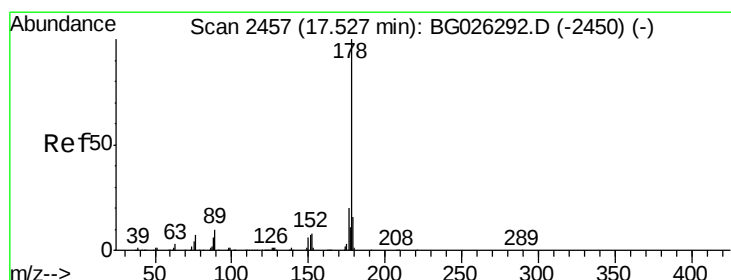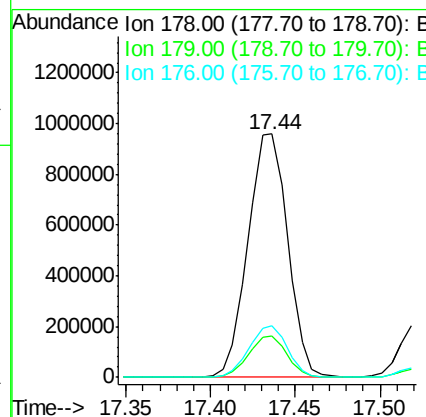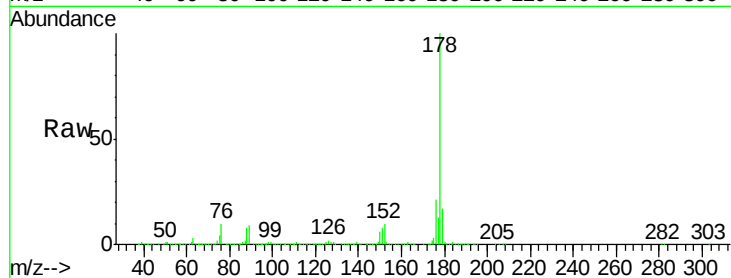

#16
Anthracene
Concen: 7.67 ng/ul
RT: 17.52 min Scan# 2457
Delta R.T. -0.00 min
Lab File: BG026304.D
Acq: 18 Mar 2017 5:46

Tgt Ion:178 Resp: 333799
Ion Ratio Lower Upper
178 100
179 15.8 12.7 19.1
176 18.7 15.8 23.8

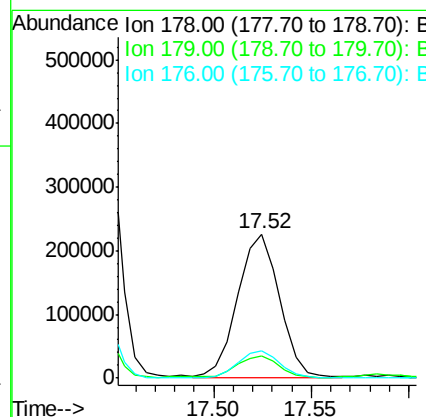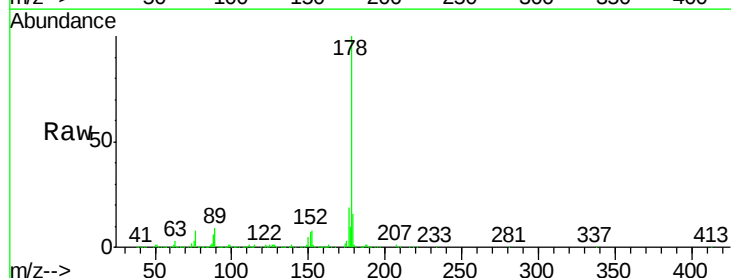

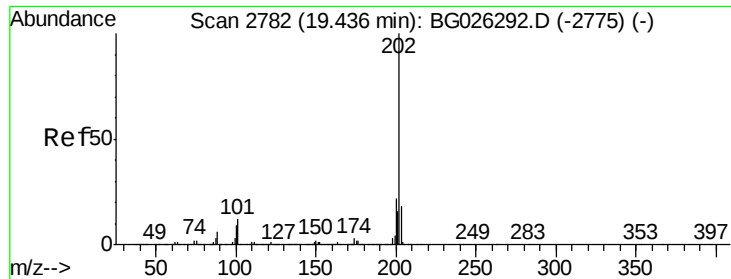

#17

Fluoranthene

Concen: 39.77 ng/ul

RT: 19.43 min Scan# 2782

Delta R.T. -0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Instrument :

BNA_G





ClientSampleId :

CB305

Tgt Ion:	202	Resp:	1779116
Ion	Ratio	Lower	Upper
202	100		
101	13.8	9.8	14.8
100	10.5	7.5	11.3

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

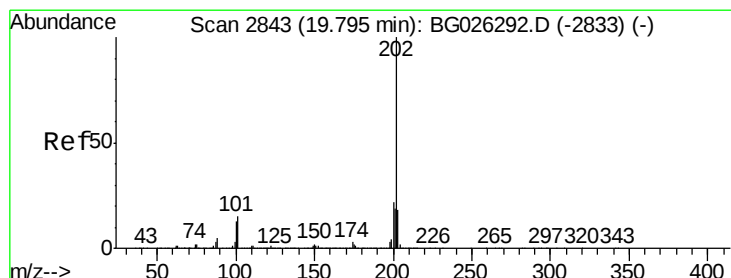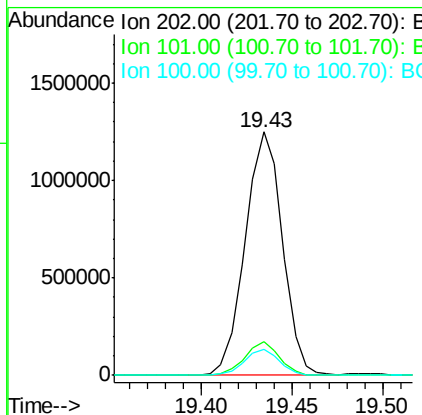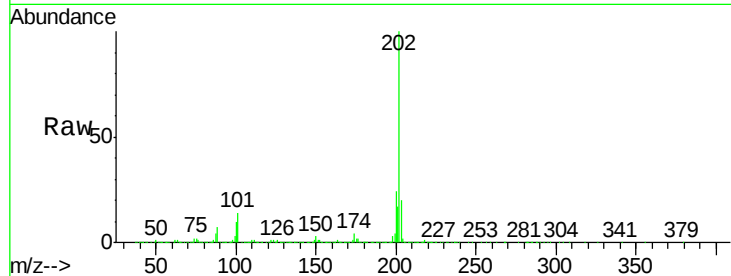

#20

Pyrene

Concen: 29.95 ng/ul




RT: 19.80 min Scan# 2844


Delta R.T. 0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Tgt Ion:	202	Resp:	1531834
Ion	Ratio	Lower	Upper
202	100		
101	14.7	11.2	16.8
100	12.0	9.8	14.6

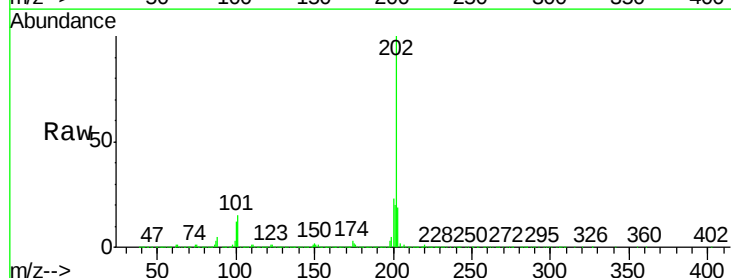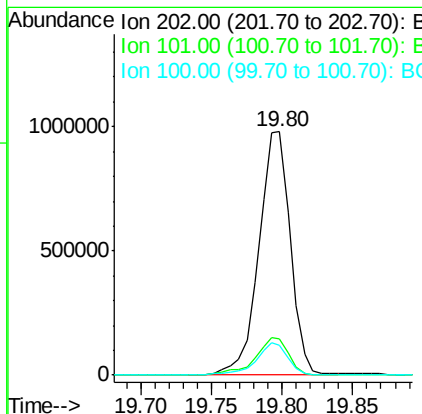

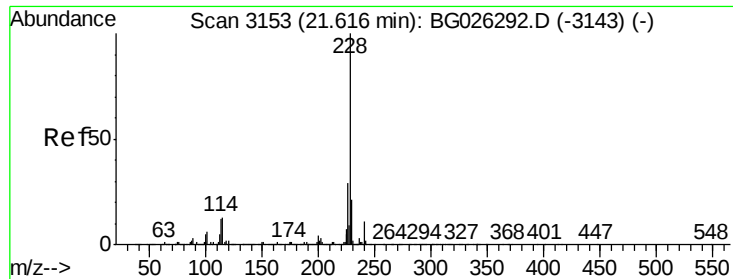





#21
Benzo(a)anthracene
Concen: 18.27 ng/ul
RT: 21.62 min Scan# 3154
Delta R.T. 0.00 min
Lab File: BG026304.D
Acq: 18 Mar 2017 5:46

Instrument :
BNA_G
ClientSampleId :
CB305

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.5	15.9	23.9
226	29.0	22.1	33.1




Manual Integrations
APPROVED


mohammad
3/20/2017 12:55:26 PM

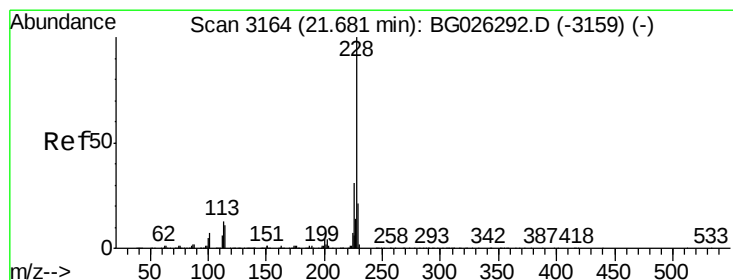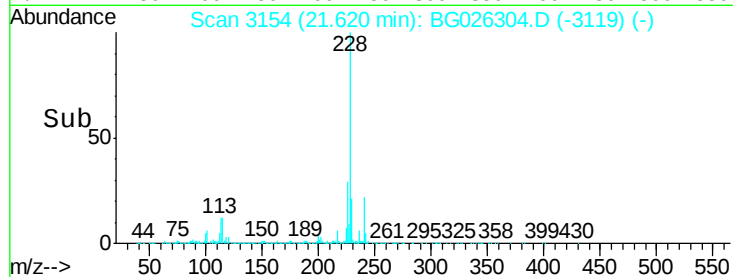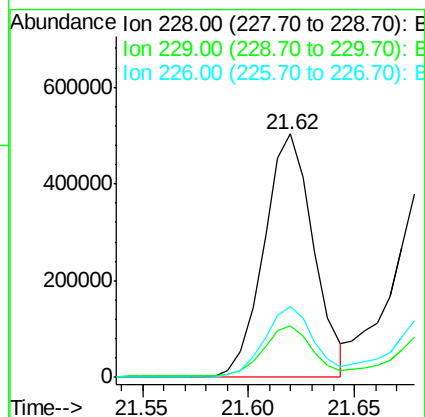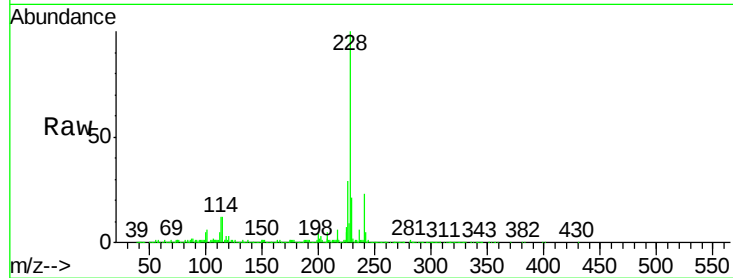

#22
Chrysene
Concen: 18.64 ng/ul
RT: 21.68 min Scan# 3165
Delta R.T. 0.00 min
Lab File: BG026304.D
Acq: 18 Mar 2017 5:46

Tgt Ion	Ratio	Lower	Upper
228	100		
226	32.5	25.0	37.6
229	21.2	16.6	25.0

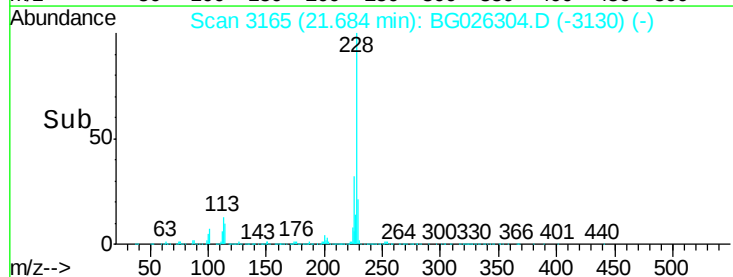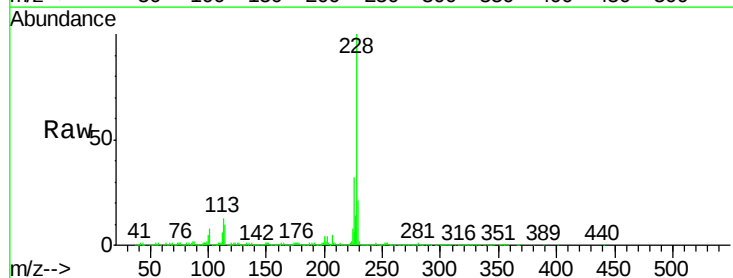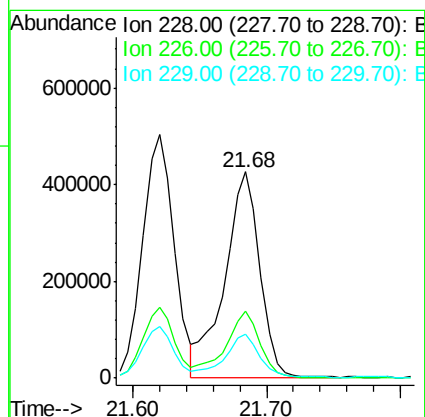

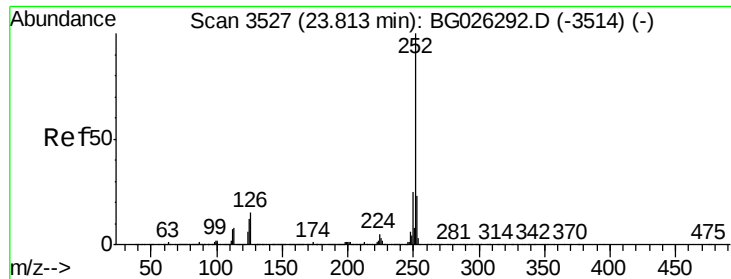

#24

Benzo(b)fluoranthene

Concen: 21.93 ng/ul

RT: 23.82 min Scan# 3528

Delta R.T. 0.00 min

Lab File: BG026304.D





Acq: 18 Mar 2017 5:46

Instrument :
BNA_G
ClientSampleId :
CB305

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	21.3	17.8	26.6
125	12.5	9.4	14.0

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

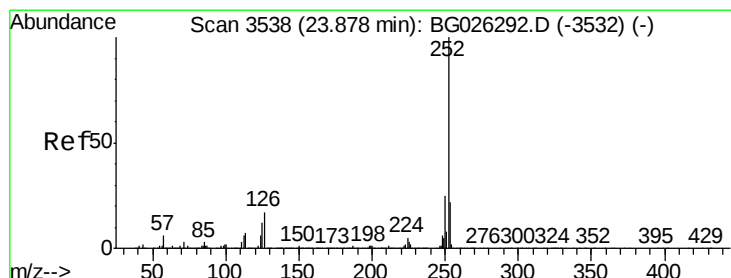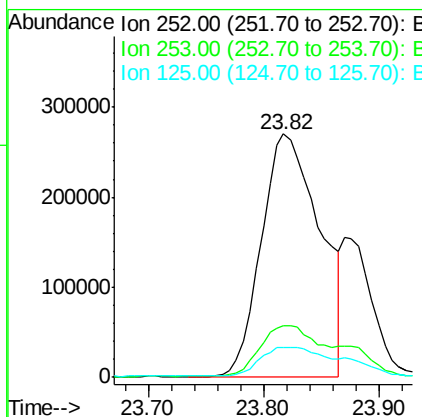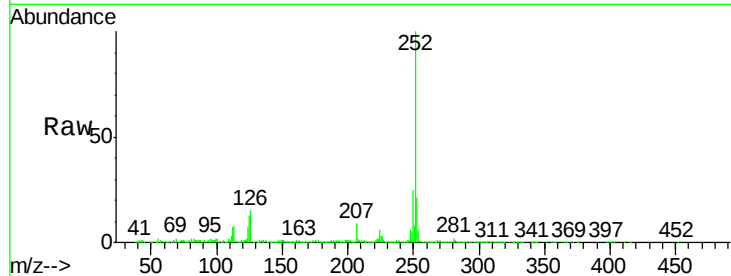

#25

Benzo(k)fluoranthene

Concen: 6.87 ng/ul m




RT: 23.87 min Scan# 3537


Delta R.T. -0.01 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	22.1	17.4	26.2
125	13.9	8.8	13.2#

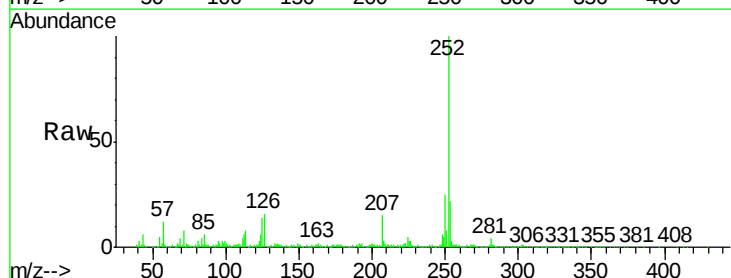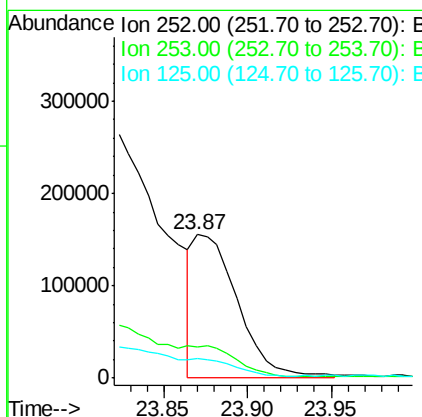

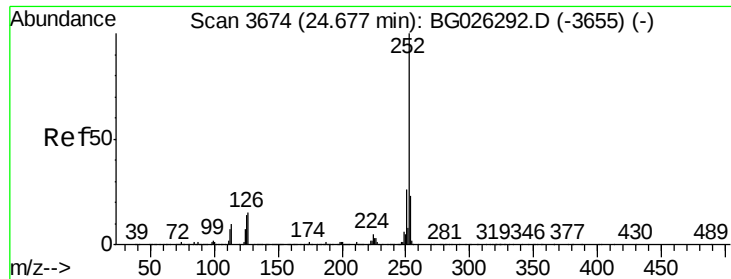

#27

Benzo(a)pyrene

Concen: 14.80 ng/ul

RT: 24.67 min Scan# 3674

Delta R.T. -0.00 min

Lab File: BG026304.D





Acq: 18 Mar 2017 5:46

Instrument :
BNA_G
ClientSampled :
CB305

Tgt Ion	Ratio	Resp Lower	Resp Upper
252	100		
253	22.3	17.1	25.7
125	12.8	9.4	14.2

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

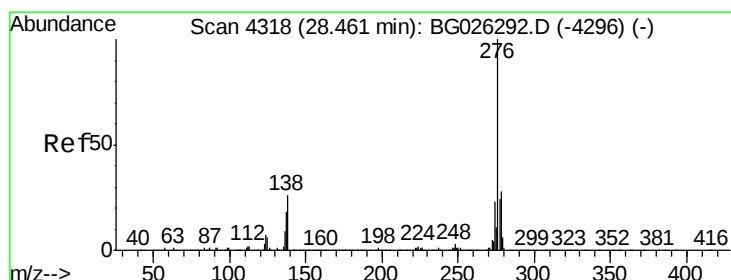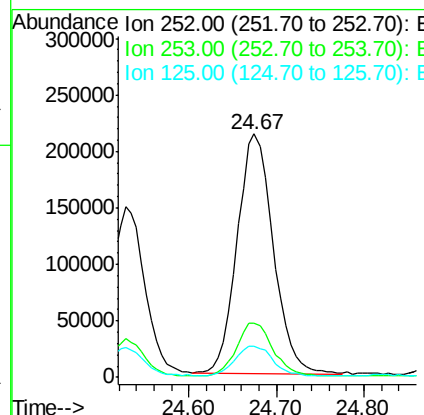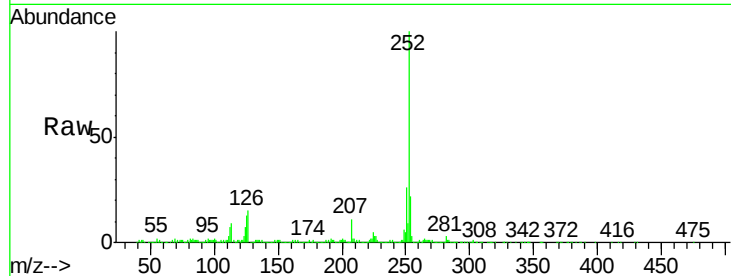

#28

Indeno(1,2,3-cd)pyrene

Concen: 6.95 ng/ul




RT: 28.46 min Scan# 4318


Delta R.T. -0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	24.0	17.8	26.6
277	22.8	19.4	29.0

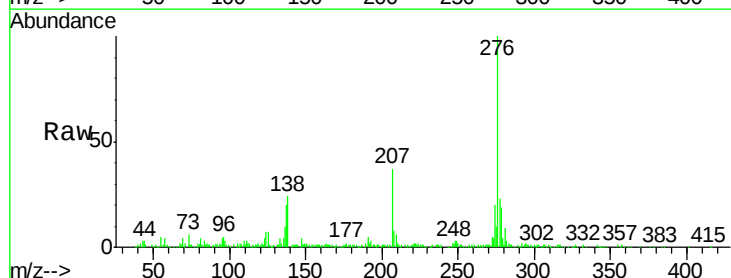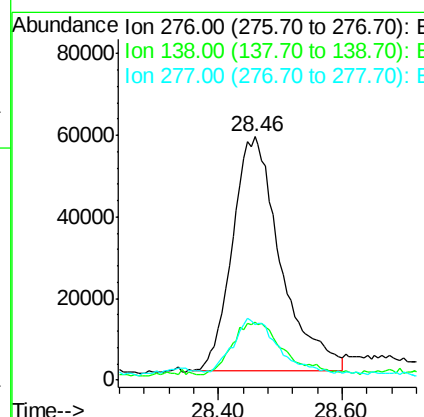

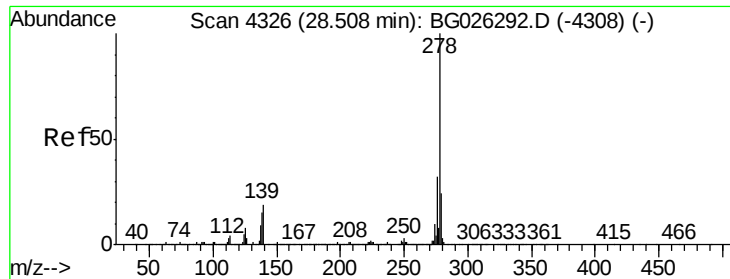

#29

Dibenzo(a,h)anthracene

Concen: 2.42 ng/ul m

RT: 28.49 min Scan# 4323

Delta R.T. -0.02 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Instrument :

BNA_G





ClientSampleId :

CB305

Tgt Ion:	278	Resp:	85530
Ion Ratio	Lower	Upper	
278	100		
139	18.6	14.0	21.0
279	25.2	20.6	31.0

Manual Integrations
APPROVED

mohammad
3/20/2017 12:55:26 PM

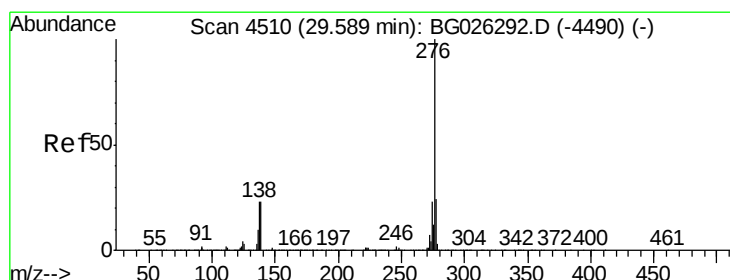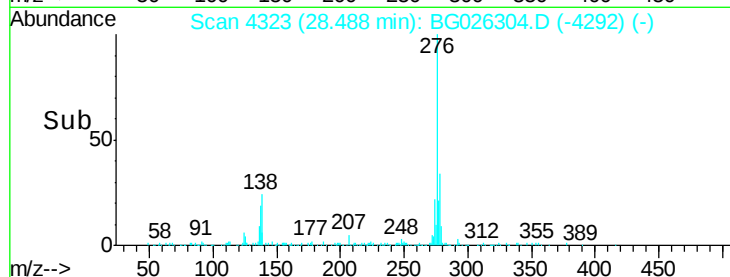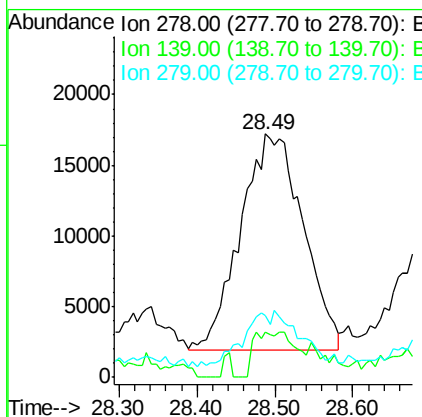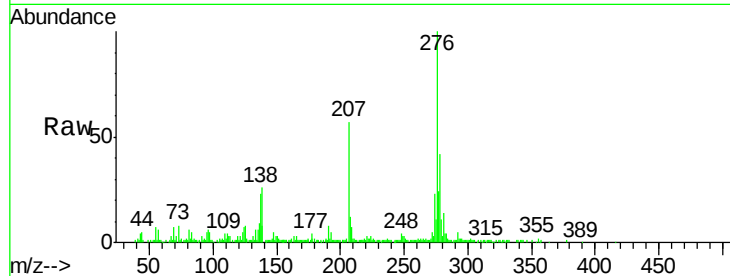

#30

Benzo(g,h,i)perylene

Concen: 6.27 ng/ul m

RT: 29.59 min Scan# 4510

Delta R.T. -0.00 min

Lab File: BG026304.D

Acq: 18 Mar 2017 5:46

Tgt Ion:	276	Resp:	238948
Ion Ratio	Lower	Upper	
276	100		
138	25.4	19.0	28.4
277	22.1	19.7	29.5

