


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031720\  
 Data File : BG044827.D  
 Acq On : 17 Mar 2020 10:32  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG031020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Mar 16 17:37:15 2020

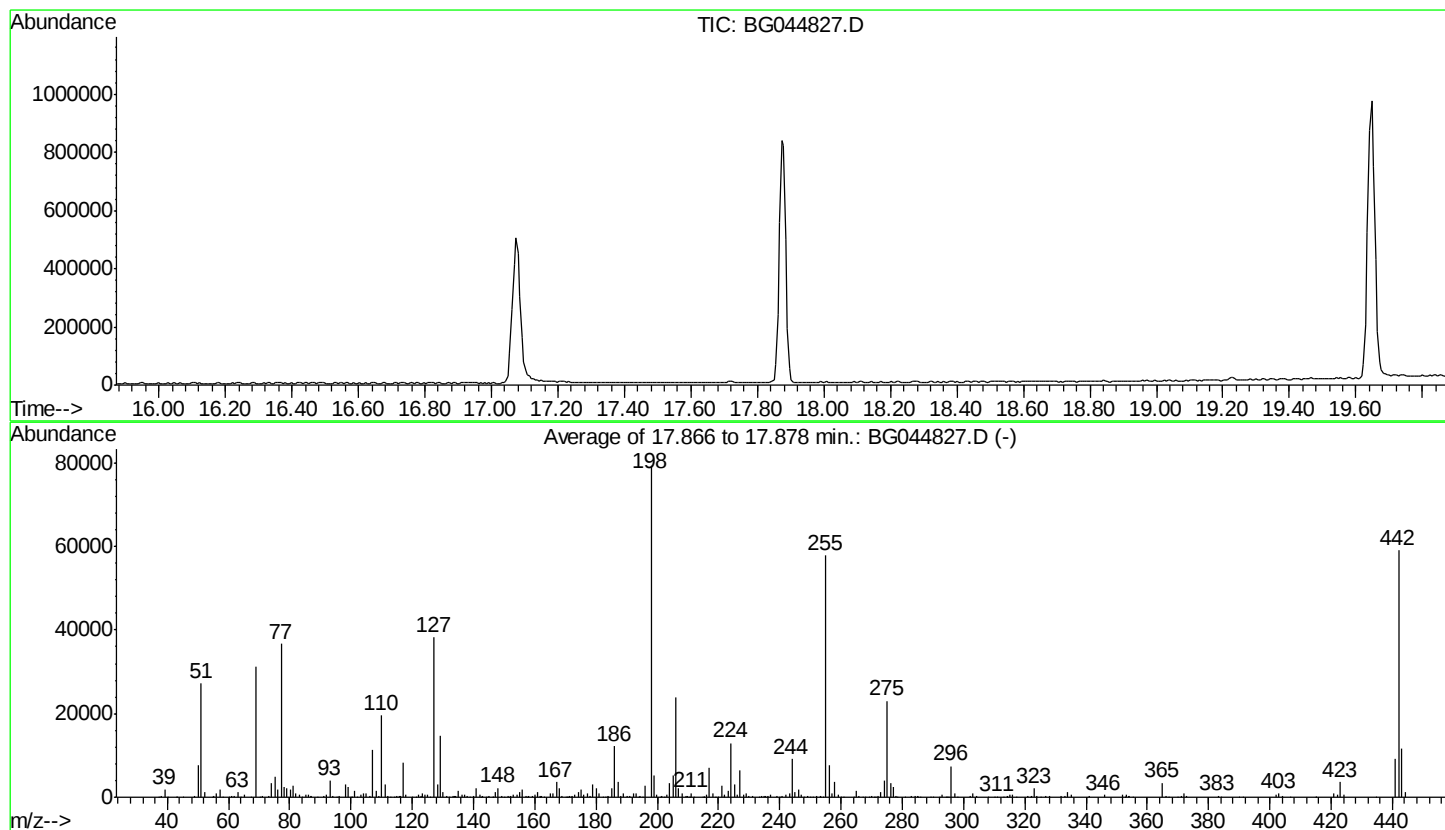

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.3      | 27186   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 39.4      | 31242   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 80      | PASS             |
| 127         | 198          | 10           | 80           | 48.2      | 38210   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 79322   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 5341    | PASS             |
| 275         | 198          | 10           | 60           | 29.1      | 23105   | PASS             |
| 365         | 198          | 1            | 100          | 4.4       | 3473    | PASS             |
| 441         | 198          | 0.01         | 100          | 11.6      | 9215    | PASS             |
| 442         | 198          | 50           | 100          | 74.3      | 58962   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 11529   | PASS             |