


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031720\
 Data File : BG044835.D
 Acq On : 17 Mar 2020 16:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 17:37:15 2020

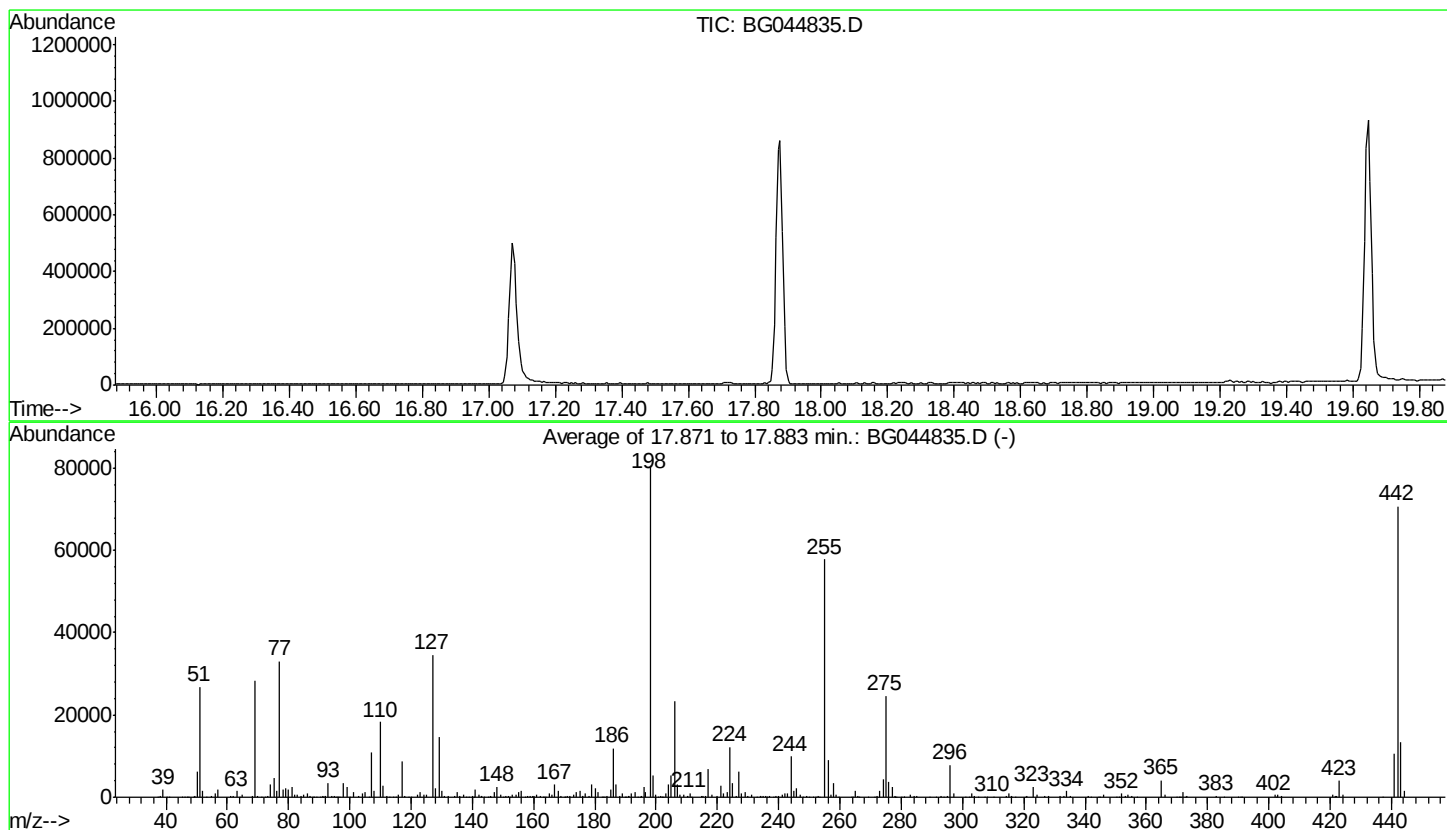

AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	26898	PASS
68	69	0.00	2	1.5	417	PASS
69	198	0.00	100	35.0	28202	PASS
70	69	0.00	2	1.1	304	PASS
127	198	10	80	43.0	34685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80610	PASS
199	198	5	9	6.7	5376	PASS
275	198	10	60	30.5	24621	PASS
365	198	1	100	5.2	4173	PASS
441	198	0.01	100	13.0	10502	PASS
442	198	50	100	87.8	70765	PASS
443	442	15	24	19.0	13418	PASS