


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031720\
 Data File : BG044854.D
 Acq On : 18 Mar 2020 6:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 17:37:15 2020

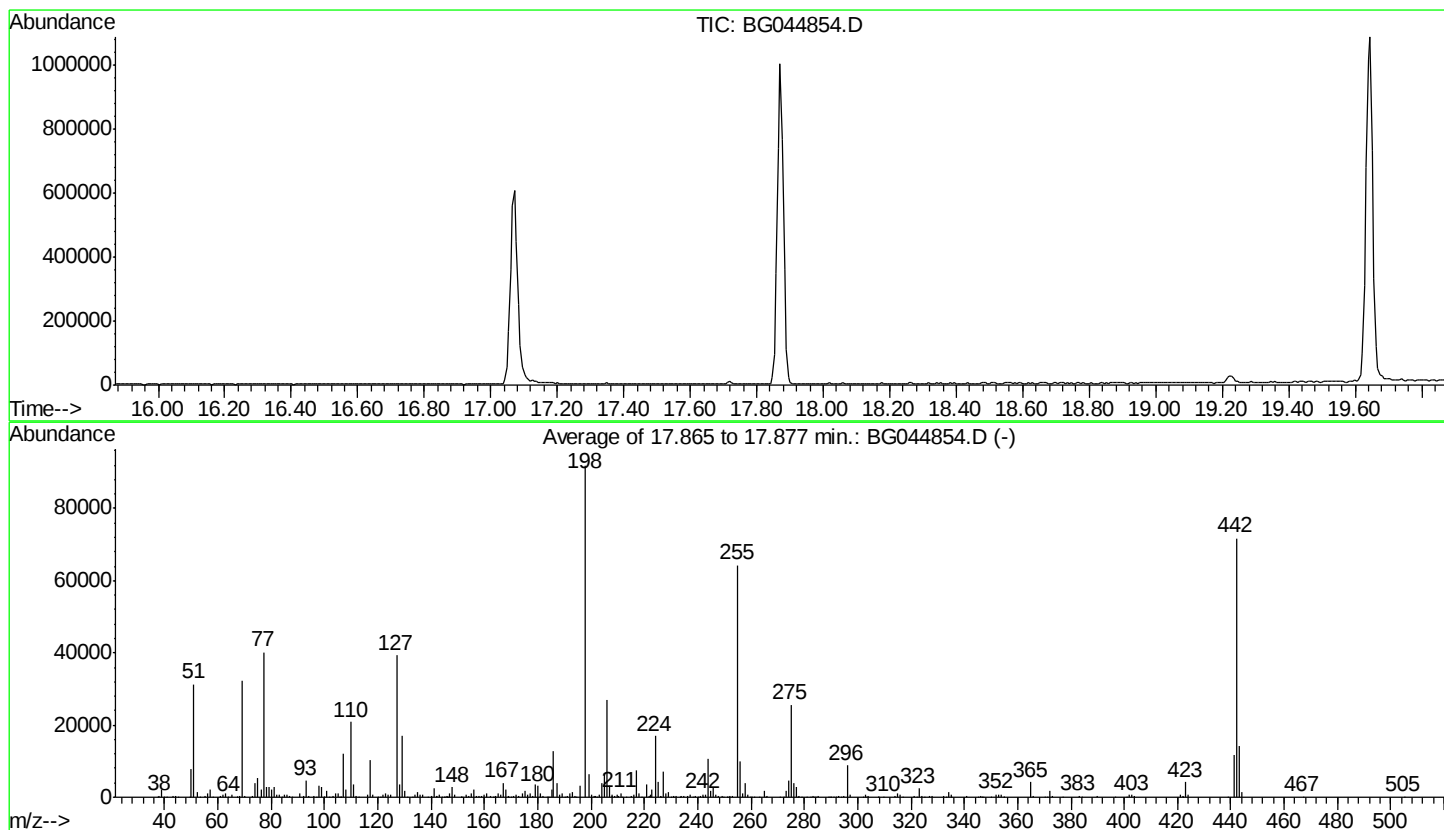

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	31325	PASS
68	69	0.00	2	0.9	282	PASS
69	198	0.00	100	35.1	32221	PASS
70	69	0.00	2	1.0	334	PASS
127	198	10	80	42.7	39245	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91866	PASS
199	198	5	9	6.8	6271	PASS
275	198	10	60	28.0	25717	PASS
365	198	1	100	4.6	4230	PASS
441	198	0.01	100	12.8	11792	PASS
442	198	50	100	78.1	71736	PASS
443	442	15	24	19.9	14299	PASS