
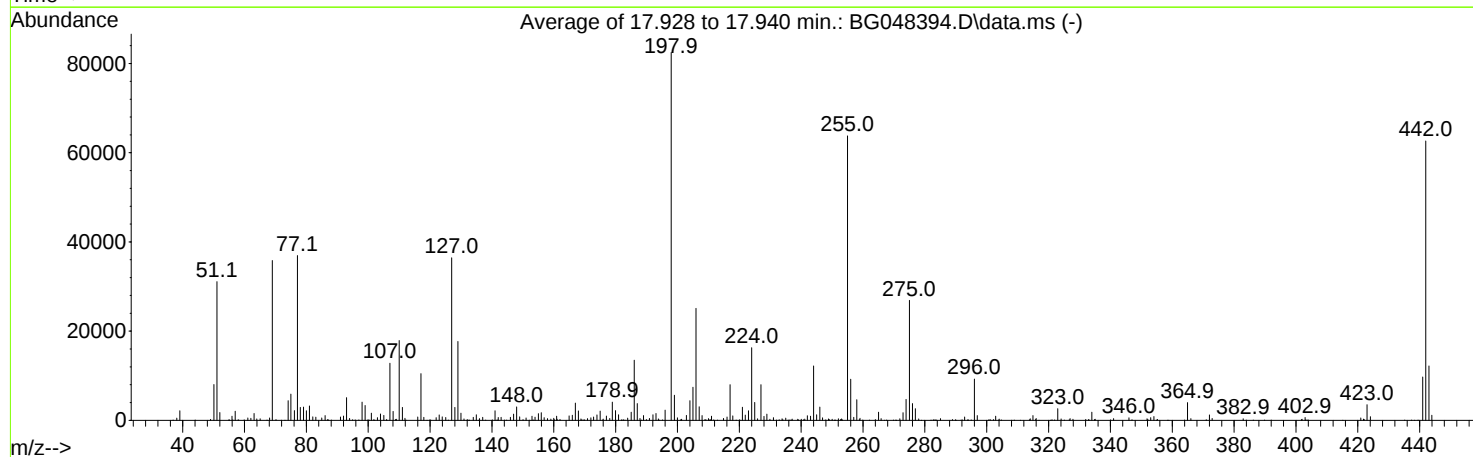


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031721\
 Data File : BG048394.D
 Acq On : 17 Mar 2021 12:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 16 16:05:10 2021

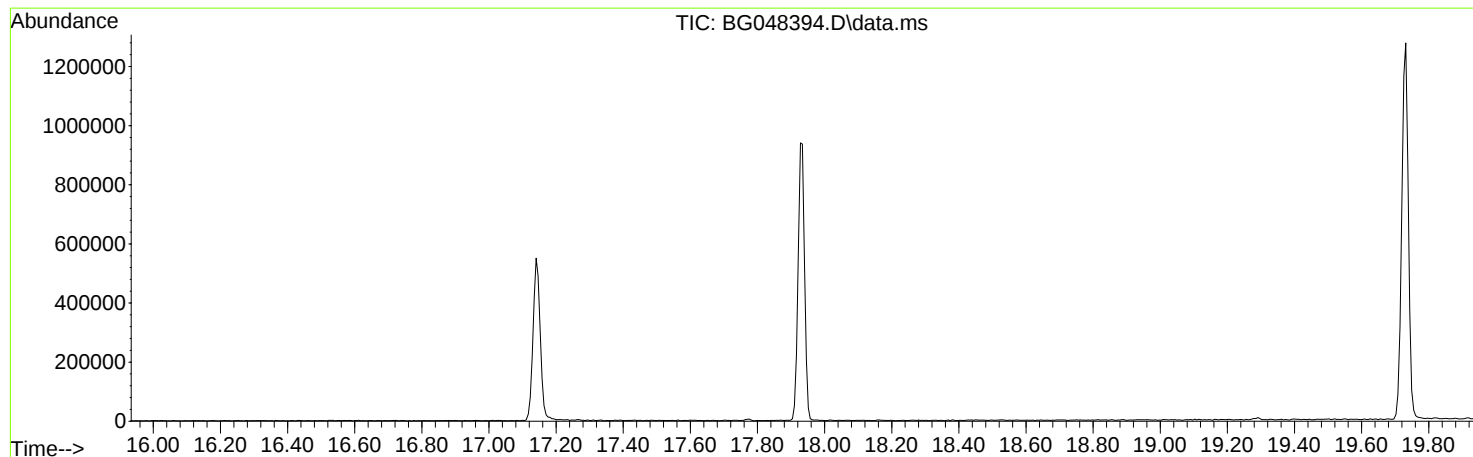

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	31099	PASS
68	69	0.00	2	1.5	546	PASS
69	198	0.00	100	43.5	35840	PASS
70	69	0.00	2	0.5	170	PASS
127	198	10	80	44.2	36453	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82475	PASS
199	198	5	9	6.8	5629	PASS
275	198	10	60	32.6	26893	PASS
365	198	1	100	4.8	3986	PASS
441	198	0.01	100	11.8	9714	PASS
442	198	50	100	76.0	62648	PASS
443	442	15	24	19.5	12203	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2021	BNA_G	<u>BG048394..D</u>
Compound Name	Response	Retention Time
DDT	309583	20.779
DDD	3720	20.344
DDE	523	16.971
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4243	313826	1.35

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031721\
Data File : BG048394.D
Acq On : 17 Mar 2021 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 17 13:09:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 16 16:05:10 2021
Response via : Initial Calibration

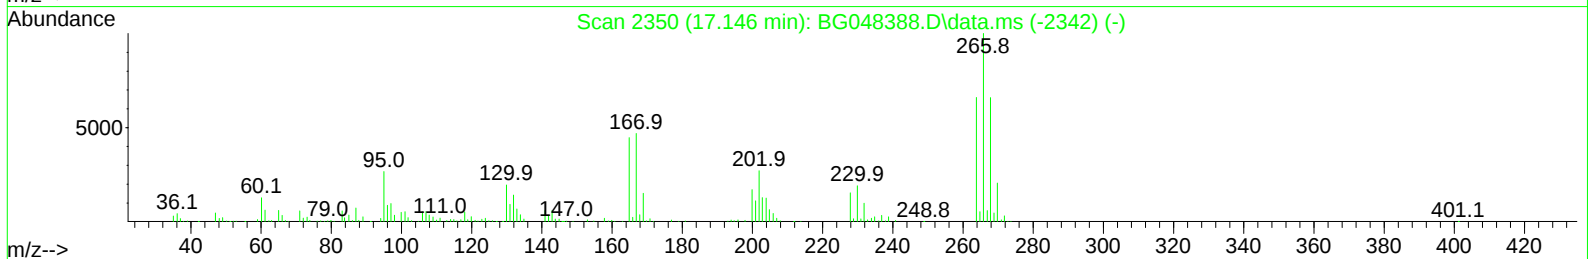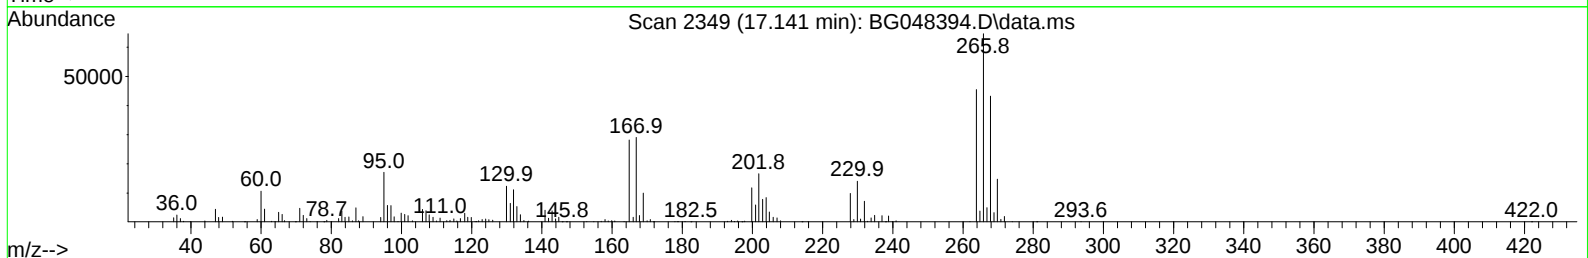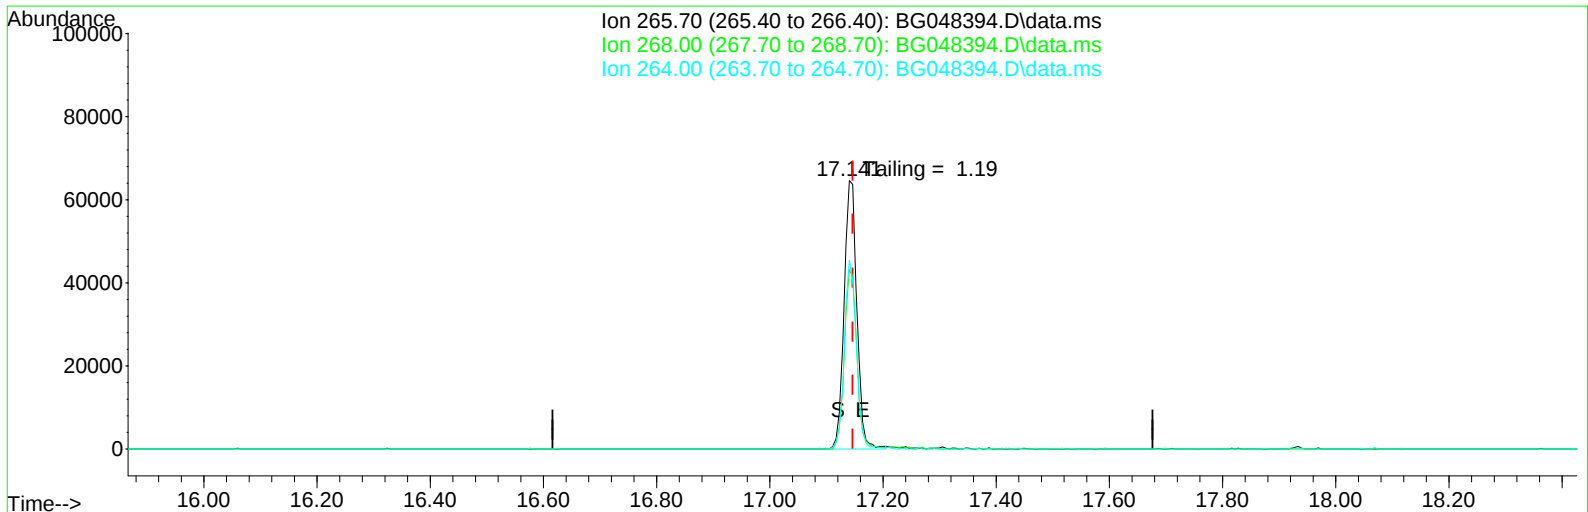

TIC: BG048394.D\data.ms

(70) Pentachlorophenol (C)

17.141min (-0.005) 225311.60 ng




response 100691

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.87
264.00	61.60	70.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031721\
Data File : BG048394.D
Acq On : 17 Mar 2021 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 17 13:09:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 16 16:05:10 2021
Response via : Initial Calibration

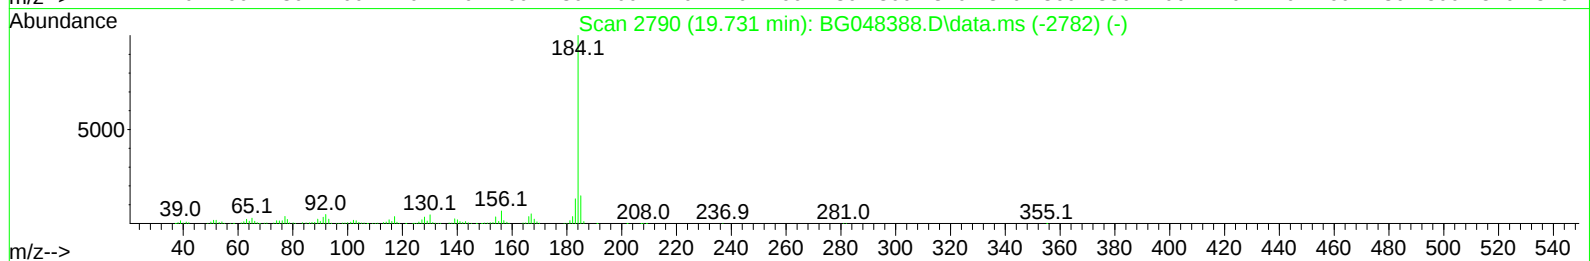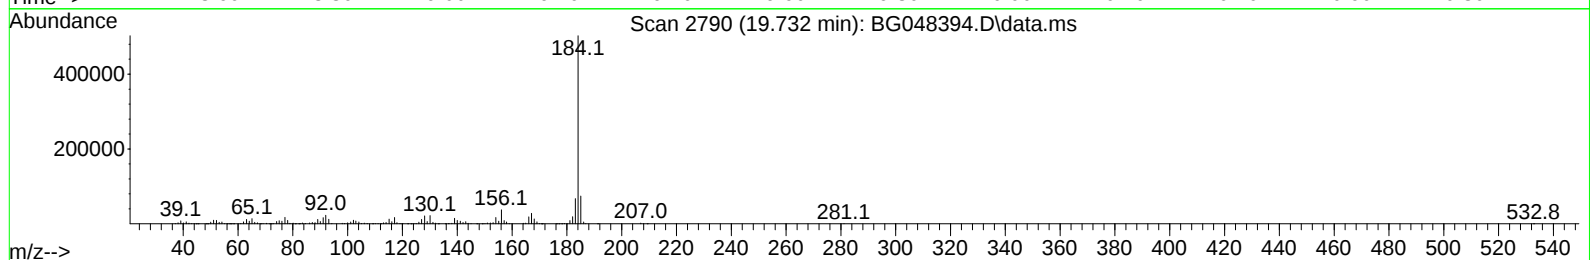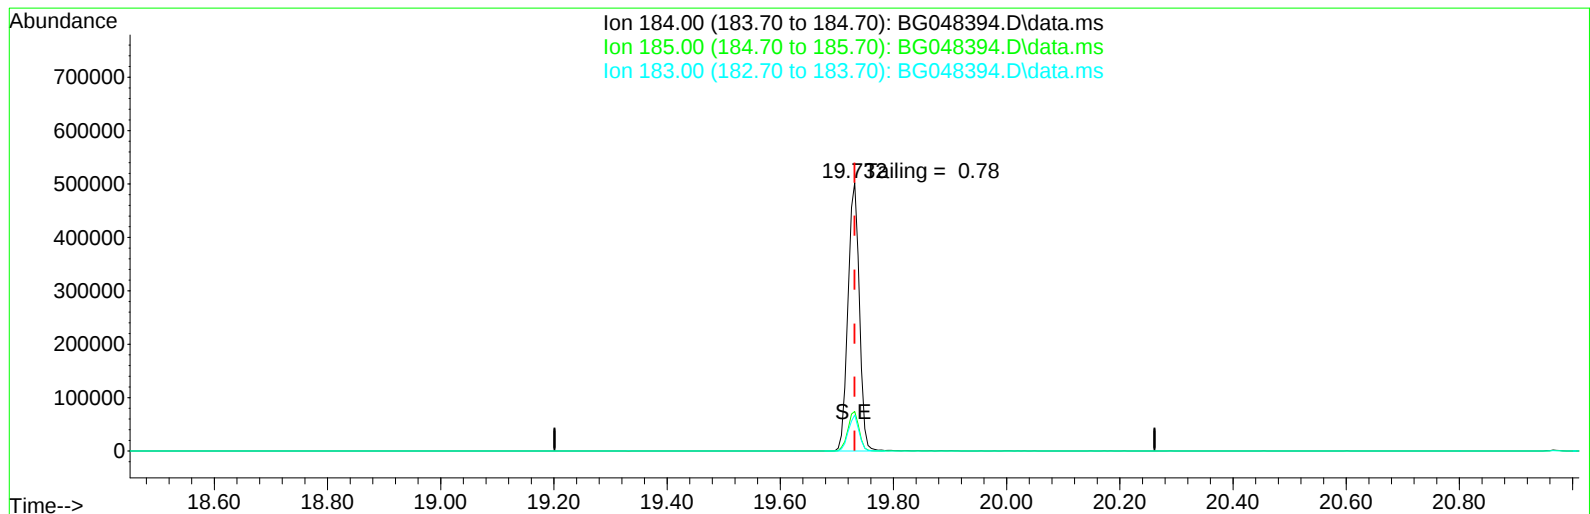

TIC: BG048394.D\data.ms

(77) Benzidine

19.732min (+ 0.001) 386956.45 ng

response 701920

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.76
183.00	13.20	13.42
0.00	0.00	0.00