

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
 Data File : BG052686.D
 Acq On : 17 Mar 2022 10:13
 Operator : CG/JU
 Sample : PB143208BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143208BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.709	387	395	407	rBV	854148	1351522	33.96%	8.982%
2	7.301	657	666	674	rBV	833566	1468307	36.89%	9.758%
3	8.153	804	811	819	rVB	170737	291152	7.32%	1.935%
4	9.310	1000	1008	1018	rBV	495477	914654	22.98%	6.078%
5	10.967	1282	1290	1299	rVB	217762	404295	10.16%	2.687%
6	13.404	1697	1705	1714	rVB	1319809	2166081	54.43%	14.395%
7	14.773	1931	1938	1945	rVB	362430	568378	14.28%	3.777%
8	16.254	2183	2190	2200	rBV	970087	1432179	35.99%	9.518%
9	17.517	2398	2405	2413	rBV	476371	739702	18.59%	4.916%
10	20.125	2842	2849	2854	rVB	2905216	3979866	100.00%	26.449%
11	21.805	3129	3135	3143	rVB	537472	893798	22.46%	5.940%
12	25.124	3691	3700	3710	rVB2	279443	837531	21.04%	5.566%




Sum of corrected areas: 15047465

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
Data File : BG052686.D
Acq On : 17 Mar 2022 10:13
Operator : CG/JU
Sample : PB143208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

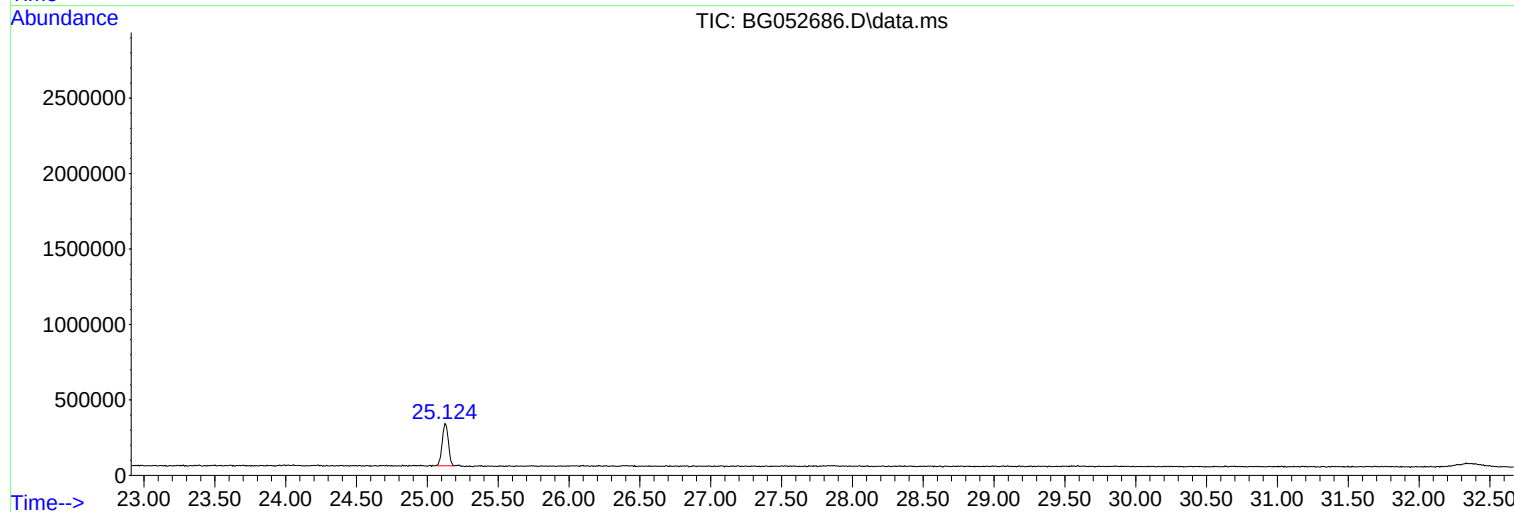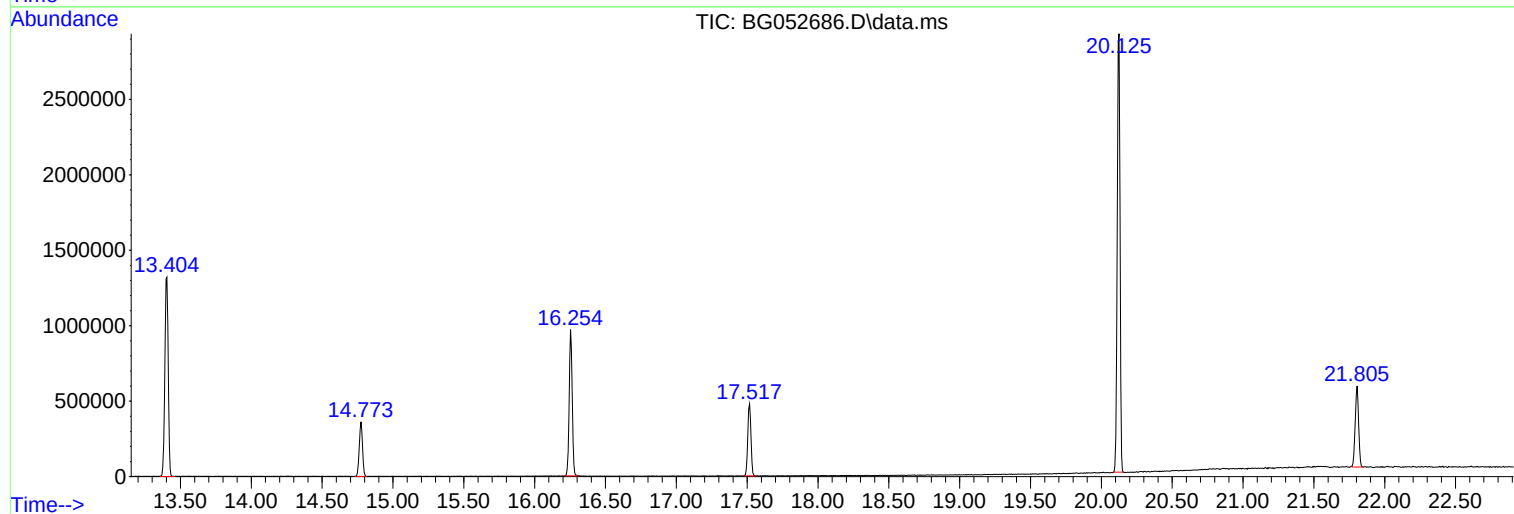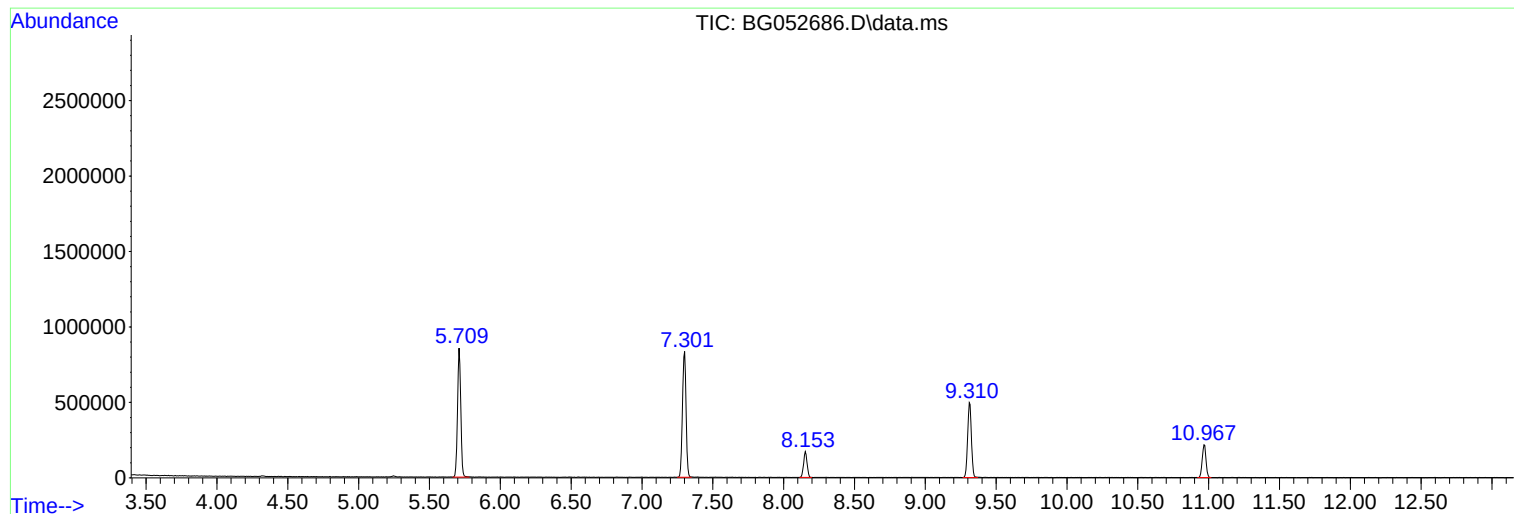

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
Data File : BG052686.D
Acq On : 17 Mar 2022 10:13
Operator : CG/JU
Sample : PB143208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
Data File : BG052686.D
Acq On : 17 Mar 2022 10:13
Operator : CG/JU
Sample : PB143208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------