
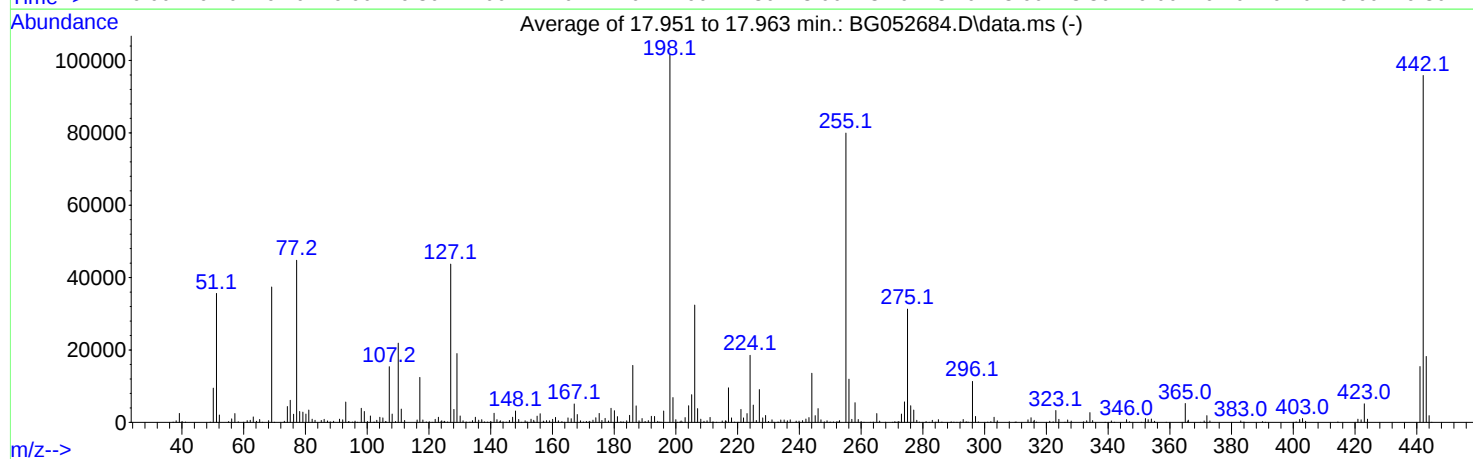


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
 Data File : BG052684.D
 Acq On : 17 Mar 2022 8:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 15 15:56:10 2022

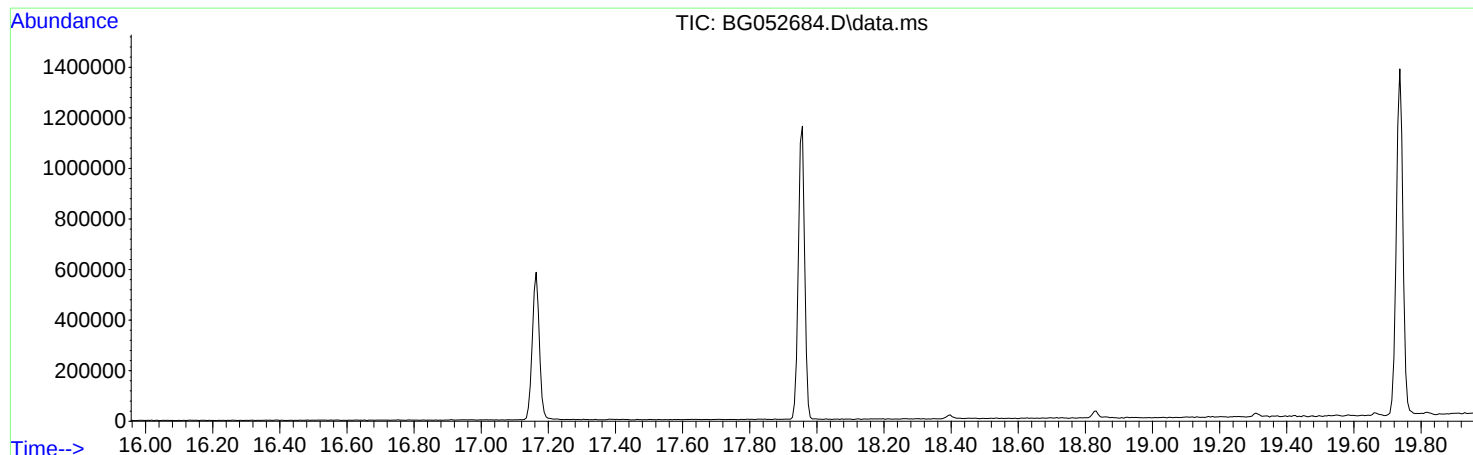




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	35619	PASS
68	69	0.00	2	1.3	470	PASS
69	198	0.00	100	36.8	37416	PASS
70	69	0.00	2	0.1	35	PASS
127	198	10	80	43.0	43749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101651	PASS
199	198	5	9	6.7	6843	PASS
275	198	10	60	30.8	31296	PASS
365	198	1	100	5.1	5218	PASS
441	198	0.01	100	15.2	15418	PASS
442	442	50	100	100.0	95845	PASS
443	442	15	24	19.0	18203	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
Data File : BG052684.D
Acq On : 17 Mar 2022 8:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 17 15:42:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 15 15:56:10 2022
Response via : Initial Calibration

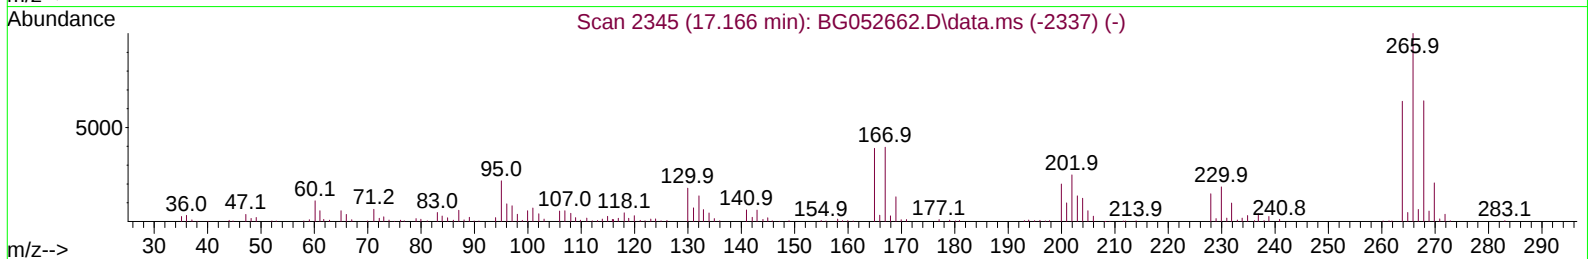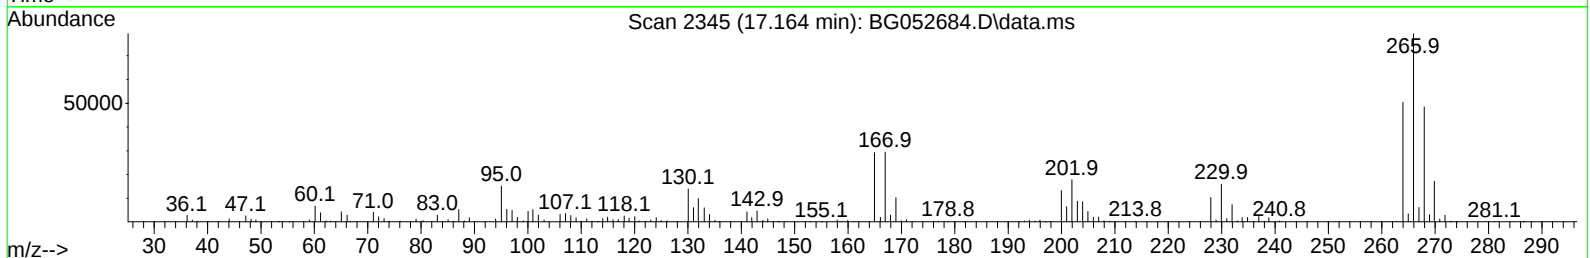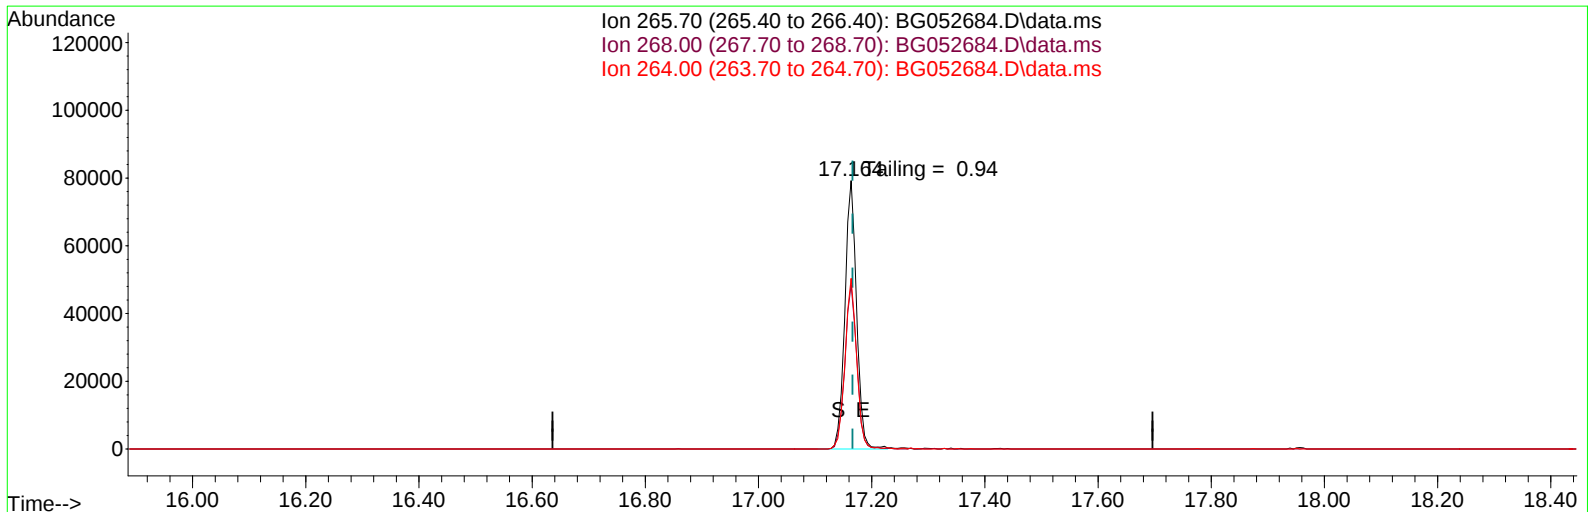

TIC: BG052684.D\data.ms

(70) Pentachlorophenol (C)

17.164min (-0.002) 21035.25 ng




response 112630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.14
264.00	56.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031722\
 Data File : BG052684.D
 Acq On : 17 Mar 2022 8:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 15:42:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 15 15:56:10 2022
 Response via : Initial Calibration

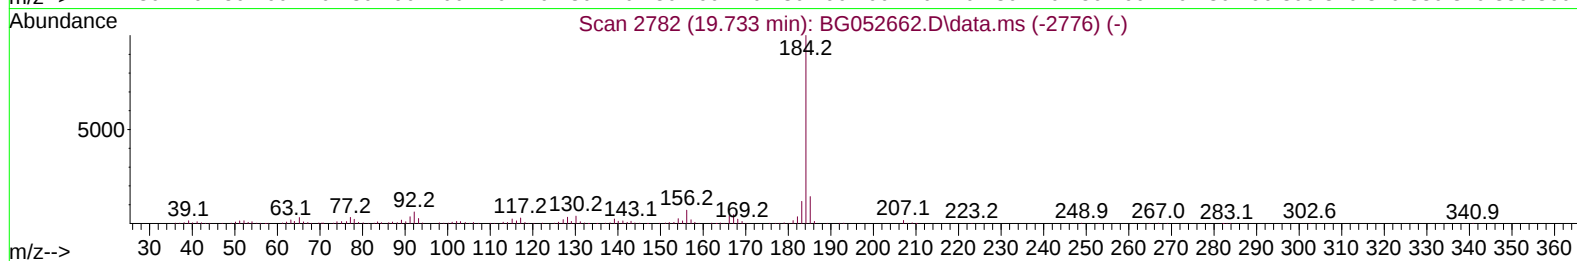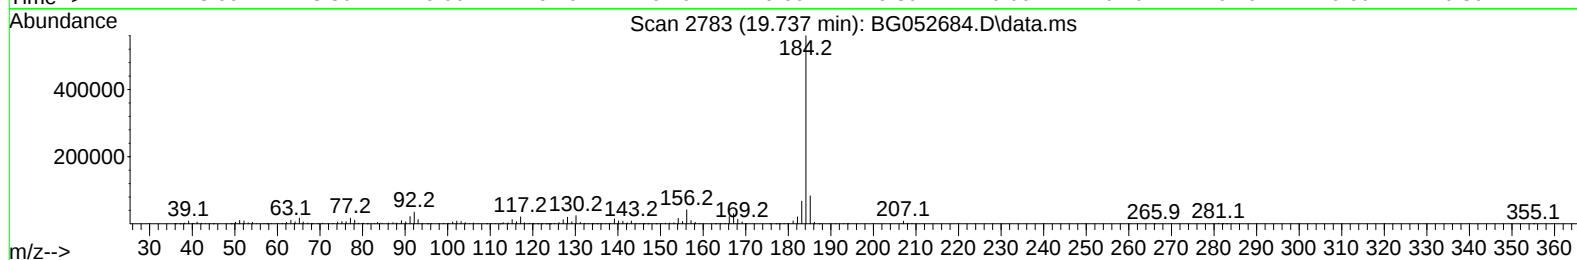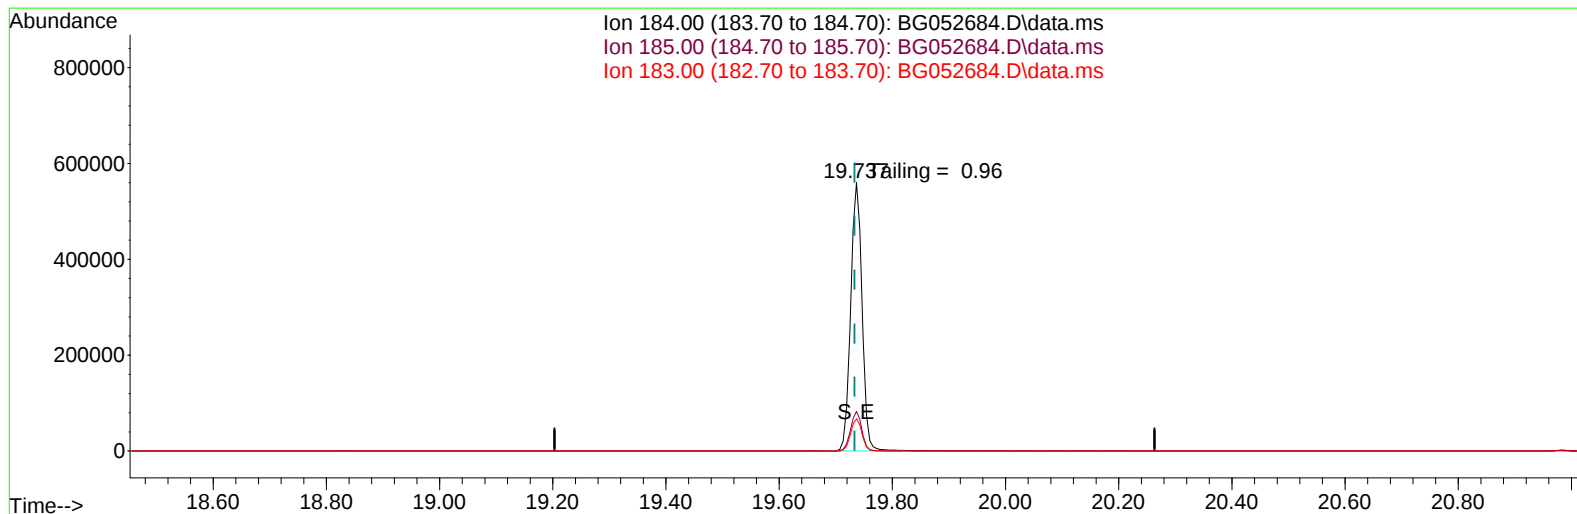

TIC: BG052684.D\data.ms

(77) Benzidine

19.737min (+ 0.004) 0.00 ng

response 780286

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.80
183.00	11.80	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2022	BNA_G	<u>BG052684.D</u>
Compound Name	Response	Retention Time
DDT	338313	20.98
DDD	2354	20.53
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2354	340667	0.69

Instrument :
BNA_G
ClientSampleId :
DFTPP