
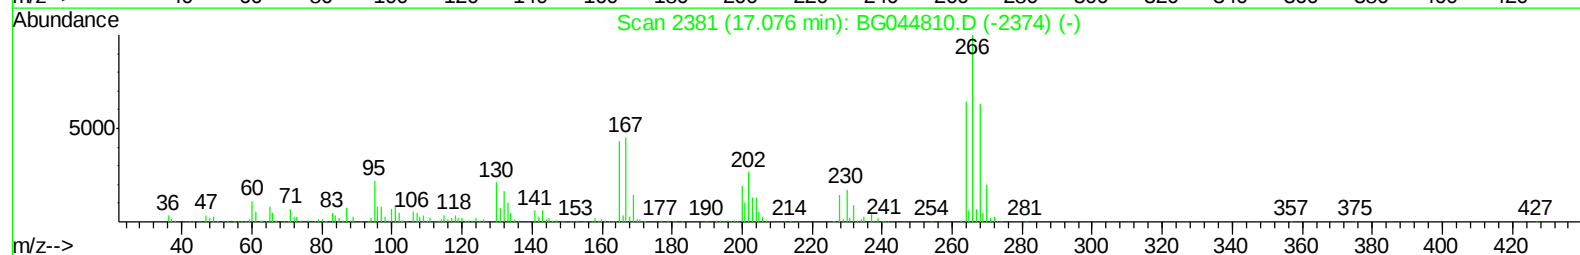
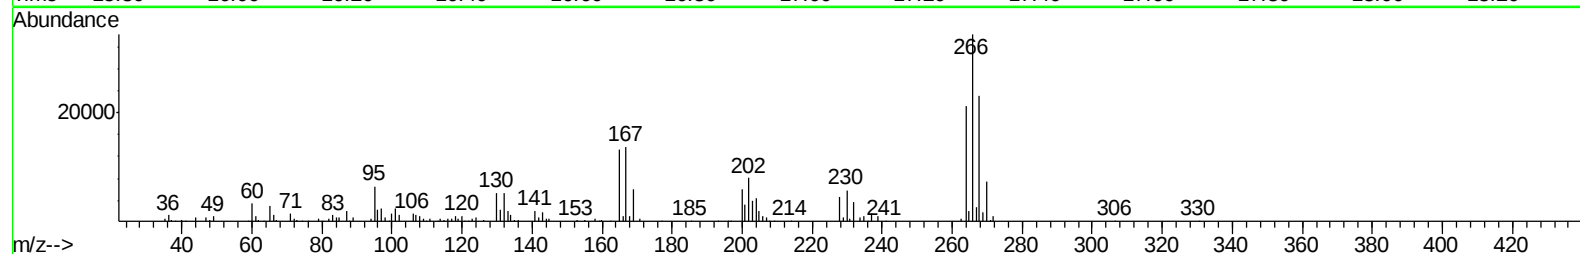


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031820\
Data File : BG044867.D
Acq On : 18 Mar 2020 16:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 04:15:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 17:37:15 2020
Response via : Initial Calibration

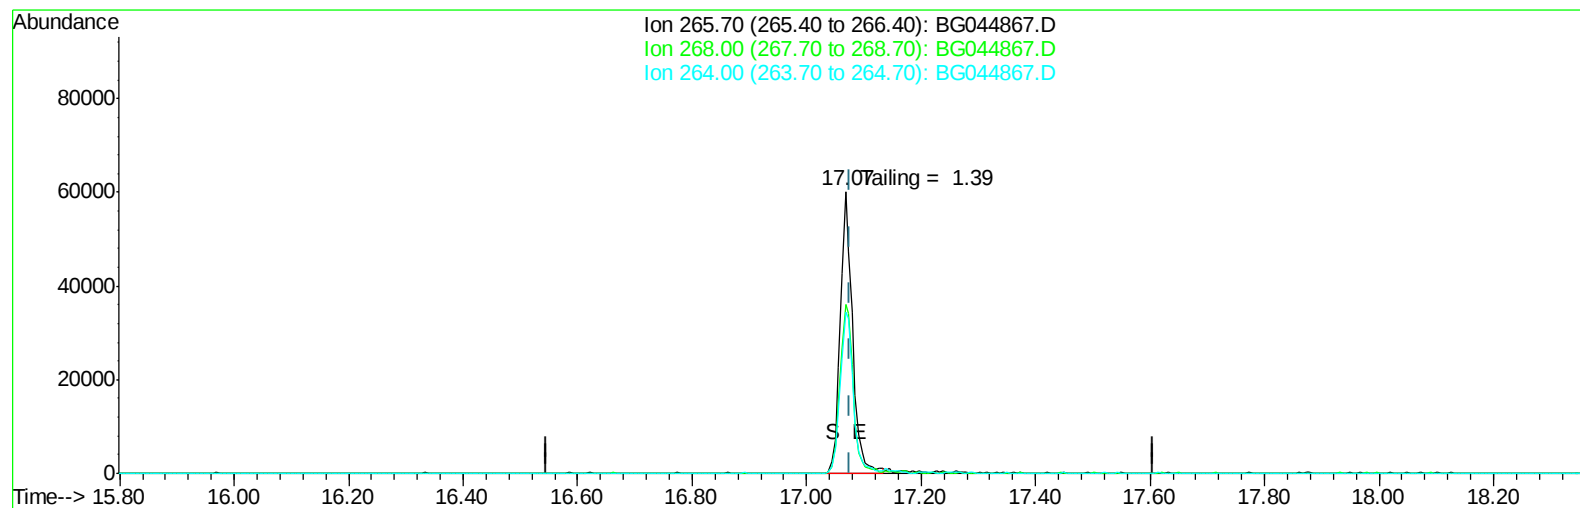

TIC: BG044867.D

(70) Pentachlorophenol (C)




17.068min (-0.009) 19534.46ng

response 90817

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	59.95
264.00	64.30	57.33
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031820\
 Data File : BG044867.D
 Acq On : 18 Mar 2020 16:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 04:15:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 17:37:15 2020
 Response via : Initial Calibration

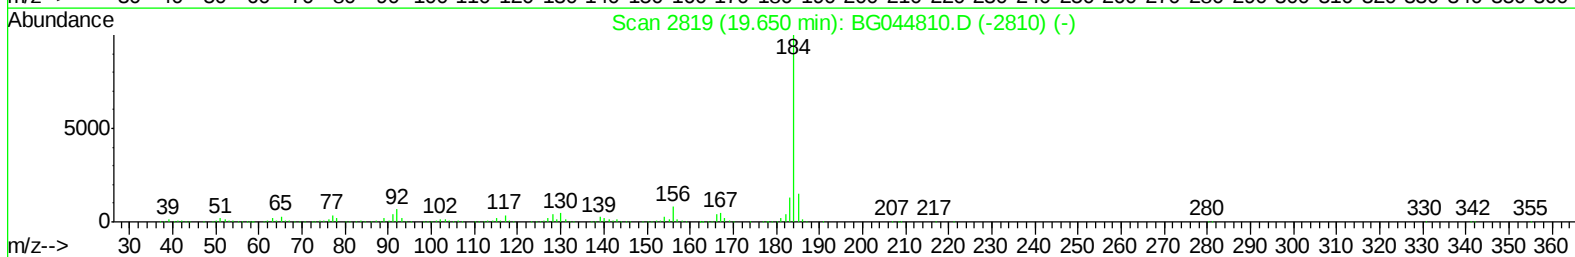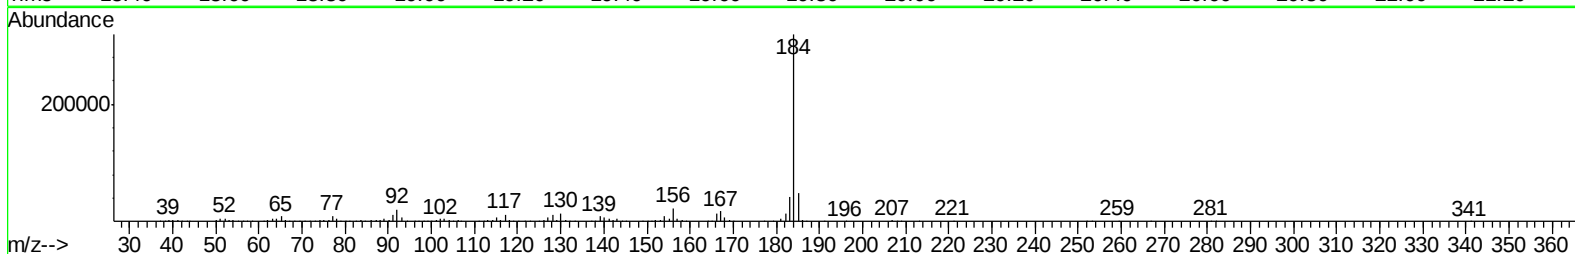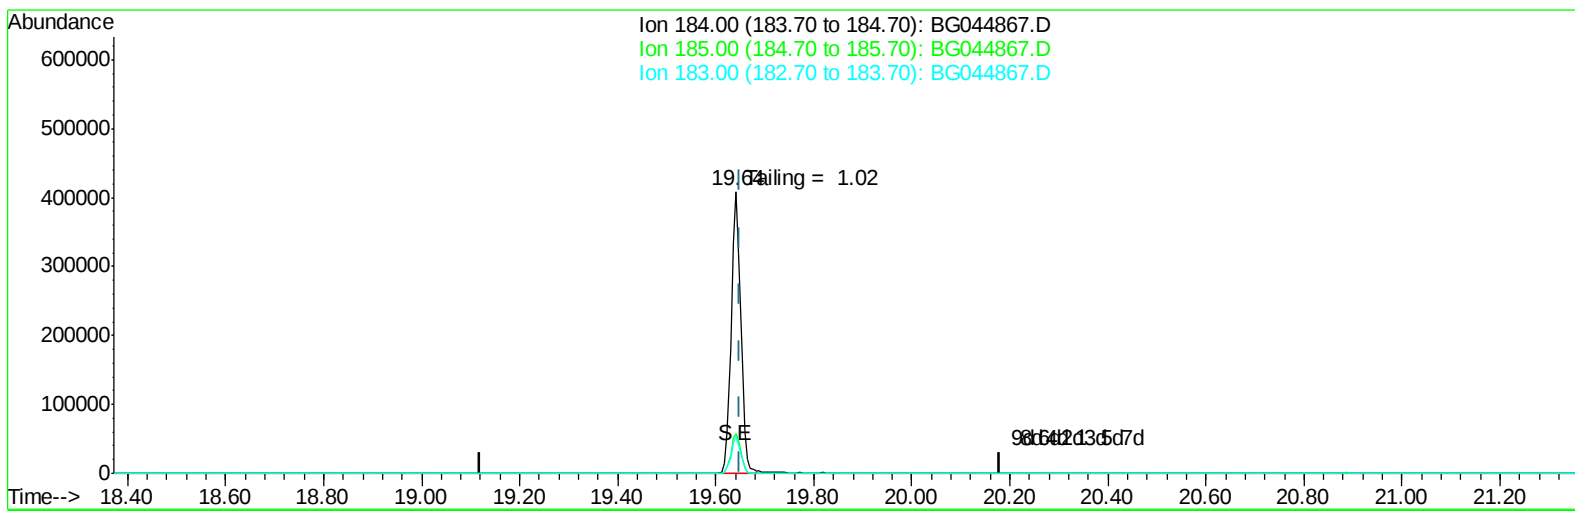

TIC: BG044867.D

(77) Benzidine

20.346min (+0.696) 96.52ng

response 188

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00