


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG031820\
 Data File : BG044867.D
 Acq On : 18 Mar 2020 16:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 17:37:15 2020

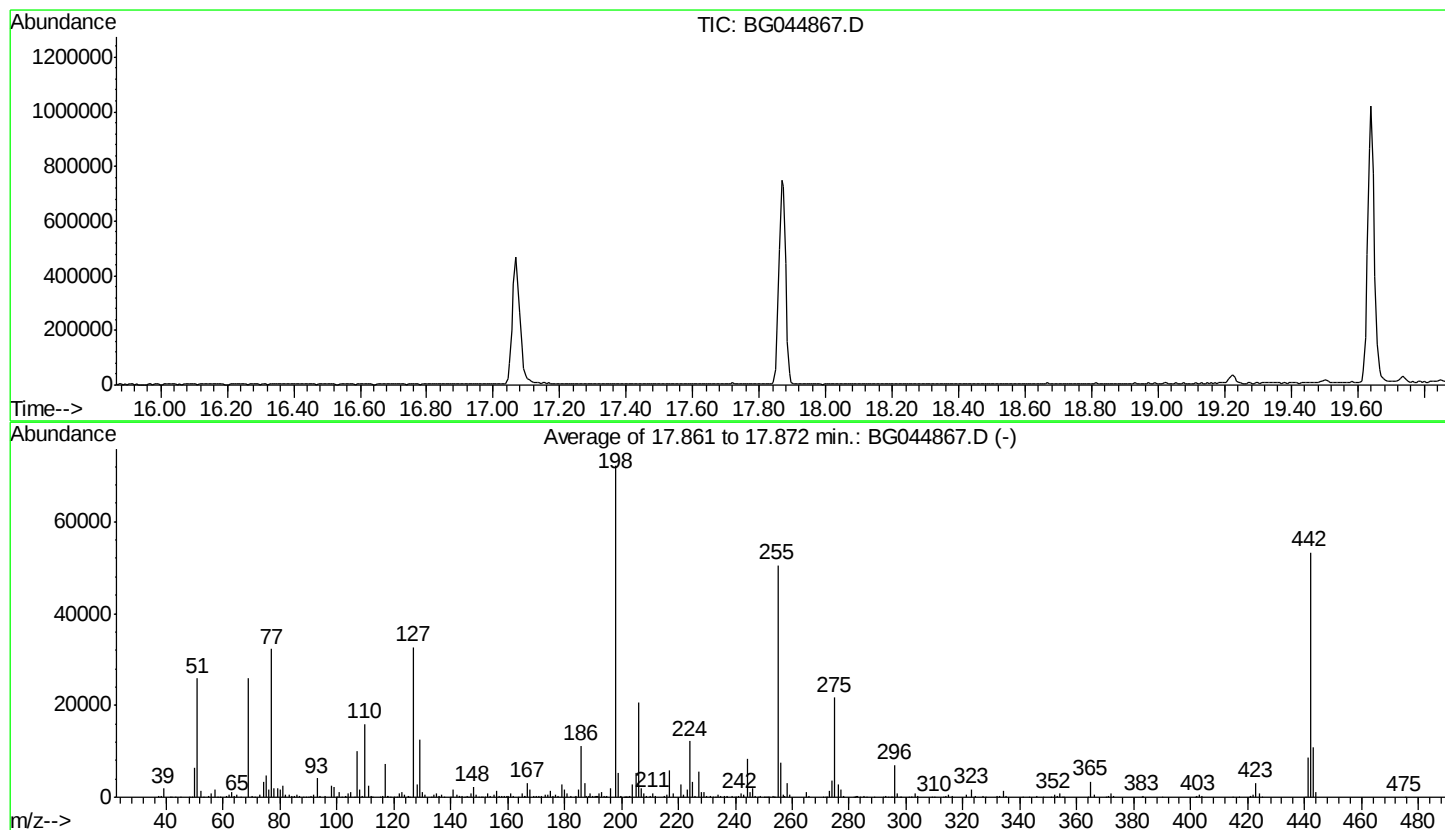

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	25821	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.0	26002	PASS
70	69	0.00	2	1.1	298	PASS
127	198	10	80	45.3	32720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72210	PASS
199	198	5	9	7.4	5312	PASS
275	198	10	60	30.1	21707	PASS
365	198	1	100	4.8	3442	PASS
441	198	0.01	100	12.0	8665	PASS
442	198	50	100	73.8	53301	PASS
443	442	15	24	20.3	10834	PASS