


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG031820\
 Data File : BG044885.D
 Acq On : 19 Mar 2020 5:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 17:37:15 2020

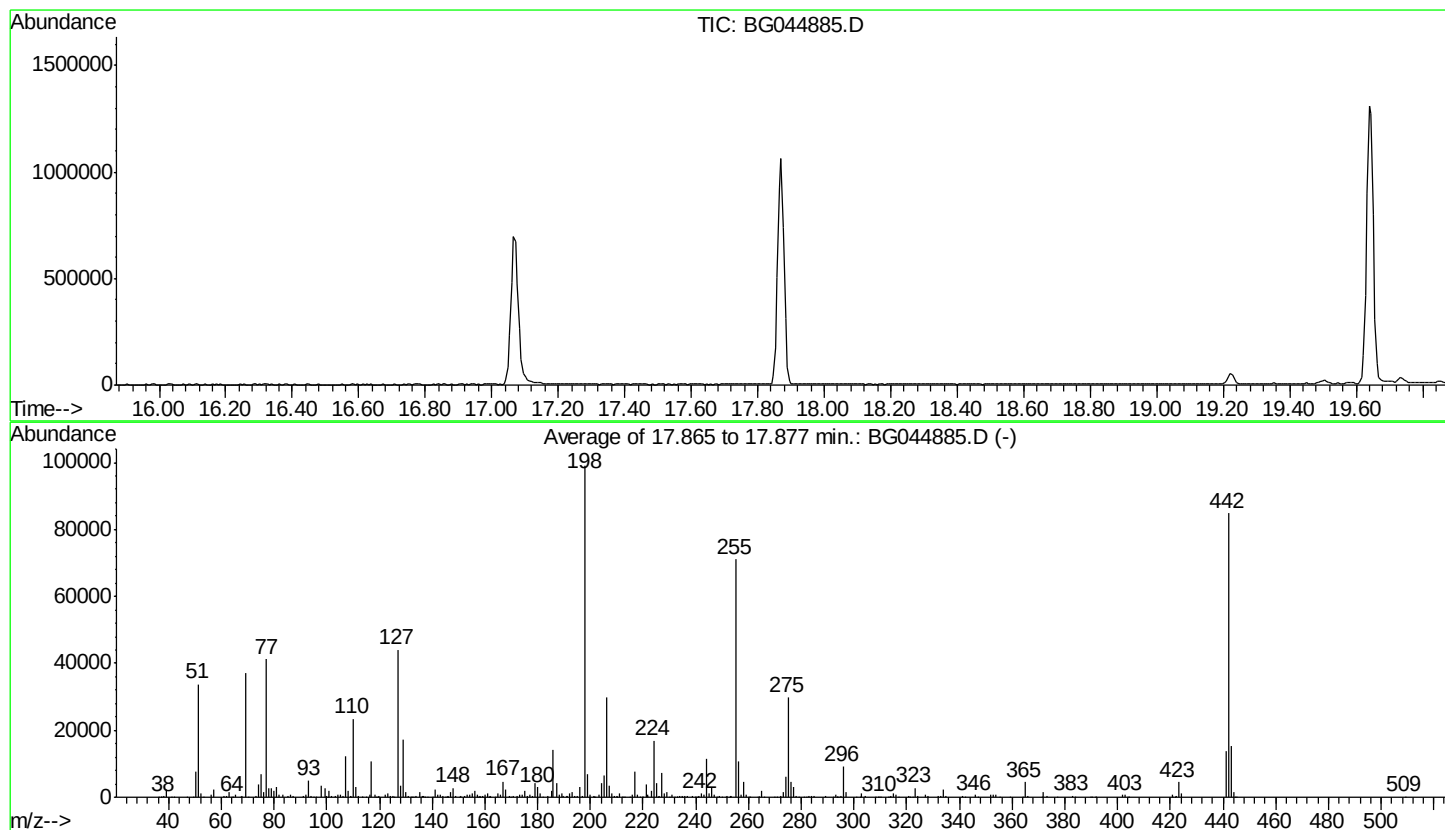

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	33754	PASS
68	69	0.00	2	1.5	539	PASS
69	198	0.00	100	37.3	36936	PASS
70	69	0.00	2	0.3	123	PASS
127	198	10	80	44.5	44080	PASS
197	198	0.00	2	0.4	371	PASS
198	198	100	100	100.0	99061	PASS
199	198	5	9	7.0	6977	PASS
275	198	10	60	30.1	29800	PASS
365	198	1	100	4.6	4572	PASS
441	198	0.01	100	14.1	13931	PASS
442	198	50	100	85.7	84869	PASS
443	442	15	24	18.0	15304	PASS