




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG031822\  
Data File : BG052708.D  
Acq On : 18 Mar 2022 13:47  
Operator : CG/JU  
Sample : N1882-09  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DBRX9

Manual IntegrationsAPPROVED

Quant Time: Mar 18 23:59:31 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Mar 18 00:55:42 2022  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022  
Supervised By :Yogesh Patel 03/24/2022

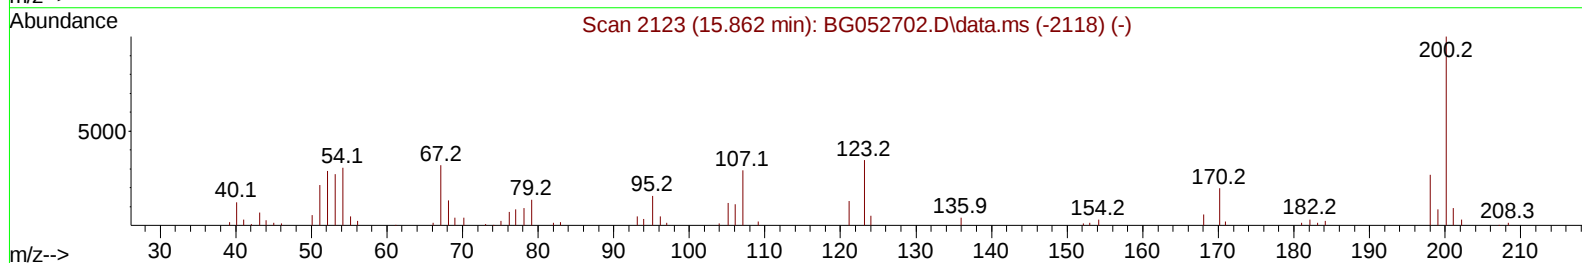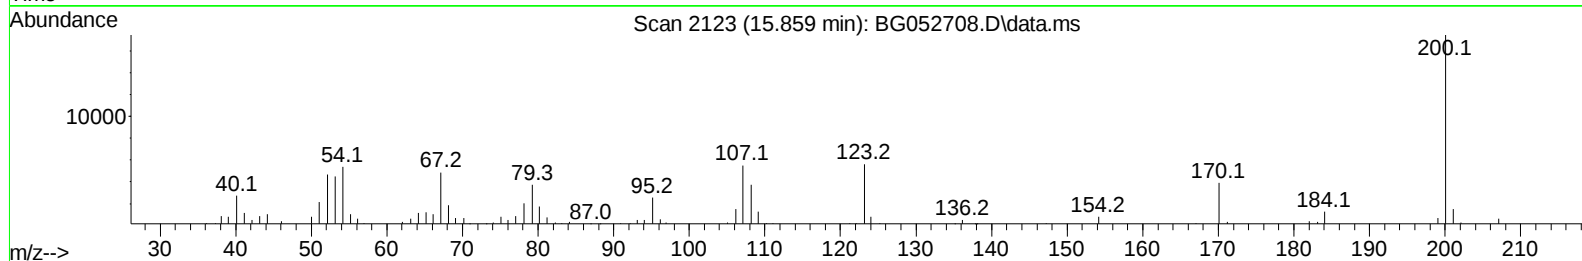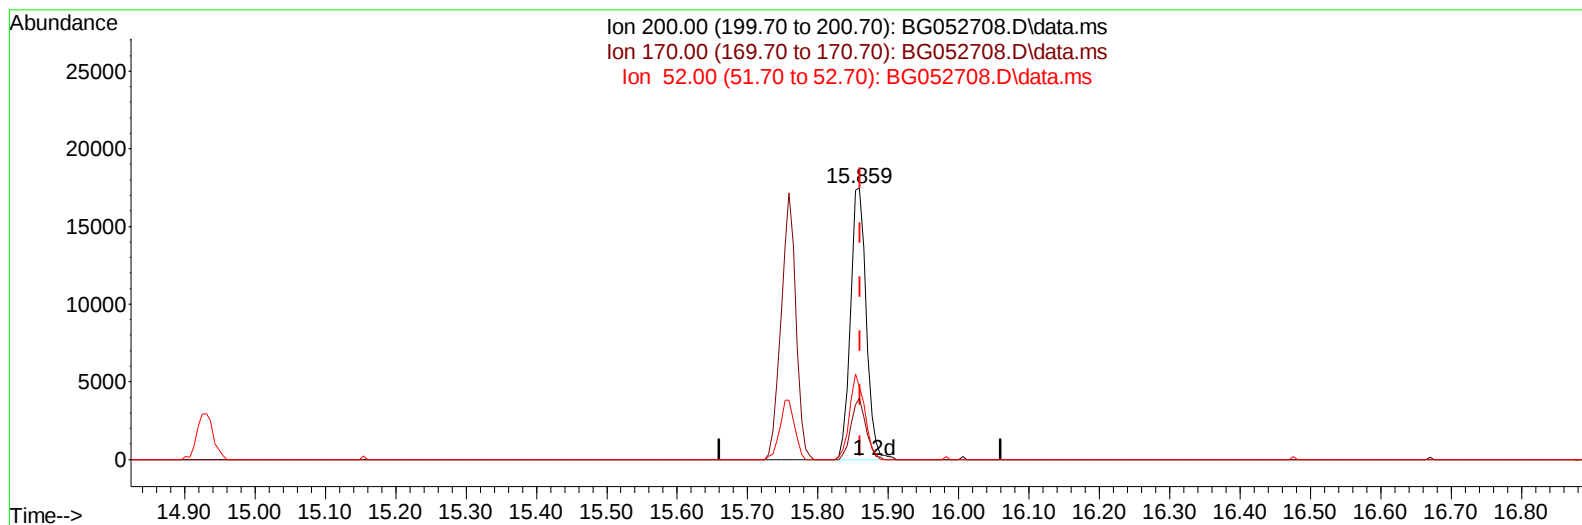

TIC: BG052708.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.859min (-0.001) 18.67 ng/u1

response 26716

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 200.00 | 100.00 | 100.00 |
| 170.00 | 20.70  | 22.51  |
| 52.00  | 31.80  | 26.66  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG031822\  
 Data File : BG052708.D  
 Acq On : 18 Mar 2022 13:47  
 Operator : CG/JU  
 Sample : N1882-09  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DBRX9

Manual IntegrationsAPPROVED

Quant Time: Mar 18 23:59:31 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Mar 18 00:55:42 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022  
 Supervised By :Yogesh Patel 03/24/2022

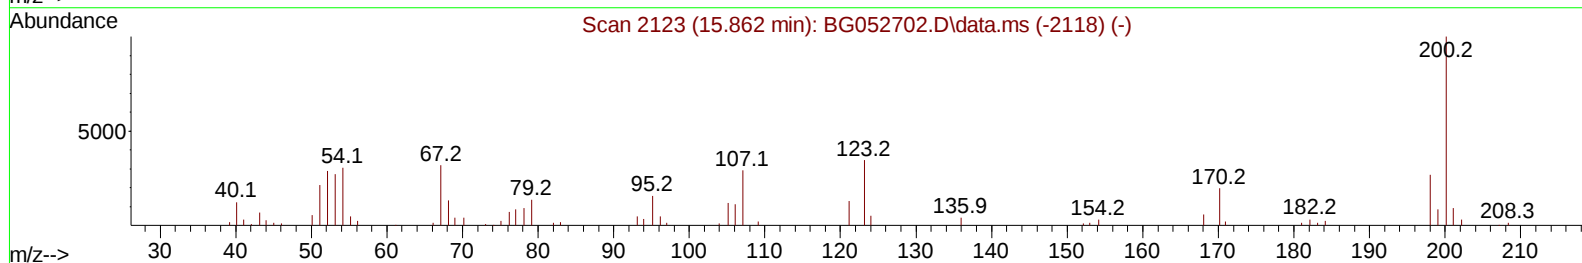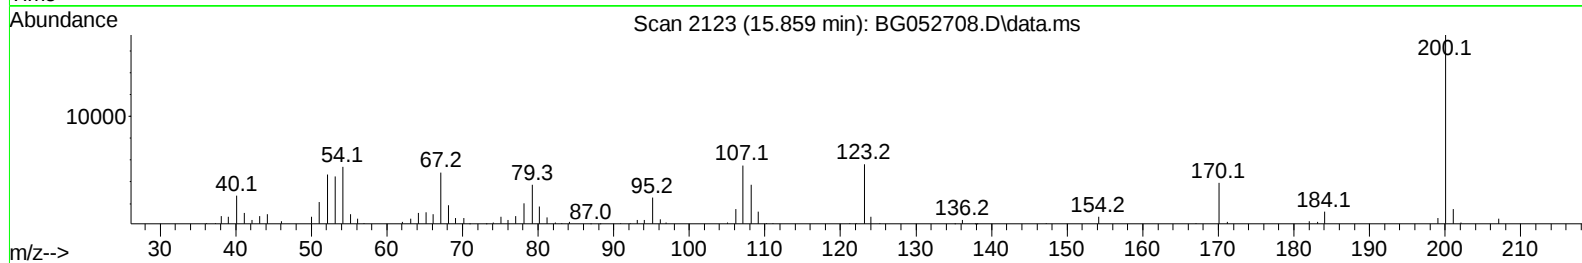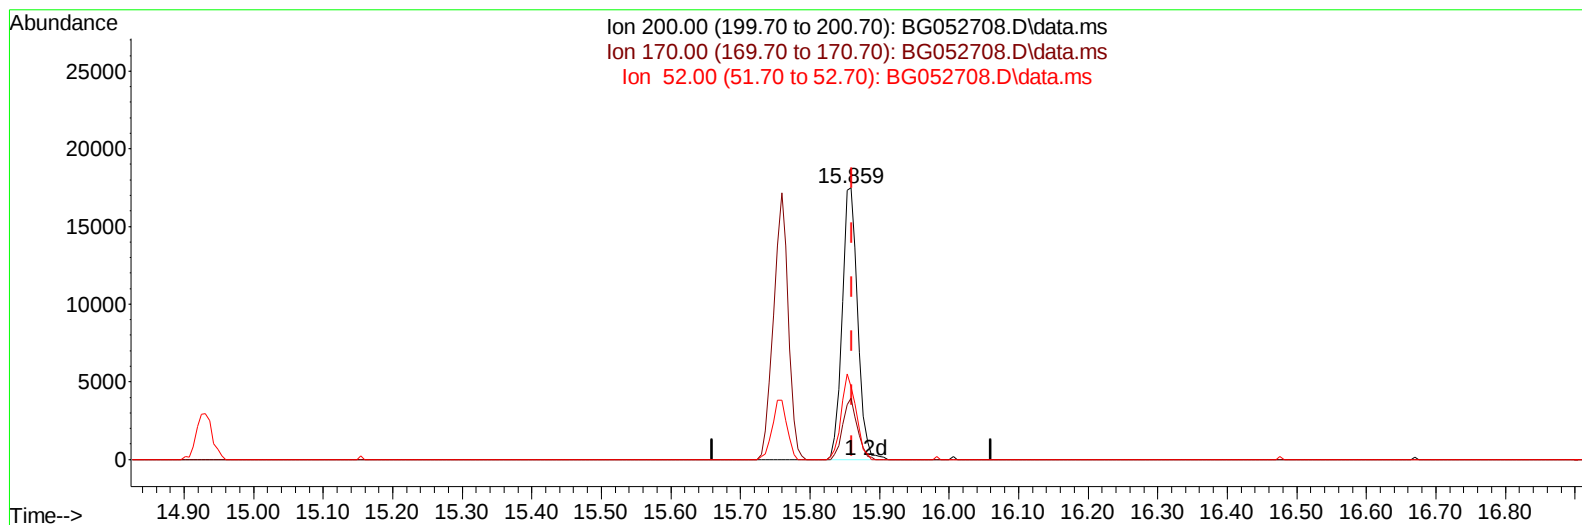

TIC: BG052708.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.859min (-0.001) 18.82 ng/ul m

response 26931

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 200.00 | 100.00 | 100.00 |
| 170.00 | 20.70  | 22.51  |
| 52.00  | 31.80  | 26.66  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG031822\  
 Data File : BG052708.D  
 Acq On : 18 Mar 2022 13:47  
 Operator : CG/JU  
 Sample : N1882-09  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DBRX9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022  
 Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 18 23:59:31 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Mar 18 00:55:42 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| -----                         |        |      |          |        |       |          |
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.152  | 152  | 42885    | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.966 | 136  | 169791   | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.766 | 164  | 120358   | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.510 | 188  | 281200   | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.798 | 240  | 304047   | 20.000 | ng/ul | 0.00     |
| 88) Perylene-d12              | 25.117 | 264  | 296643   | 20.000 | ng/ul | 0.00     |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.564  | 96   | 5721     | 4.712  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.981  | 84   | 70092    | 23.125 | ng/ul | 0.00     |
| 7) Phenol-d5                  | 7.288  | 99   | 97724    | 25.442 | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.464  | 67   | 60184    | 25.655 | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.682  | 132  | 65097    | 24.960 | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.839  | 113  | 69106    | 24.837 | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 9.309  | 128  | 32983    | 26.986 | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 10.032 | 143  | 34461    | 26.732 | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.572 | 165  | 69037    | 24.616 | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.083 | 131  | 92542    | 24.966 | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 14.167 | 166  | 241477   | 26.116 | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 14.461 | 160  | 290126   | 25.822 | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.931 | 143  | 33778    | 21.728 | ng/ul | 0.00     |
| 60) Fluorene-d10              | 15.759 | 176  | 209950   | 25.860 | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.859 | 200  | 26931m   | 18.819 | ng/ul | 0.00     |
| 73) Anthracene-d10            | 17.610 | 188  | 344947   | 26.343 | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.889 | 212  | 437523   | 25.723 | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 24.888 | 264  | 403273   | 26.310 | ng/ul | 0.00     |

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG031822\  
Data File : BG052708.D  
Acq On : 18 Mar 2022 13:47  
Operator : CG/JU  
Sample : N1882-09  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DBRX9

Manual IntegrationsAPPROVED

Quant Time: Mar 18 23:59:31 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Mar 18 00:55:42 2022  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022  
Supervised By :Yogesh Patel 03/24/2022

