




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052711.D
Acq On : 18 Mar 2022 15:44
Operator : CG/JU
Sample : N1882-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRY0

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

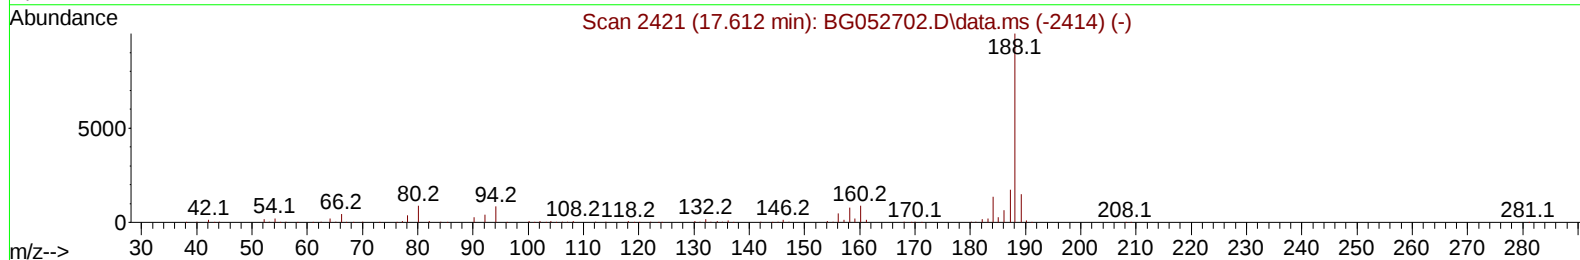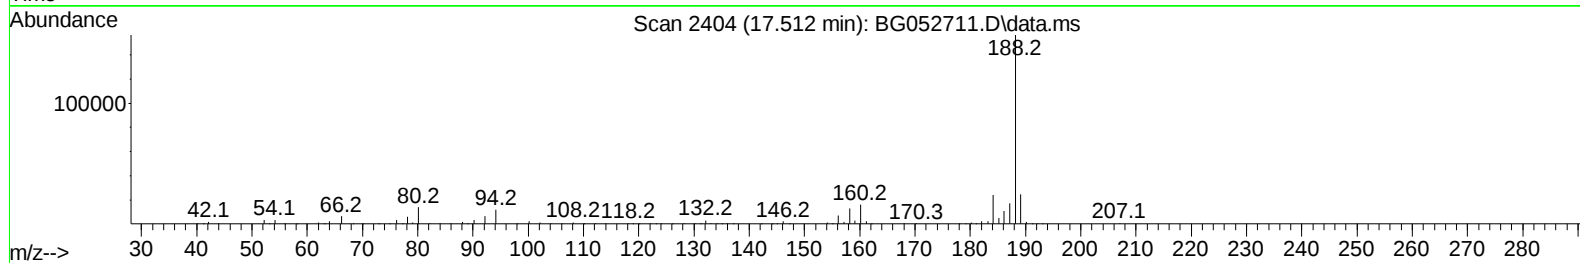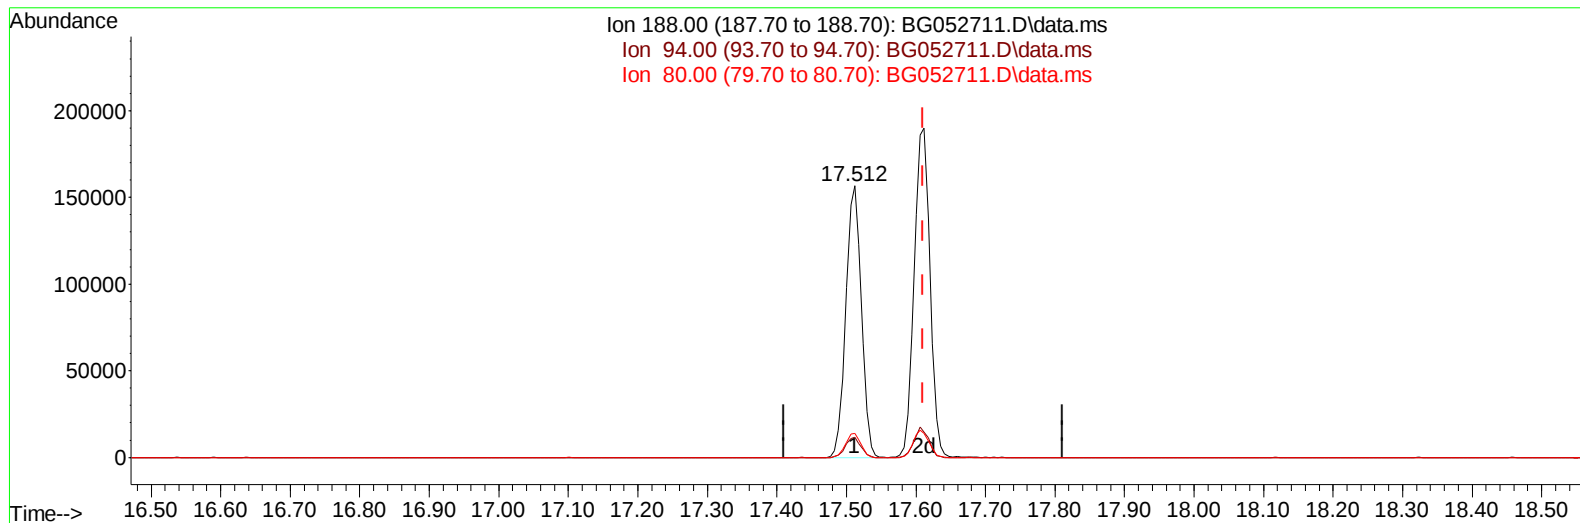

TIC: BG052711.D\data.ms

(73) Anthracene-d10 (S)

17.512min (-0.099) 21.47 ng/u1

response 242952

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	7.46
80.00	9.50	8.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052711.D
 Acq On : 18 Mar 2022 15:44
 Operator : CG/JU
 Sample : N1882-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY0

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

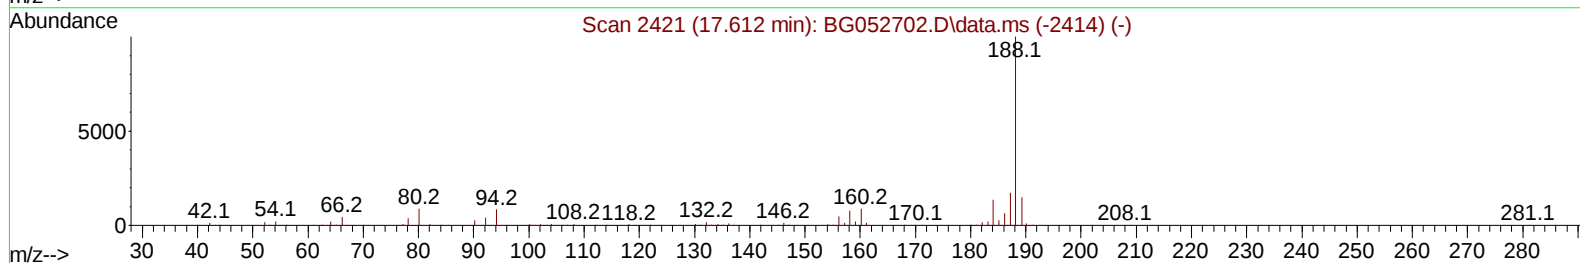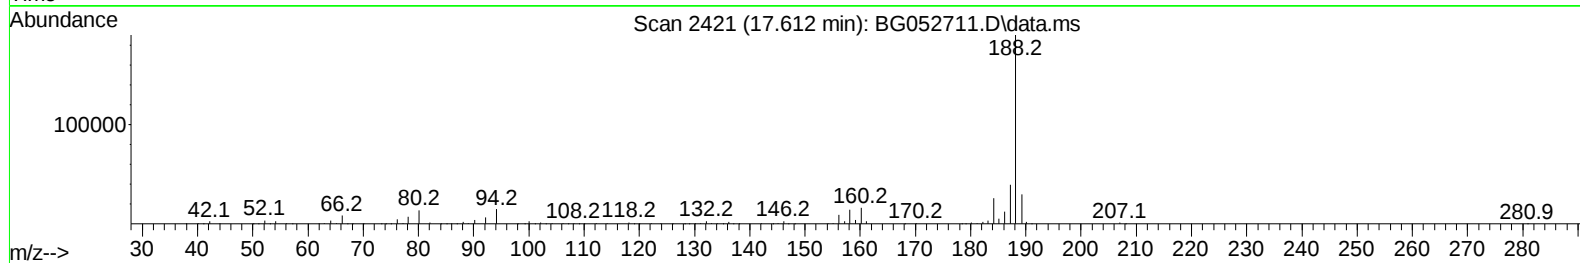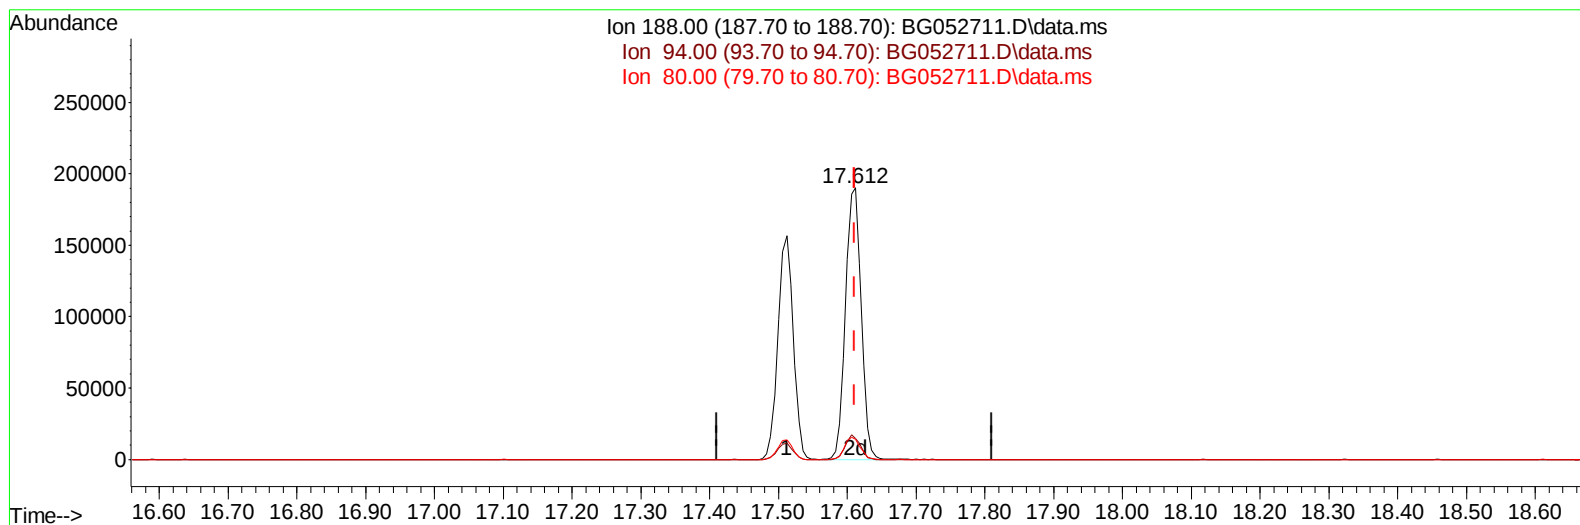

TIC: BG052711.D\data.ms

(73) Anthracene-d10 (S)

17.612min (+ 0.001) 26.64 ng/ul m

response 301407

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	7.79
80.00	9.50	7.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052711.D
 Acq On : 18 Mar 2022 15:44
 Operator : CG/JU
 Sample : N1882-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY0

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.148	152	36909	20.000	ng/ul	0.00
20) Naphthalene-d8	10.962	136	143657	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	102552	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.512	188	242952	20.000	ng/ul	0.00
79) Chrysene-d12	21.795	240	256671	20.000	ng/ul	-0.01
88) Perylene-d12	25.119	264	256963	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.566	96	4363	4.176	ng/uL	0.00
4) Pyridine-d5	3.983	84	60447	23.172	ng/ul	0.00
7) Phenol-d5	7.291	99	83635	25.300	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.467	67	51275	25.396	ng/ul	0.00
11) 2-Chlorophenol-d4	7.678	132	58381	26.009	ng/ul	0.00
15) 4-Methylphenol-d8	8.841	113	60312	25.186	ng/ul	0.00
21) Nitrobenzene-d5	9.306	128	29379	28.410	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	29326	26.887	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	61155	25.773	ng/ul	0.00
31) 4-Chloroaniline-d4	11.085	131	82279	26.236	ng/ul	0.00
46) Dimethylphthalate-d6	14.164	166	203951	25.887	ng/ul	0.00
49) Acenaphthylene-d8	14.463	160	249814	26.094	ng/ul	0.00
54) 4-Nitrophenol-d4	14.927	143	29706	22.426	ng/ul	0.00
60) Fluorene-d10	15.756	176	180119	26.037	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.855	200	24647	19.935	ng/ul	0.00
73) Anthracene-d10	17.612	188	301407m	26.642	ng/ul	0.00
81) Pyrene-d10	19.891	212	376805	26.242	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.884	264	357580	26.932	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052711.D
Acq On : 18 Mar 2022 15:44
Operator : CG/JU
Sample : N1882-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRY0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 19 00:00:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

