




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052713.D
 Acq On : 18 Mar 2022 17:02
 Operator : CG/JU
 Sample : N1882-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY5

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

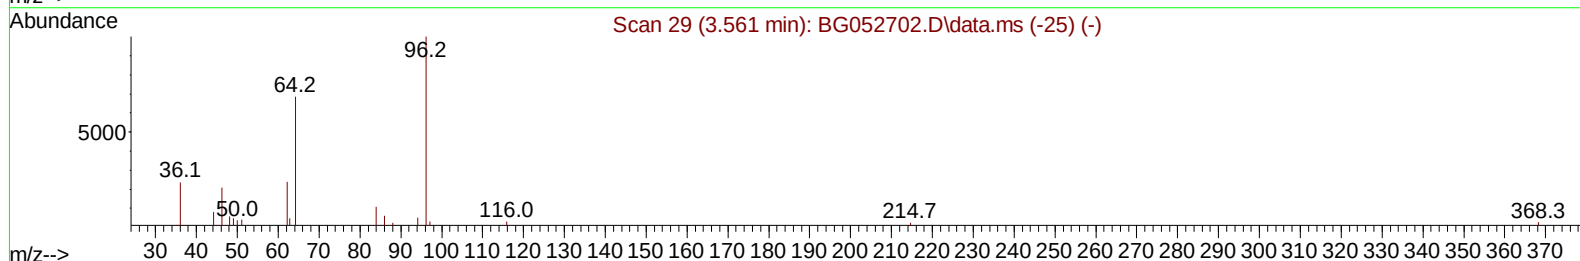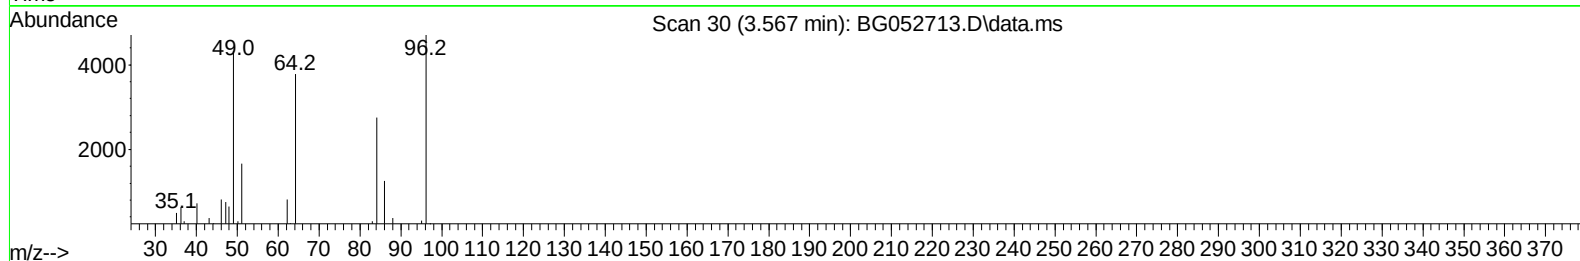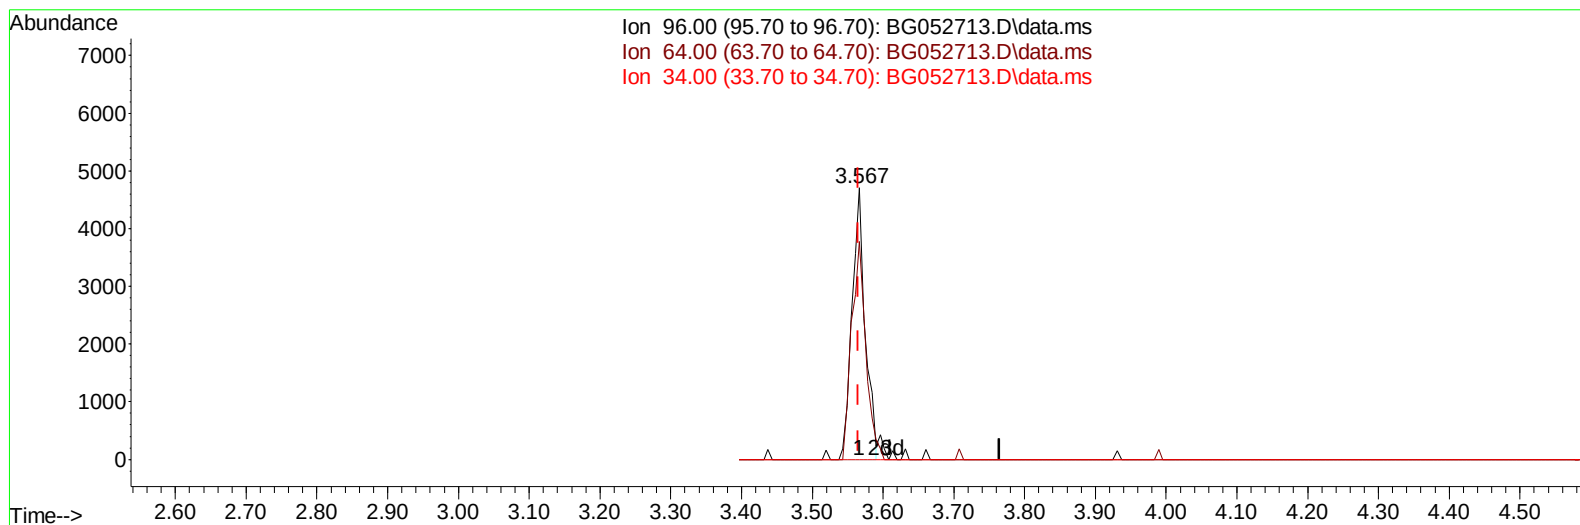

TIC: BG052713.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.567min (+ 0.002) 5.32 ng/uL

response 6079

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	80.26
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052713.D
 Acq On : 18 Mar 2022 17:02
 Operator : CG/JU
 Sample : N1882-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY5

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

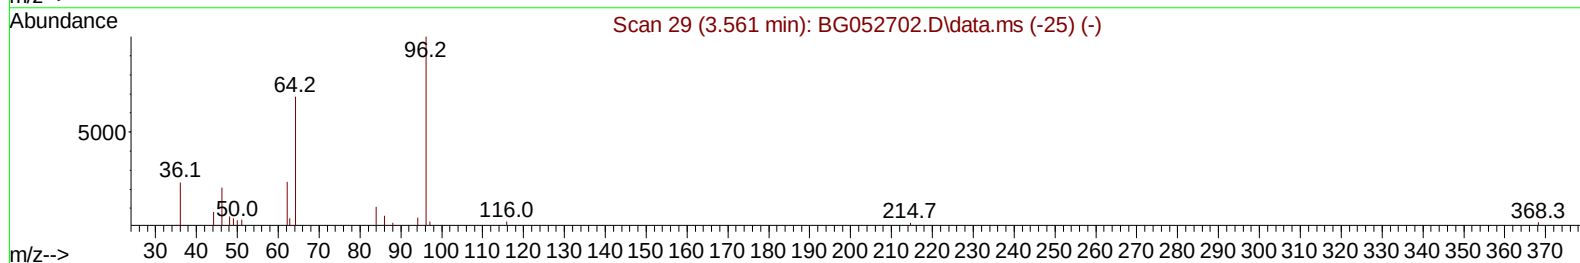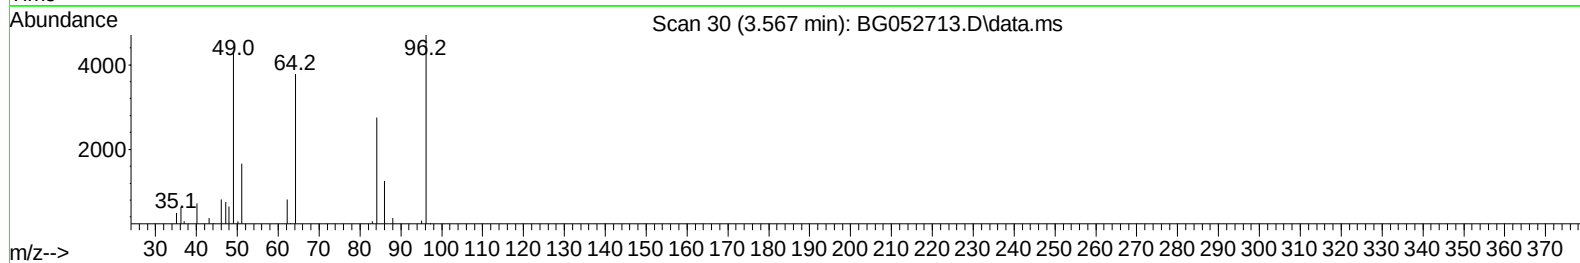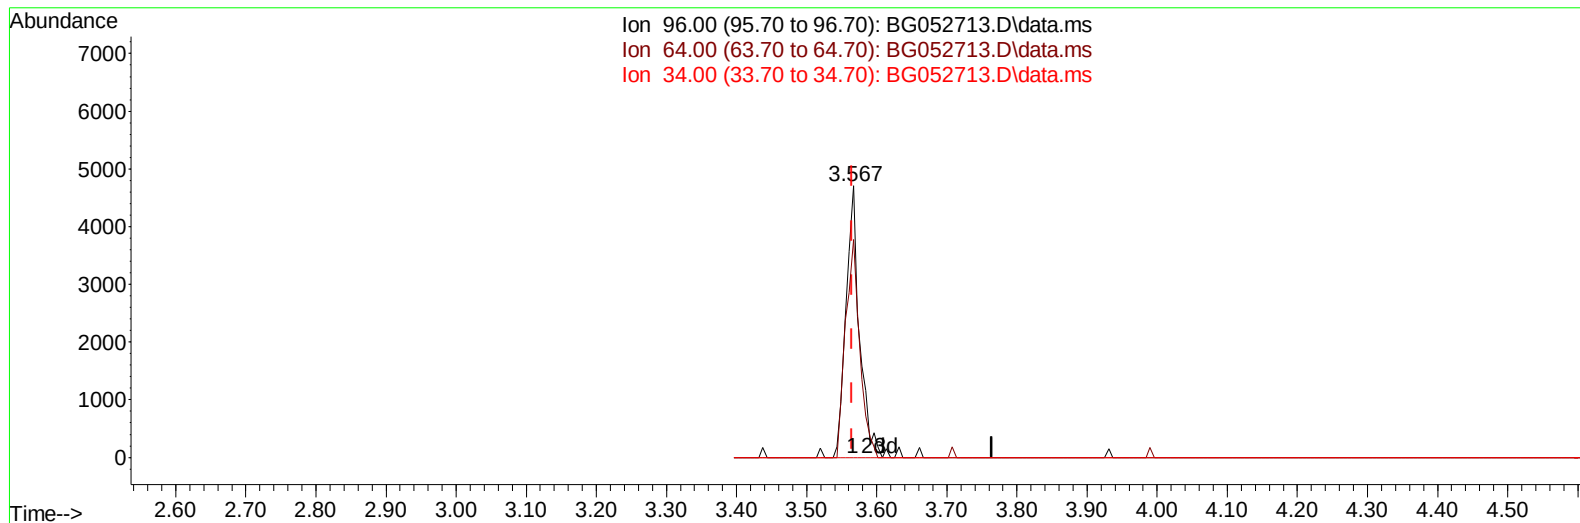

TIC: BG052713.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.567min (+ 0.002) 5.51 ng/uL m

response 6297

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	80.26
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052713.D
 Acq On : 18 Mar 2022 17:02
 Operator : CG/JU
 Sample : N1882-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 19 00:00:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.149	152	40373	20.000	ng/ul	0.00
20) Naphthalene-d8	10.963	136	160455	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	115990	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.513	188	265921	20.000	ng/ul	0.00
79) Chrysene-d12	21.795	240	287863	20.000	ng/ul	0.00
88) Perylene-d12	25.120	264	280326	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.567	96	6297m	5.509	ng/uL	0.00
4) Pyridine-d5	3.984	84	73779	25.856	ng/ul	0.00
7) Phenol-d5	7.291	99	107211	29.649	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.467	67	66243	29.995	ng/ul	0.00
11) 2-Chlorophenol-d4	7.679	132	71664	29.187	ng/ul	0.00
15) 4-Methylphenol-d8	8.842	113	78054	29.798	ng/ul	0.00
21) Nitrobenzene-d5	9.312	128	36673	31.751	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	37344	30.654	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.575	165	74397	28.071	ng/ul	0.00
31) 4-Chloroaniline-d4	11.086	131	103929	29.670	ng/ul	0.00
46) Dimethylphthalate-d6	14.164	166	253801	28.482	ng/ul	0.00
49) Acenaphthylene-d8	14.464	160	318388	29.404	ng/ul	0.00
54) 4-Nitrophenol-d4	14.928	143	39224	26.181	ng/ul	0.00
60) Fluorene-d10	15.756	176	228514	29.206	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.862	200	31868	23.549	ng/ul	0.00
73) Anthracene-d10	17.607	188	371710	30.018	ng/ul	0.00
81) Pyrene-d10	19.892	212	455573	28.290	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.891	264	423605	29.245	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052713.D
Acq On : 18 Mar 2022 17:02
Operator : CG/JU
Sample : N1882-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRY5

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

