




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052714.D
 Acq On : 18 Mar 2022 17:41
 Operator : CG/JU
 Sample : N1882-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY8

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

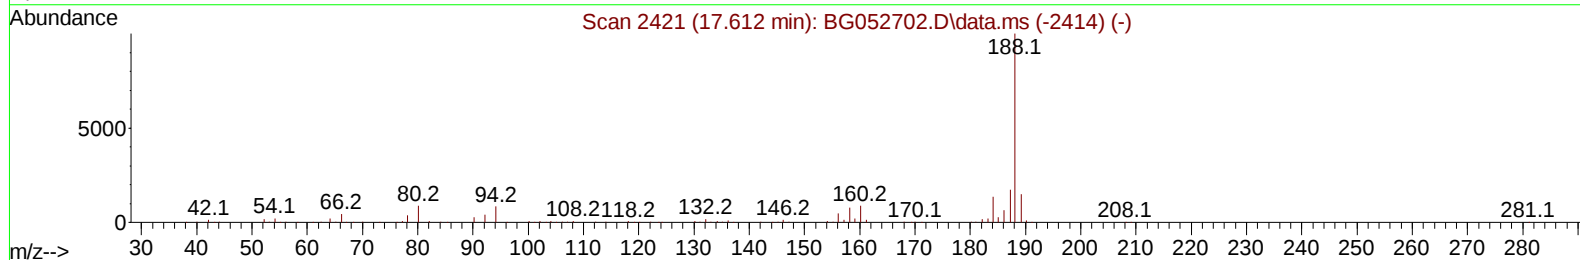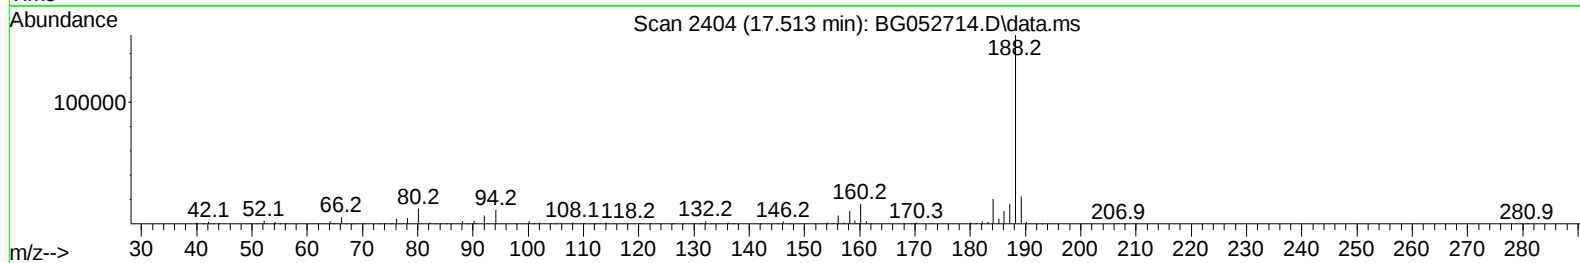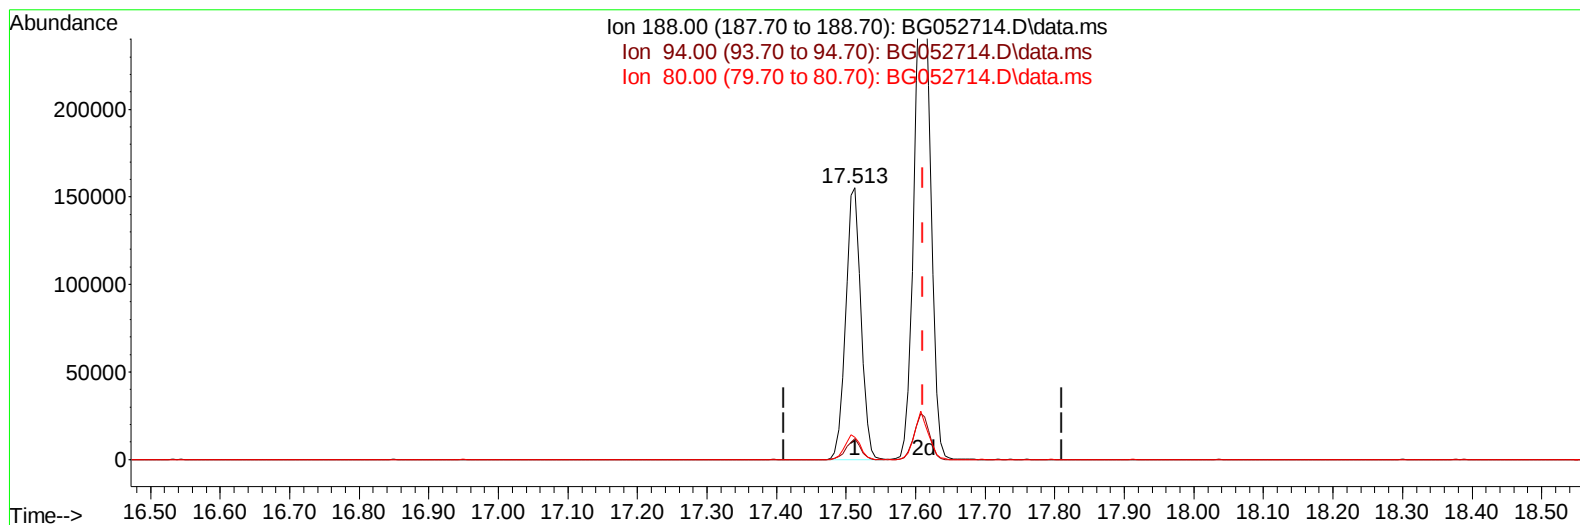

TIC: BG052714.D\data.ms

(73) Anthracene-d10 (S)

17.513min (-0.098) 21.47 ng/u1

response 234426

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	7.70
80.00	9.50	8.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052714.D
 Acq On : 18 Mar 2022 17:41
 Operator : CG/JU
 Sample : N1882-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY8

Manual IntegrationsAPPROVED

Quant Time: Mar 19 00:00:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

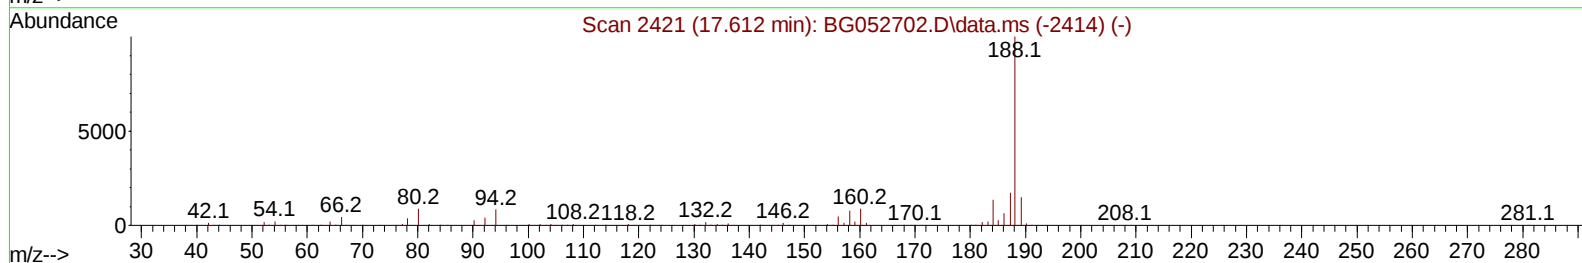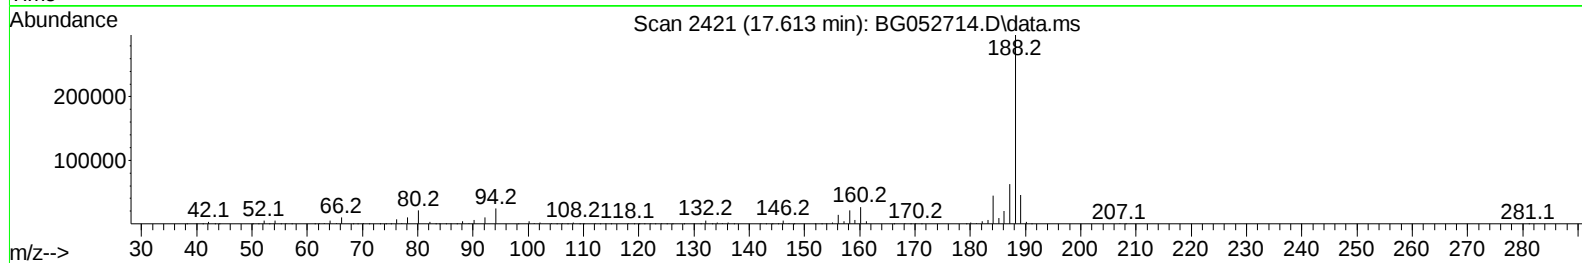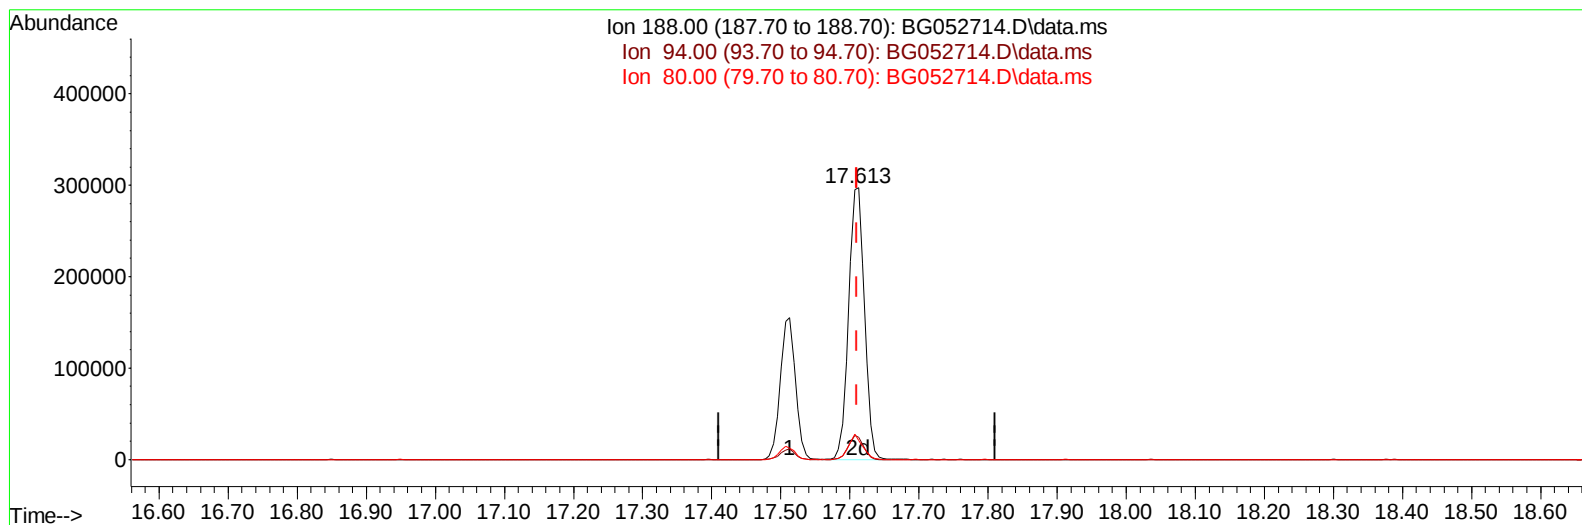

TIC: BG052714.D\data.ms

(73) Anthracene-d10 (S)

17.613min (+ 0.002) 43.24 ng/ul m

response 472057

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	8.19
80.00	9.50	7.03#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052714.D
 Acq On : 18 Mar 2022 17:41
 Operator : CG/JU
 Sample : N1882-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRY8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 19 00:00:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.149	152	34919	20.000	ng/ul	0.00
20) Naphthalene-d8	10.963	136	145780	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.770	164	101061	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.513	188	234426	20.000	ng/ul	0.00
79) Chrysene-d12	21.795	240	264315	20.000	ng/ul	0.00
88) Perylene-d12	25.114	264	257683	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.567	96	5691	5.757	ng/uL	0.00
4) Pyridine-d5	3.984	84	74804	30.310	ng/ul	0.00
7) Phenol-d5	7.291	99	117250	37.490	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.468	67	70813	37.072	ng/ul	0.00
11) 2-Chlorophenol-d4	7.679	132	78097	36.775	ng/ul	0.00
15) 4-Methylphenol-d8	8.836	113	88630	39.121	ng/ul	0.00
21) Nitrobenzene-d5	9.312	128	40186	38.295	ng/ul	0.00
24) 2-Nitrophenol-d4	10.029	143	42988	38.839	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	90391	37.539	ng/ul	0.00
31) 4-Chloroaniline-d4	11.086	131	118540	37.248	ng/ul	0.00
46) Dimethylphthalate-d6	14.164	166	326951	42.111	ng/ul	0.00
49) Acenaphthylene-d8	14.464	160	385999	40.914	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	53470	40.962	ng/ul	0.00
60) Fluorene-d10	15.756	176	281807	41.338	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.856	200	47468	39.789	ng/ul	0.00
73) Anthracene-d10	17.613	188	472057m	43.243	ng/ul	0.00
81) Pyrene-d10	19.892	212	589916	39.896	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.891	264	587947	44.158	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052714.D
Acq On : 18 Mar 2022 17:41
Operator : CG/JU
Sample : N1882-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRY8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 19 00:00:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

