




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052740.D
Acq On : 19 Mar 2022 11:13
Operator : CG/JU
Sample : N1883-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 21 00:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

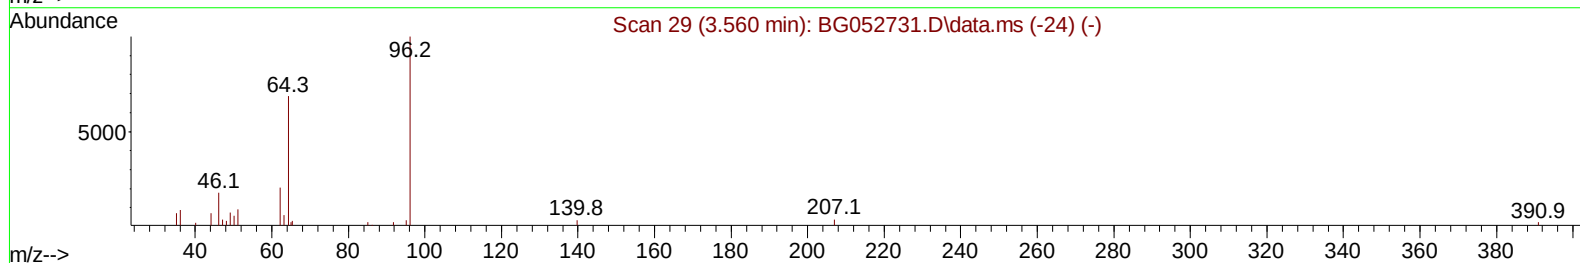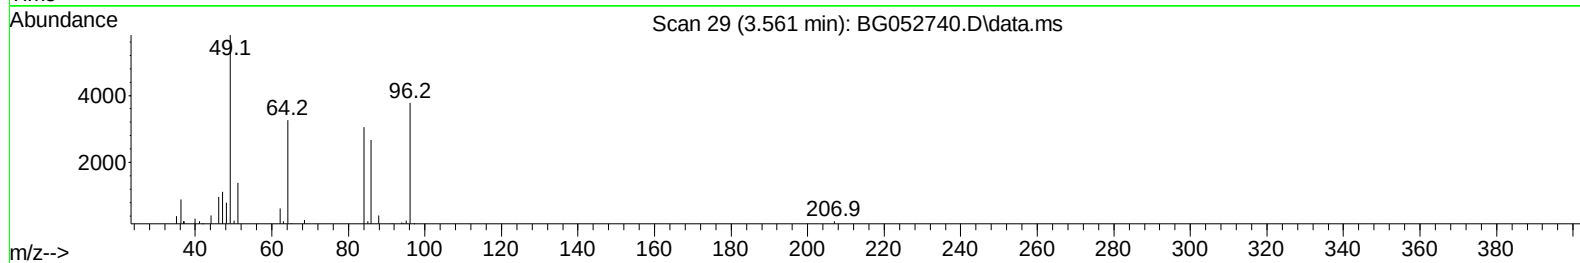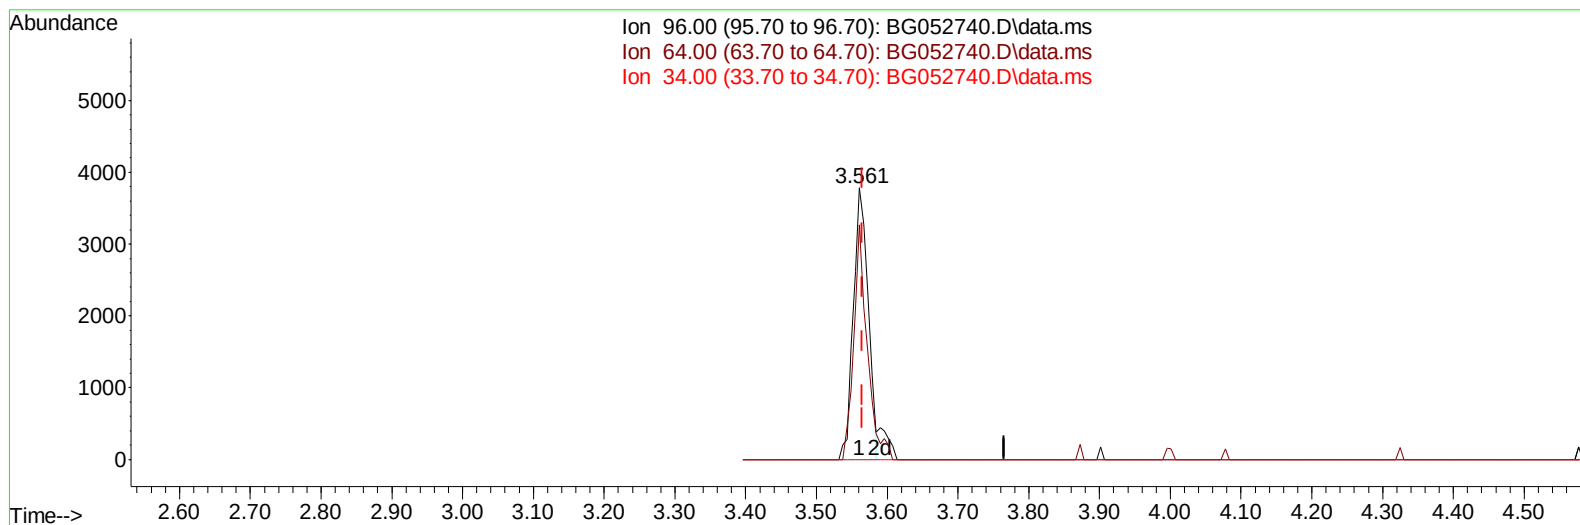

TIC: BG052740.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.561min (-0.004) 4.00 ng/uL****response 5501**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	86.46
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052740.D
 Acq On : 19 Mar 2022 11:13
 Operator : CG/JU
 Sample : N1883-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSA5

Manual IntegrationsAPPROVED

Quant Time: Mar 21 00:48:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

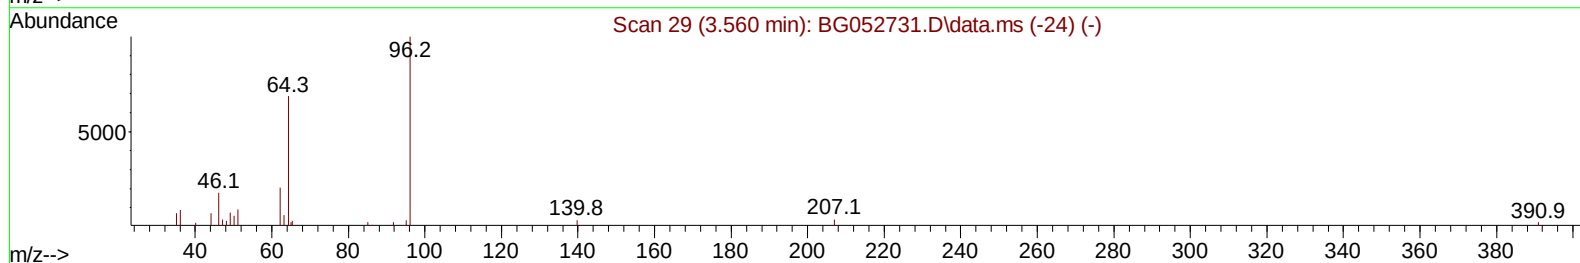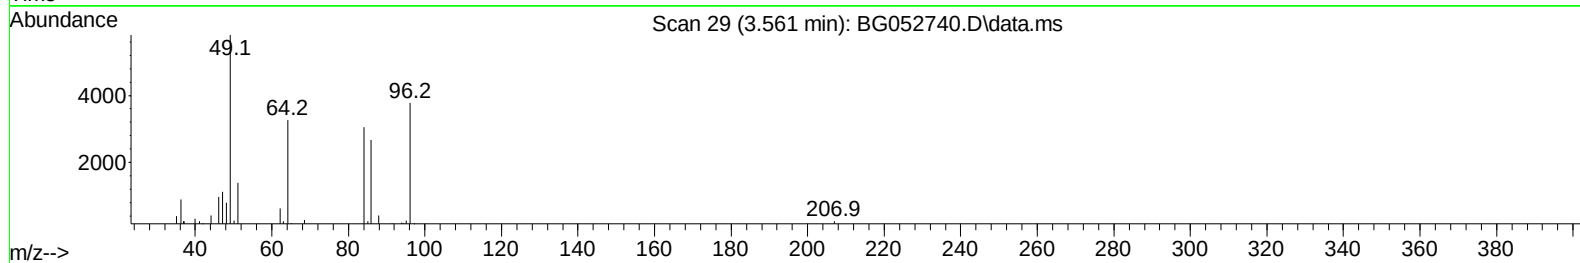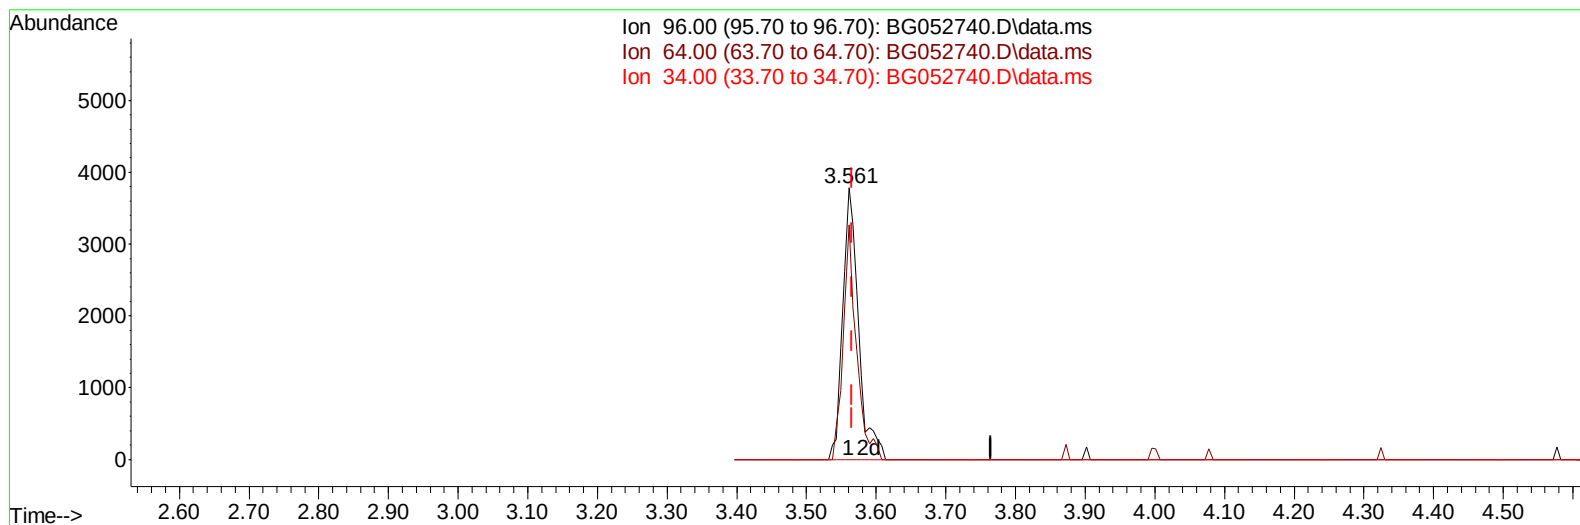

TIC: BG052740.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.561min (-0.004) 4.33 ng/uL m

response 5963

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	86.46
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052740.D
 Acq On : 19 Mar 2022 11:13
 Operator : CG/JU
 Sample : N1883-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSA5

Manual IntegrationsAPPROVED

Quant Time: Mar 21 00:48:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.149	152	48637	20.000	ng/ul	0.00
20) Naphthalene-d8	10.963	136	197219	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.769	164	140485	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.513	188	336061	20.000	ng/ul	0.00
79) Chrysene-d12	21.795	240	355081	20.000	ng/ul	# 0.00
88) Perylene-d12	25.120	264	345152	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.561	96	5963m	4.331	ng/uL	0.00
4) Pyridine-d5	3.978	84	73153	21.281	ng/ul	0.00
7) Phenol-d5	7.291	99	105687	24.261	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.461	67	64781	24.349	ng/ul	0.00
11) 2-Chlorophenol-d4	7.679	132	70773	23.927	ng/ul	0.00
15) 4-Methylphenol-d8	8.836	113	79510	25.197	ng/ul	0.00
21) Nitrobenzene-d5	9.306	128	37571	26.465	ng/ul	0.00
24) 2-Nitrophenol-d4	10.034	143	42158	28.154	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	81458	25.006	ng/ul	0.00
31) 4-Chloroaniline-d4	11.086	131	107986	25.081	ng/ul	0.00
46) Dimethylphthalate-d6	14.164	166	312216	28.929	ng/ul	0.00
49) Acenaphthylene-d8	14.458	160	360171	27.463	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	50345	27.745	ng/ul	0.00
60) Fluorene-d10	15.756	176	266085	28.078	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.856	200	45419	26.558	ng/ul	0.00
73) Anthracene-d10	17.607	188	444209	28.386	ng/ul	0.00
81) Pyrene-d10	19.892	212	551856	27.782	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.891	264	512097	28.715	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.315	94	6867	1.636	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052740.D
Acq On : 19 Mar 2022 11:13
Operator : CG/JU
Sample : N1883-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 21 00:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

