




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052756.D
 Acq On : 19 Mar 2022 22:14
 Operator : CG/JU
 Sample : N1820-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRZ6

Manual IntegrationsAPPROVED

Quant Time: Mar 21 00:52:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

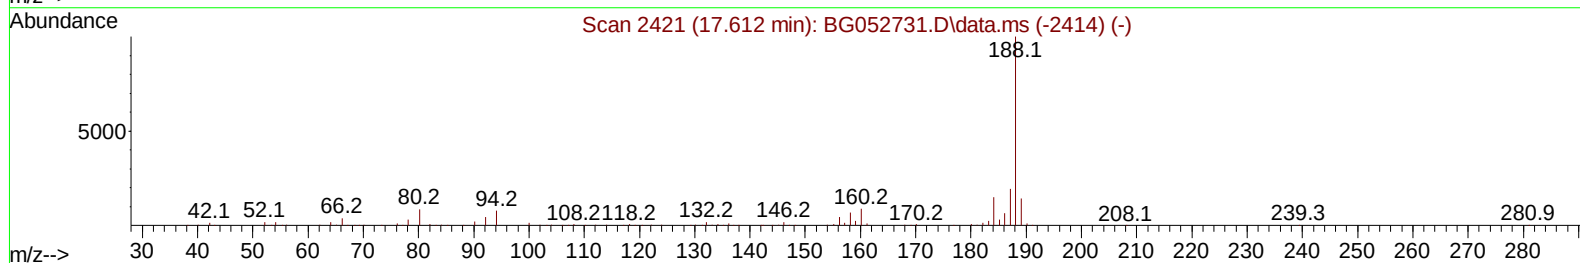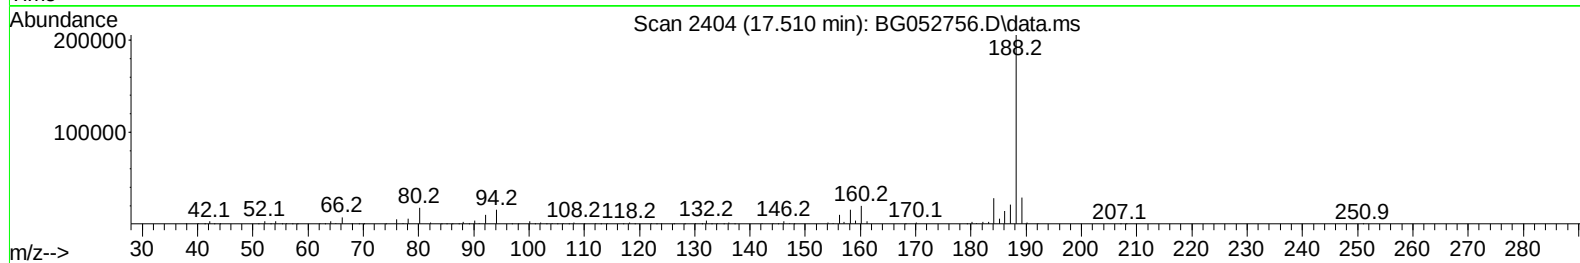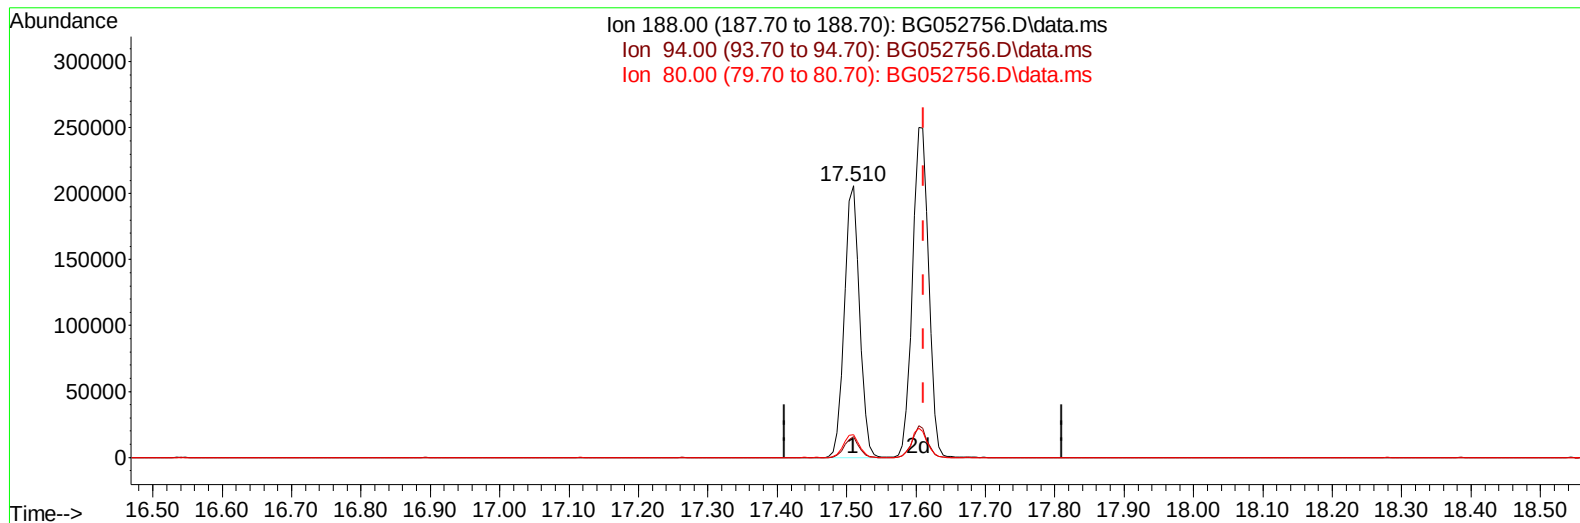

TIC: BG052756.D\data.ms

(73) Anthracene-d10 (S)

17.510min (-0.101) 21.47 ng/u1

response 313546

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	7.60
80.00	9.50	8.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052756.D
 Acq On : 19 Mar 2022 22:14
 Operator : CG/JU
 Sample : N1820-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRZ6

Manual IntegrationsAPPROVED

Quant Time: Mar 21 00:52:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

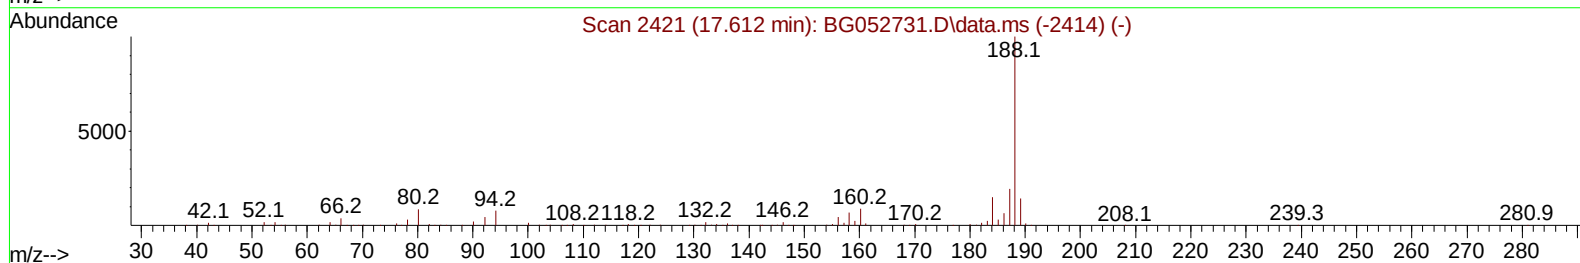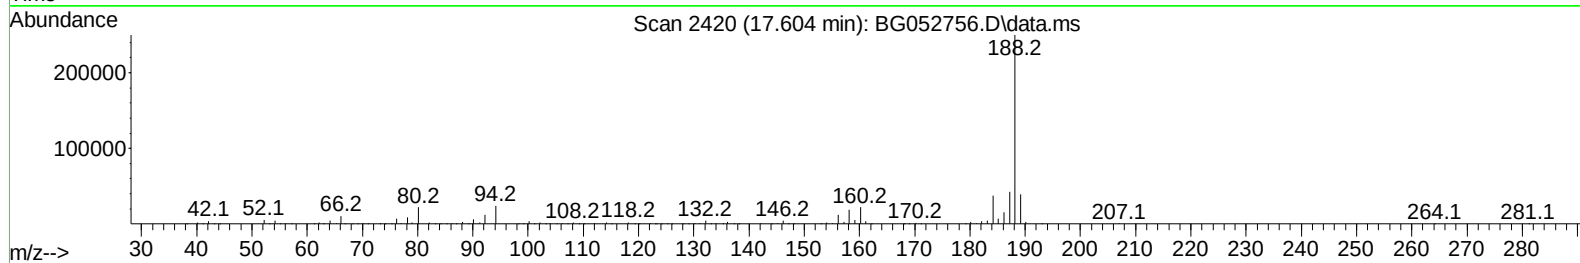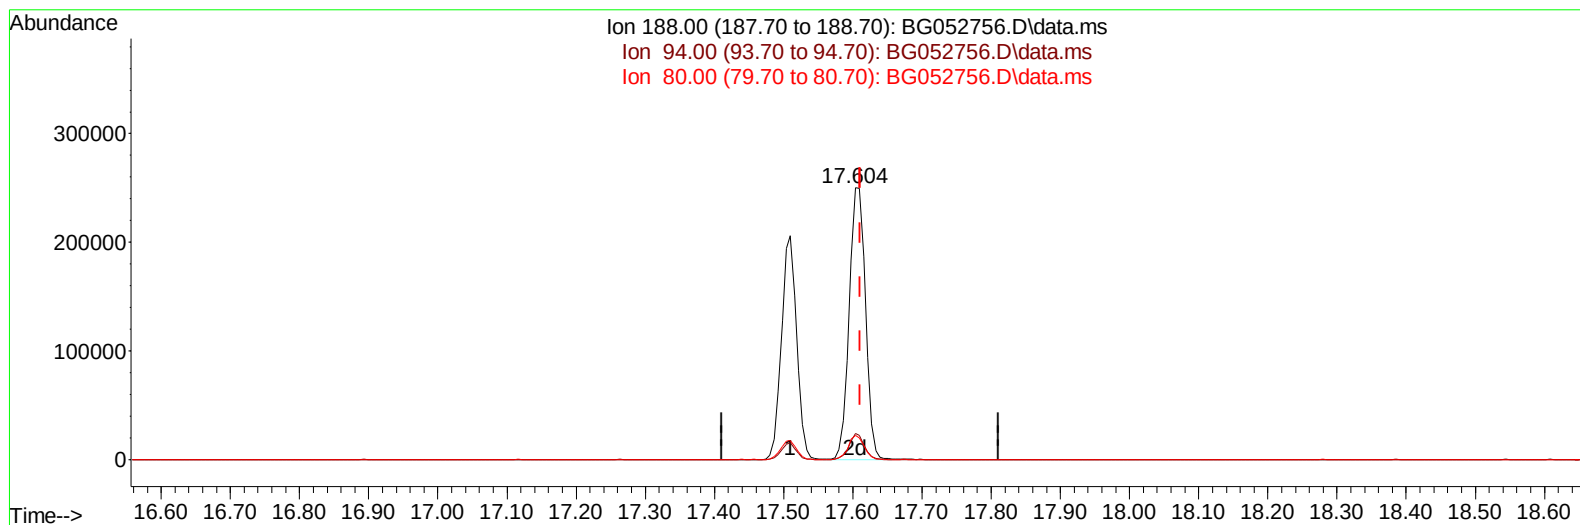

TIC: BG052756.D\data.ms

(73) Anthracene-d10 (S)

17.604min (-0.007) 27.69 ng/ul m

response 404311

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	9.57#
80.00	9.50	8.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052756.D
 Acq On : 19 Mar 2022 22:14
 Operator : CG/JU
 Sample : N1820-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRZ6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 21 00:52:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.146	152	46948	20.000	ng/ul	0.00
20) Naphthalene-d8	10.960	136	187894	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.766	164	132150	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	313546	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	336984	20.000	ng/ul	#-0.01
88) Perylene-d12	25.111	264	320937	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.564	96	6377	4.798	ng/uL	0.00
4) Pyridine-d5	3.975	84	71991	21.696	ng/ul	0.00
7) Phenol-d5	7.288	99	115236	27.405	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.464	67	70683	27.523	ng/ul	0.00
11) 2-Chlorophenol-d4	7.676	132	77109	27.007	ng/ul	0.00
15) 4-Methylphenol-d8	8.839	113	83258	27.334	ng/ul	0.00
21) Nitrobenzene-d5	9.303	128	40611	30.026	ng/ul	0.00
24) 2-Nitrophenol-d4	10.032	143	44131	30.935	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.572	165	82898	26.711	ng/ul	0.00
31) 4-Chloroaniline-d4	11.083	131	110489	26.936	ng/ul	0.00
46) Dimethylphthalate-d6	14.161	166	280853	27.664	ng/ul	0.00
49) Acenaphthylene-d8	14.461	160	340759	27.622	ng/ul	0.00
54) 4-Nitrophenol-d4	14.931	143	45077	26.408	ng/ul	0.00
60) Fluorene-d10	15.753	176	246021	27.599	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	38341	24.029	ng/ul	0.00
73) Anthracene-d10	17.604	188	404311m	27.691	ng/ul	0.00
81) Pyrene-d10	19.889	212	503770	26.723	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.882	264	465393	28.065	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052756.D
Acq On : 19 Mar 2022 22:14
Operator : CG/JU
Sample : N1820-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRZ6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 21 00:52:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

