

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052736.D
 Acq On : 19 Mar 2022 8:37
 Operator : CG/JU
 Sample : N1883-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSA4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
 Supervised By :Yogesh Patel 03/24/2022

Quant Time: Mar 21 00:48:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.150	152	35733	20.000	ng/u1	0.00
20) Naphthalene-d8	10.958	136	146990	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.764	164	104337	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.508	188	246193	20.000	ng/u1	0.00
79) Chrysene-d12	21.796	240	272249	20.000	ng/u1	0.00
88) Perylene-d12	25.115	264	267838	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.562	96	4702m	4.648	ng/uL	0.00
4) Pyridine-d5	3.979	84	51047	20.213	ng/u1	0.00
7) Phenol-d5	7.292	99	83745	26.167	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.462	67	52601	26.910	ng/u1	0.00
11) 2-Chlorophenol-d4	7.680	132	58100	26.736	ng/u1	0.00
15) 4-Methylphenol-d8	8.837	113	59686	25.745	ng/u1	0.00
21) Nitrobenzene-d5	9.307	128	29298	27.689	ng/u1	0.00
24) 2-Nitrophenol-d4	10.029	143	30290	27.141	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.570	165	60739	25.017	ng/u1	0.00
31) 4-Chloroaniline-d4	11.081	131	82403	25.680	ng/u1	0.00
46) Dimethylphthalate-d6	14.165	166	203907	25.439	ng/u1	0.00
49) Acenaphthylene-d8	14.459	160	256061	26.289	ng/u1	0.00
54) 4-Nitrophenol-d4	14.929	143	27988m	20.768	ng/u1	0.00
60) Fluorene-d10	15.757	176	182939	25.993	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	22041	17.592	ng/u1	0.00
73) Anthracene-d10	17.607	188	302817	26.414	ng/u1	0.00
81) Pyrene-d10	19.887	212	379556	24.921	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.886	264	359974	26.011	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.321	94	7517	2.437	ng/u1	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052736.D
Acq On : 19 Mar 2022 8:37
Operator : CG/JU
Sample : N1883-05
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA4




Quant Time: Mar 21 00:48:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

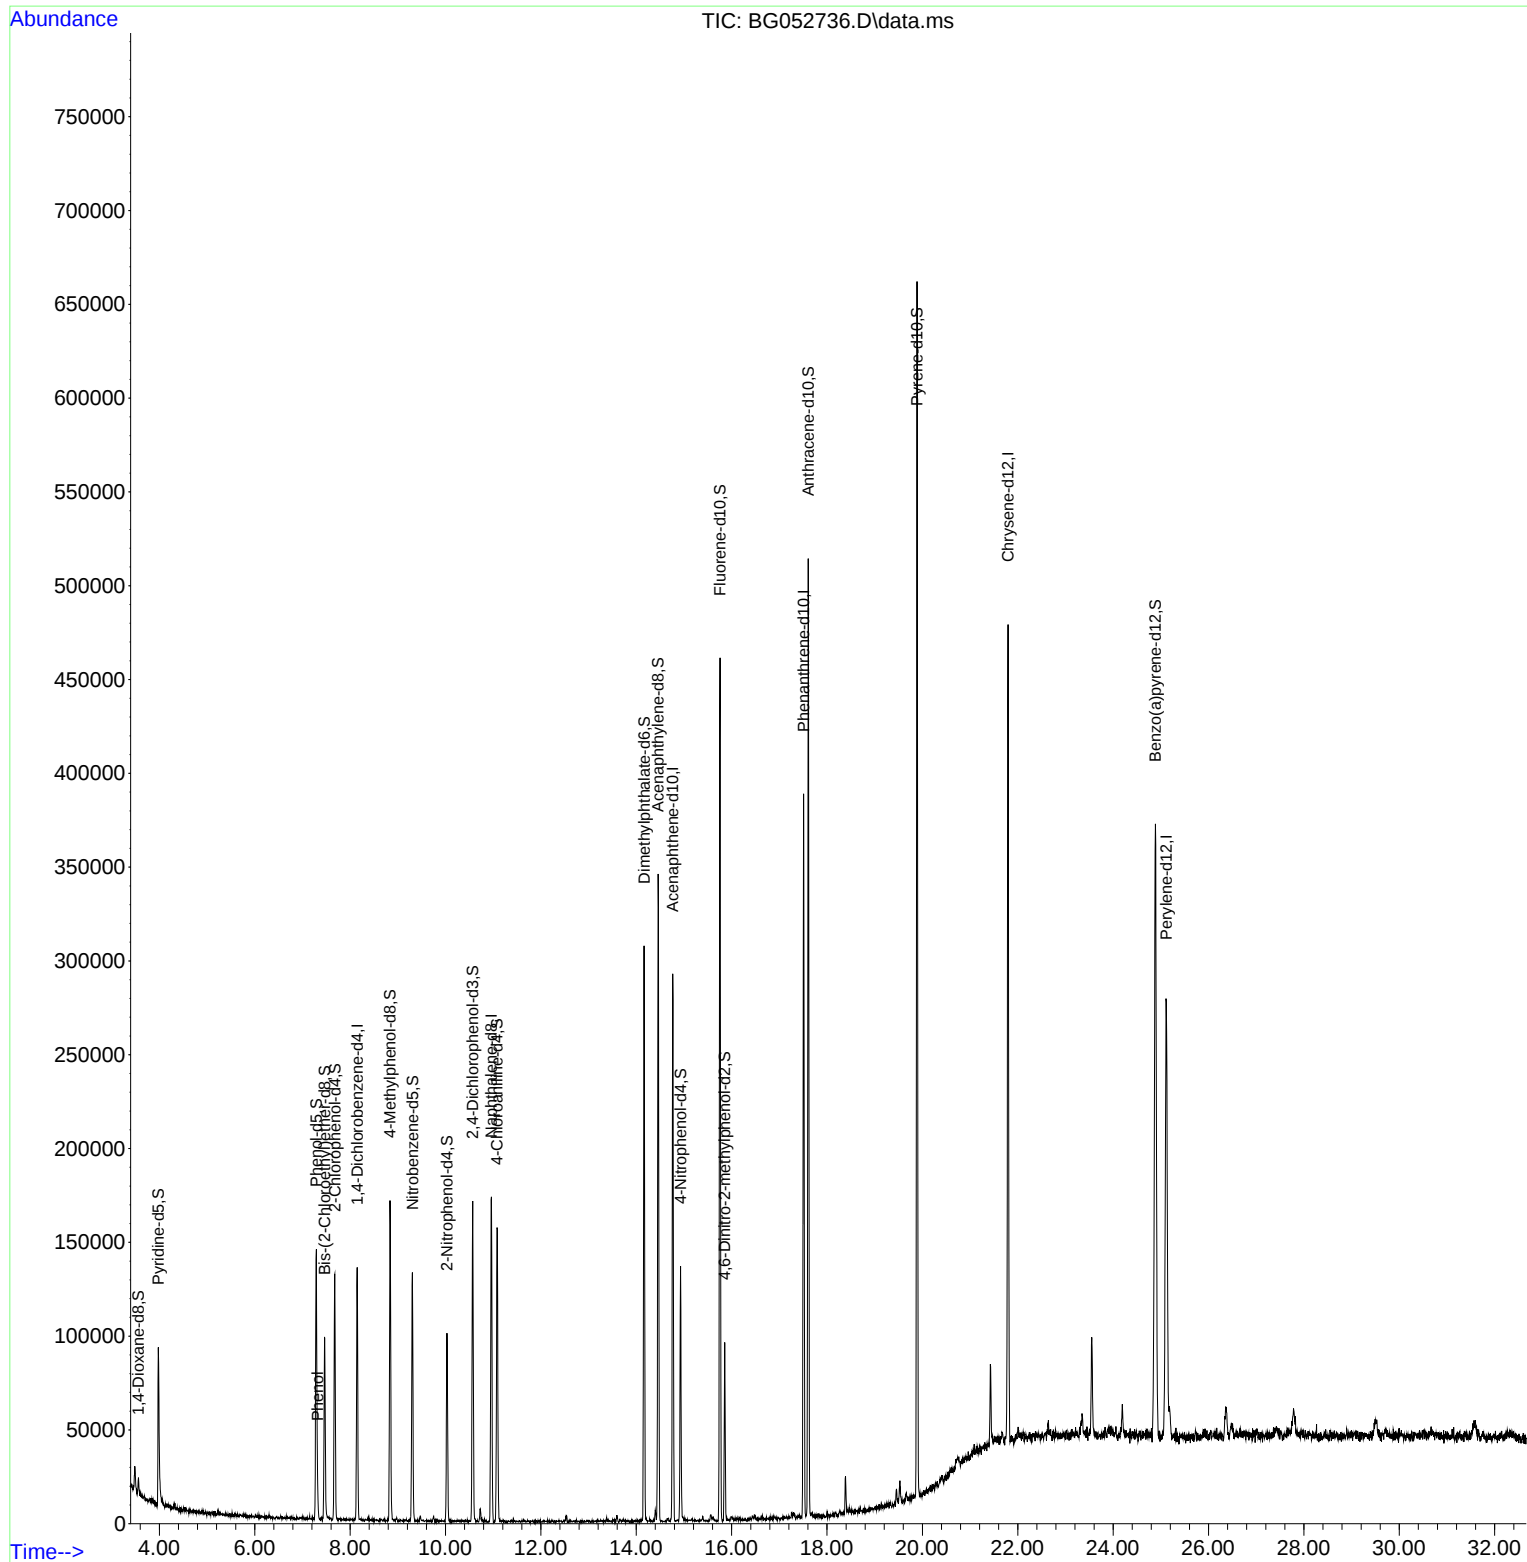

Abundance Scan 669 (7.320 min): BG052731.D\data.ms (-66

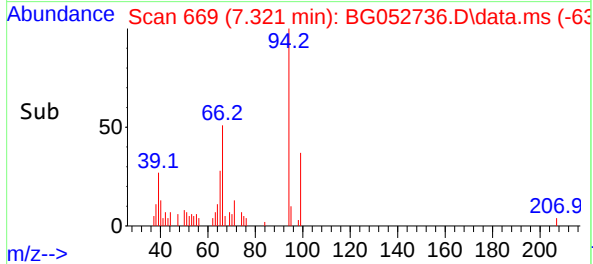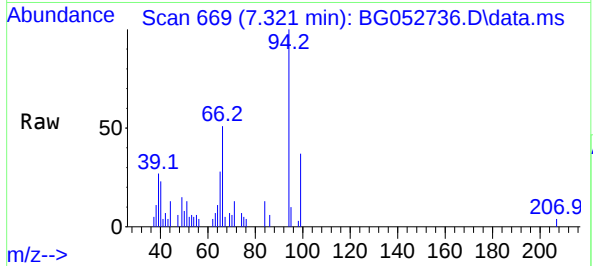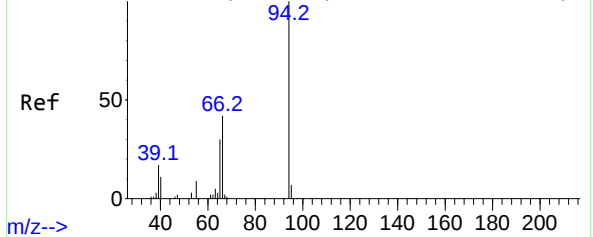

#8
Phenol
Concen: 2.437 ng/ul
RT: 7.321 min Scan# 60
Delta R.T. 0.003 min
Lab File: BG052736.D
Acq: 19 Mar 2022 8:37

Instrument :
BNA_G
ClientSampleId :
DBSA4

Tgt Ion:	94	Resp:	751
Ion	Ratio	Lower	Upper
94	100		
65	28.2	25.9	38.9
66	50.7	35.4	53.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/21/2022
Supervised By :Yogesh Patel 03/24/2022

