

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052737.D
 Acq On : 19 Mar 2022 9:16
 Operator : CG/JU
 Sample : N1883-09
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSA8

Quant Time: Mar 21 00:48:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 00:55:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.148	152	44827	20.000	ng/u1	0.00
20) Naphthalene-d8	10.962	136	176841	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.769	164	124760	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.512	188	292561	20.000	ng/u1	0.00
79) Chrysene-d12	21.794	240	334927	20.000	ng/u1	-0.01
88) Perylene-d12	25.113	264	331792	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.566	96	5184	4.085	ng/uL	0.00
4) Pyridine-d5	3.983	84	65341	20.624	ng/u1	0.00
7) Phenol-d5	7.290	99	92995	23.162	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.461	67	59192	24.139	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.678	132	62095	22.777	ng/u1	0.00
15) 4-Methylphenol-d8	8.835	113	66749	22.951	ng/u1	-0.01
21) Nitrobenzene-d5	9.305	128	33027	25.945	ng/u1	0.00
24) 2-Nitrophenol-d4	10.034	143	33897	25.246	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.568	165	67173	22.997	ng/u1	0.00
31) 4-Chloroaniline-d4	11.085	131	89930	23.295	ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	234070	24.421	ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	283068	24.305	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.933	143	35665	22.132	ng/u1	0.00
60) Fluorene-d10	15.755	176	204072	24.249	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.855	200	32193	21.623	ng/u1	0.00
73) Anthracene-d10	17.606	188	336293	24.685	ng/u1	0.00
81) Pyrene-d10	19.891	212	438026	23.378	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.890	264	422259	24.630	ng/u1	0.00


Target Compounds					Qvalue	
8) Phenol	7.314	94	7522	1.944	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052737.D
Acq On : 19 Mar 2022 9:16
Operator : CG/JU
Sample : N1883-09
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA8

Quant Time: Mar 21 00:48:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 00:55:42 2022
Response via : Initial Calibration

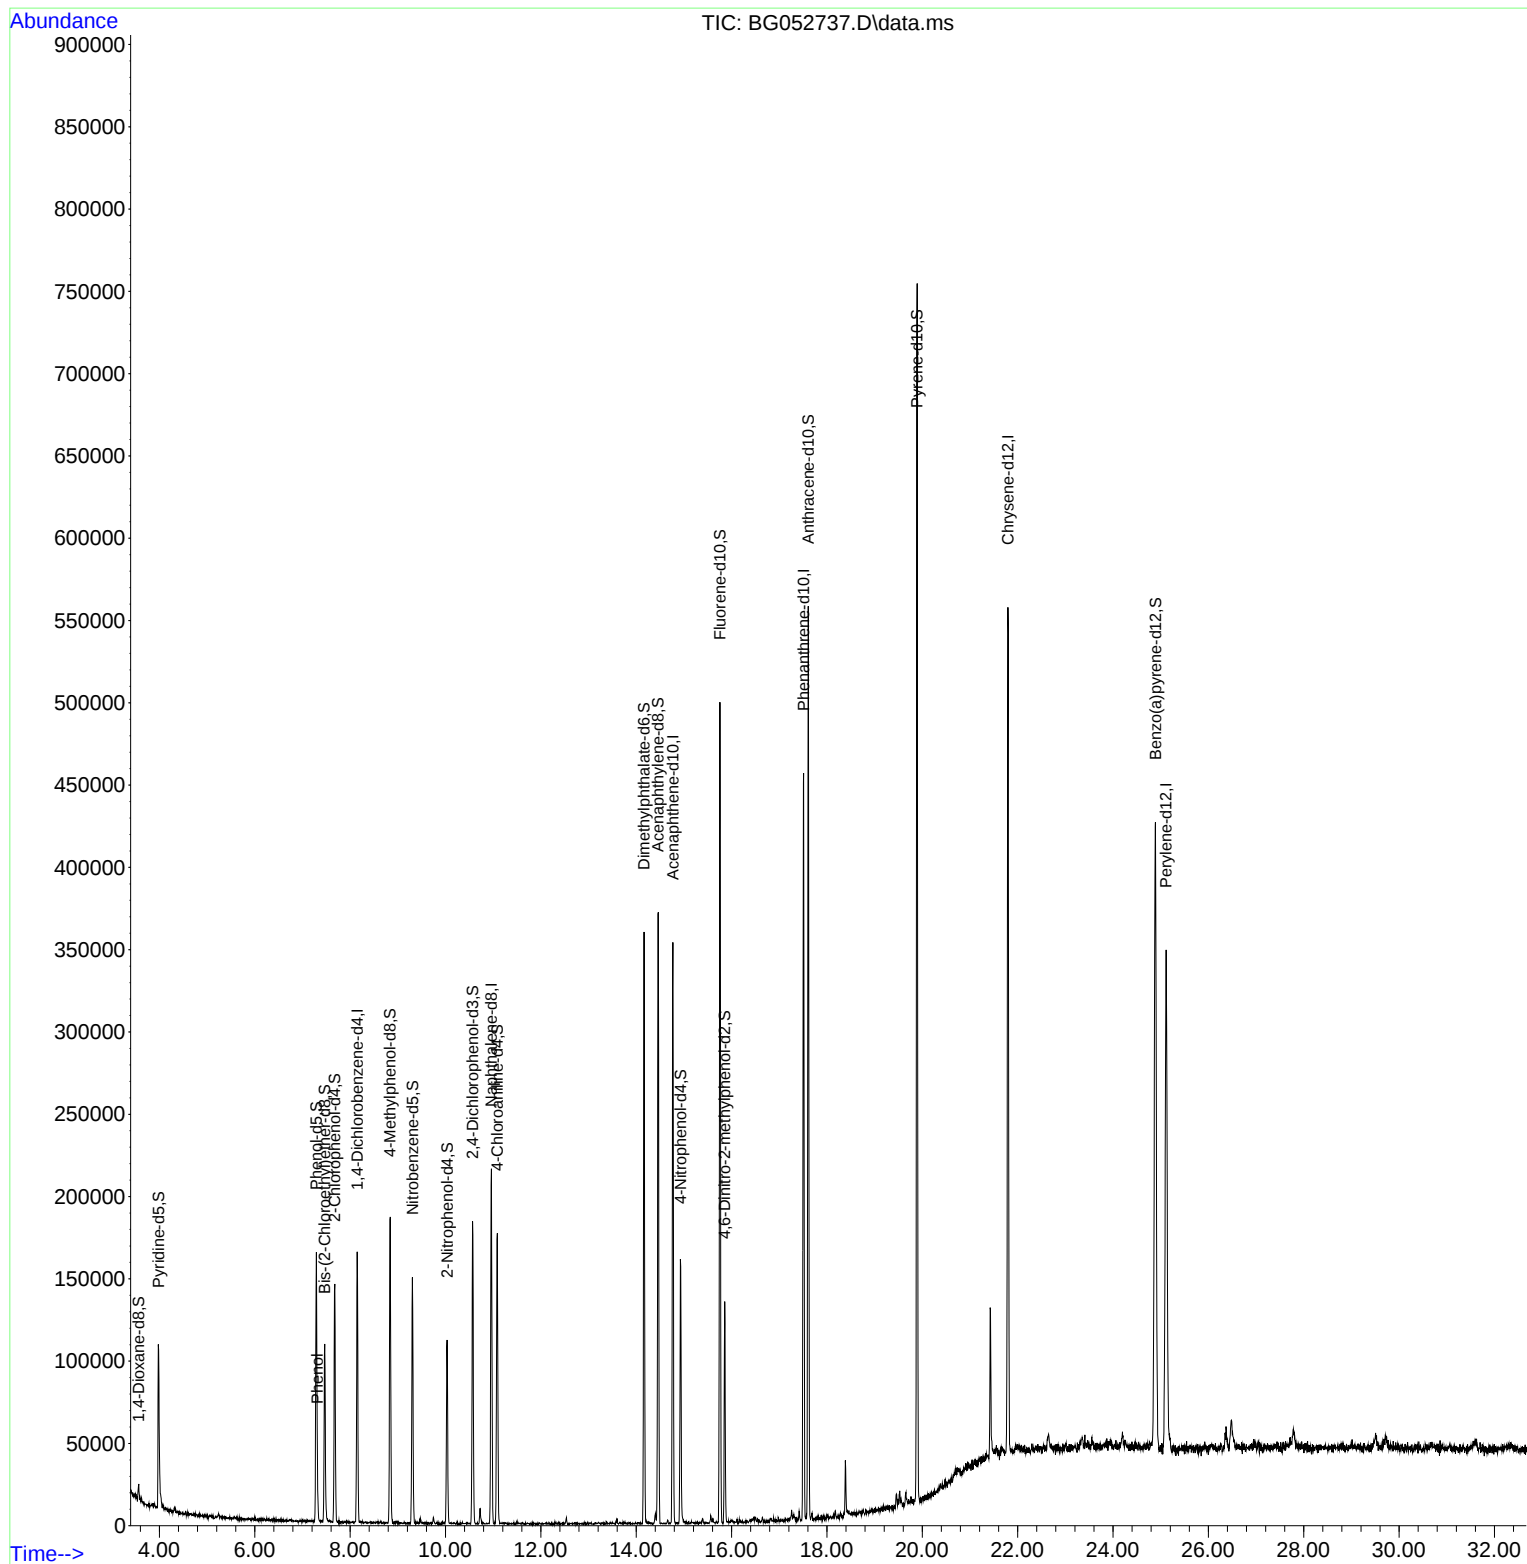

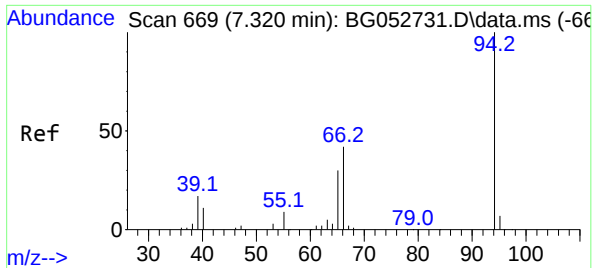

#8
Phenol
Concen: 1.944 ng/ul
RT: 7.314 min Scan# 60
Delta R.T. -0.005 min
Lab File: BG052737.D
Acq: 19 Mar 2022 9:16

Instrument :
BNA_G
ClientSampleId :
DBSA8

Tgt Ion: 94 Resp: 7522

Ion	Ratio	Lower	Upper
94	100		
65	33.1	25.9	38.9
66	48.7	35.4	53.2

