

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052717.D
 Acq On : 18 Mar 2022 19:39
 Operator : CG/JU
 Sample : N1882-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	26	30	36	rVB4	11117	19164	1.19%	0.134%
2	3.752	60	62	64	rBV2	2047	1736	0.11%	0.012%
3	3.852	76	79	83	rBV4	2560	3687	0.23%	0.026%
4	3.981	96	101	114	rBV	137921	252692	15.67%	1.763%
5	4.186	132	136	137	rBV4	1611	1705	0.11%	0.012%
6	4.327	158	160	164	rVB3	2868	3186	0.20%	0.022%
7	4.404	171	173	177	rBV3	2741	3249	0.20%	0.023%
8	4.433	177	178	181	rBV2	1823	2120	0.13%	0.015%
9	4.551	197	198	201	rVB2	2374	2053	0.13%	0.014%
10	5.244	313	316	320	rVB5	3380	4883	0.30%	0.034%
11	5.532	364	365	369	rBV2	1229	1749	0.11%	0.012%
12	5.831	413	416	419	rVB4	1835	2001	0.12%	0.014%
13	5.861	419	421	425	rBV2	1106	1787	0.11%	0.012%
14	6.971	608	610	614	rVB3	1256	1759	0.11%	0.012%
15	7.135	634	638	646	rVB4	1164	2664	0.17%	0.019%
16	7.294	656	665	672	rBV	198429	349095	21.64%	2.435%
17	7.394	678	682	683	rBV4	1412	1626	0.10%	0.011%
18	7.470	688	695	704	rVV	134142	236051	14.63%	1.646%
19	7.676	724	730	740	rBV	166218	296431	18.38%	2.068%
20	8.152	804	811	818	rVB	124778	217707	13.50%	1.519%
21	8.210	818	821	823	rBV4	2223	2691	0.17%	0.019%
22	8.404	850	854	857	rBV3	923	1615	0.10%	0.011%
23	8.839	921	928	940	rVB	255086	435544	27.00%	3.038%
24	9.309	1000	1008	1017	rBV	187295	346106	21.46%	2.414%
25	9.403	1020	1024	1025	rBV2	1955	1652	0.10%	0.012%
26	9.749	1079	1083	1089	rVB2	6161	8597	0.53%	0.060%
27	10.037	1123	1132	1139	rBV	144030	266285	16.51%	1.857%
28	10.572	1216	1223	1231	rBV	243892	440992	27.34%	3.076%
29	10.725	1245	1249	1257	rVB3	7700	13436	0.83%	0.094%
30	10.965	1281	1290	1297	rVB	169186	307198	19.04%	2.143%
31	11.083	1303	1310	1318	rVV	248387	453349	28.11%	3.162%
32	11.982	1461	1463	1466	rVB3	1405	1627	0.10%	0.011%
33	12.240	1504	1507	1513	rVB3	1632	2295	0.14%	0.016%
34	12.381	1524	1531	1533	rBV4	3621	6859	0.43%	0.048%
35	12.540	1553	1558	1562	rVB2	5657	7594	0.47%	0.053%
36	13.174	1664	1666	1671	rVB3	2074	2227	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052717.D
 Acq On : 18 Mar 2022 19:39
 Operator : CG/JU
 Sample : N1882-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	13.321	1687	1691	1695	rVB3	2328	3745	0.23%	0.026%
38	13.386	1698	1702	1706	rBV3	1457	2124	0.13%	0.015%
39	13.597	1733	1738	1744	rBV3	11505	17502	1.09%	0.122%
40	14.167	1828	1835	1842	rVB	518271	768878	47.67%	5.363%
41	14.408	1872	1876	1879	rBV4	4018	6433	0.40%	0.045%
42	14.461	1879	1885	1895	rVV	540240	888300	55.07%	6.196%
43	14.672	1916	1921	1924	rBV3	3905	6491	0.40%	0.045%
44	14.766	1931	1937	1945	rVB	273439	436938	27.09%	3.048%
45	14.931	1957	1965	1974	rBV	258948	411047	25.48%	2.867%
46	14.989	1974	1975	1978	rVV2	3611	2751	0.17%	0.019%
47	15.048	1981	1985	1988	rVB3	1213	1824	0.11%	0.013%
48	15.348	2032	2036	2040	rVV3	1642	2756	0.17%	0.019%
49	15.565	2067	2073	2077	rBV3	3579	6379	0.40%	0.044%
50	15.612	2077	2081	2085	rVB4	2994	3796	0.24%	0.026%
51	15.759	2098	2106	2114	rBV	717765	1123392	69.65%	7.836%
52	15.859	2116	2123	2129	rVV	194962	287921	17.85%	2.008%
53	16.000	2143	2147	2152	rVV4	4215	5647	0.35%	0.039%
54	16.111	2161	2166	2170	rBV4	1635	3142	0.19%	0.022%
55	16.164	2172	2175	2179	rVV4	2196	3128	0.19%	0.022%
56	16.235	2183	2187	2188	rVV3	1492	1681	0.10%	0.012%
57	16.264	2188	2192	2194	rVB3	1768	2327	0.14%	0.016%
58	16.399	2211	2215	2218	rBV2	1362	2314	0.14%	0.016%
59	16.429	2218	2220	2223	rBV3	2102	1959	0.12%	0.014%
60	16.476	2223	2228	2231	rVV6	1746	3029	0.19%	0.021%
61	16.552	2236	2241	2244	rBV4	4075	7691	0.48%	0.054%
62	16.758	2272	2276	2279	rVV3	2275	3855	0.24%	0.027%
63	16.816	2282	2286	2288	rVB4	1506	2238	0.14%	0.016%
64	16.916	2300	2303	2308	rVB4	3600	5383	0.33%	0.038%
65	17.116	2333	2337	2339	rBV2	1676	2040	0.13%	0.014%
66	17.251	2357	2360	2364	rBV4	6059	9796	0.61%	0.068%
67	17.421	2386	2389	2393	rVB5	2510	3363	0.21%	0.023%
68	17.510	2397	2404	2411	rVB	353645	564599	35.00%	3.938%
69	17.609	2413	2421	2430	rBV	850969	1284815	79.65%	8.962%
70	17.686	2430	2434	2437	rVV5	5369	6790	0.42%	0.047%
71	17.786	2448	2451	2453	rVV4	1335	1795	0.11%	0.013%
72	17.880	2465	2467	2470	rVB4	1374	1723	0.11%	0.012%
73	18.050	2494	2496	2500	rVB3	1979	2729	0.17%	0.019%
74	18.238	2523	2528	2531	rBV4	1453	2573	0.16%	0.018%
75	18.297	2536	2538	2540	rBV4	2221	2305	0.14%	0.016%
76	18.391	2550	2554	2559	rBV3	26680	38477	2.39%	0.268%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052717.D
 Acq On : 18 Mar 2022 19:39
 Operator : CG/JU
 Sample : N1882-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	18.467	2562	2567	2570	rVV6	3881	5503	0.34%	0.038%
78	18.820	2625	2627	2630	rVB4	3287	3463	0.21%	0.024%
79	18.855	2630	2633	2634	rBV3	1406	1806	0.11%	0.013%
80	19.072	2668	2670	2673	rVB4	2222	1799	0.11%	0.013%
81	19.166	2684	2686	2687	rBV2	2268	1941	0.12%	0.014%
82	19.213	2692	2694	2696	rBV2	1820	1778	0.11%	0.012%
83	19.237	2696	2698	2701	rBV4	2131	2426	0.15%	0.017%
84	19.260	2701	2702	2704	rVV	2354	1714	0.11%	0.012%
85	19.325	2710	2713	2715	rBV4	1928	2791	0.17%	0.019%
86	19.407	2725	2727	2729	rBV3	1897	1838	0.11%	0.013%
87	19.460	2731	2736	2741	rBV3	14159	21212	1.32%	0.148%
88	19.524	2743	2747	2751	rVV	15788	20041	1.24%	0.140%
89	19.560	2751	2753	2755	rVV2	2212	2366	0.15%	0.017%
90	19.613	2759	2762	2763	rBV3	2779	2258	0.14%	0.016%
91	19.654	2766	2769	2773	rBV6	10744	14196	0.88%	0.099%
92	19.701	2775	2777	2778	rBV2	2693	2244	0.14%	0.016%
93	19.795	2791	2793	2796	rBV3	3487	3682	0.23%	0.026%
94	19.889	2802	2809	2816	rBV	1057744	1603991	99.44%	11.188%
95	20.071	2837	2840	2842	rBV3	4916	5892	0.37%	0.041%
96	21.428	3067	3071	3081	rBV7	56107	86958	5.39%	0.607%
97	21.798	3127	3134	3142	rVB	415797	693404	42.99%	4.837%
98	24.894	3650	3661	3673	rVB2	551504	1613016	100.00%	11.251%
99	25.117	3690	3699	3708	rBV2	207220	599156	37.15%	4.179%
100	27.249	4060	4062	4064	rBV3	7711	6314	0.39%	0.044%




Sum of corrected areas: 14336877

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052717.D
Acq On : 18 Mar 2022 19:39
Operator : CG/JU
Sample : N1882-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

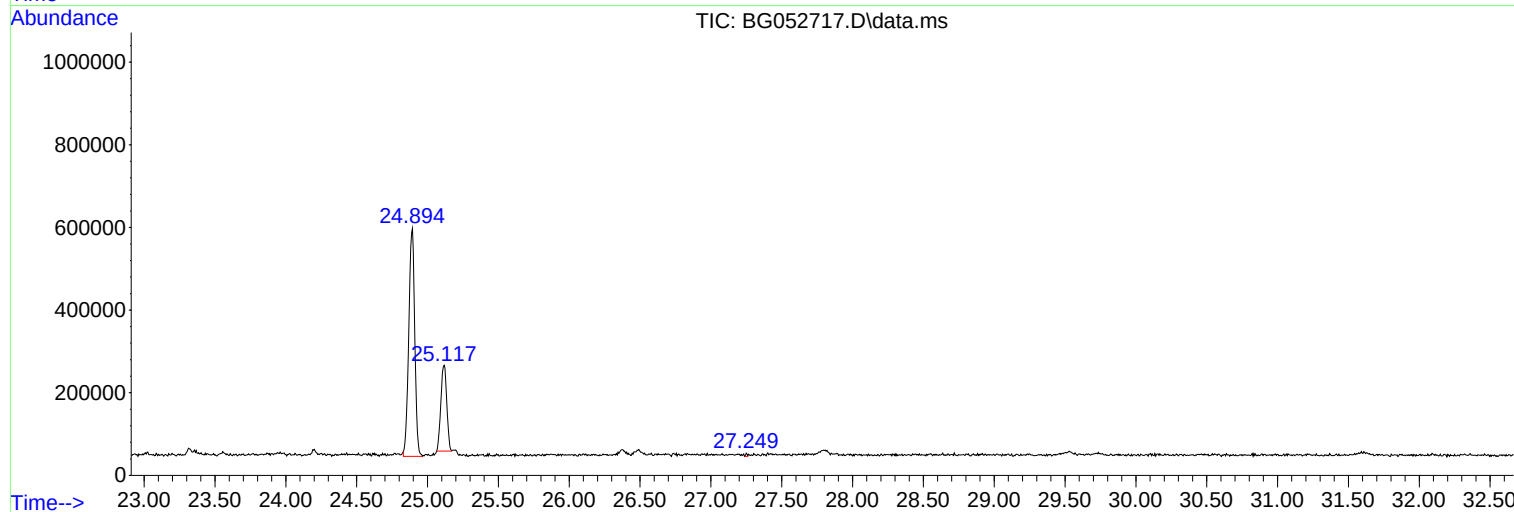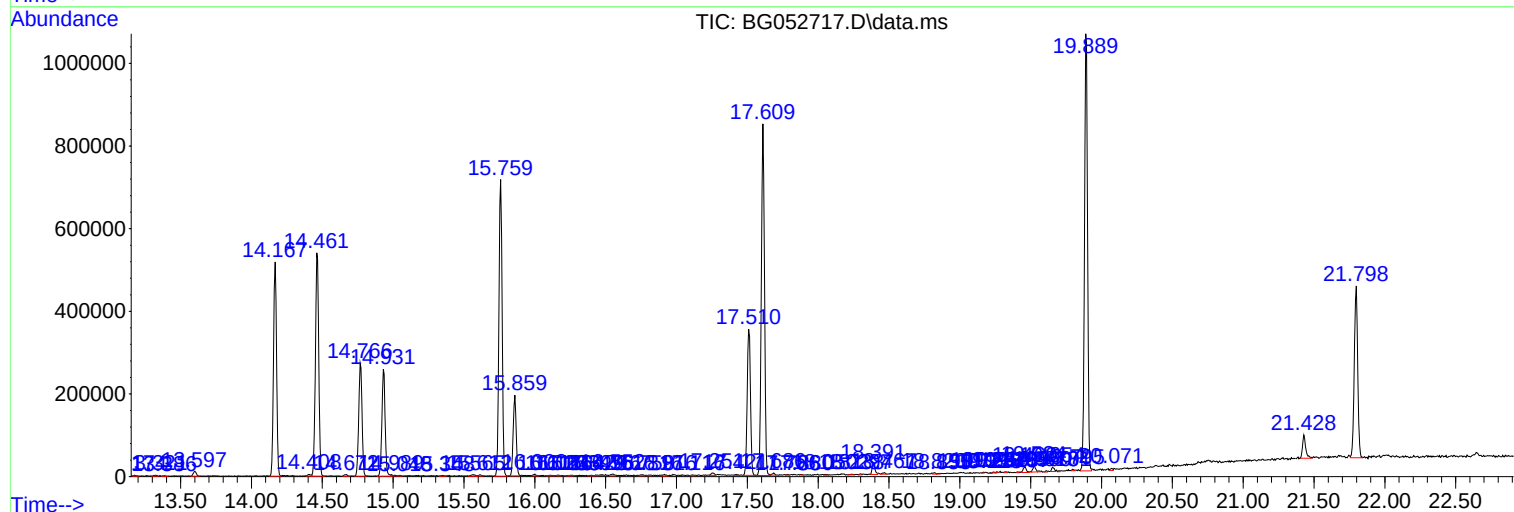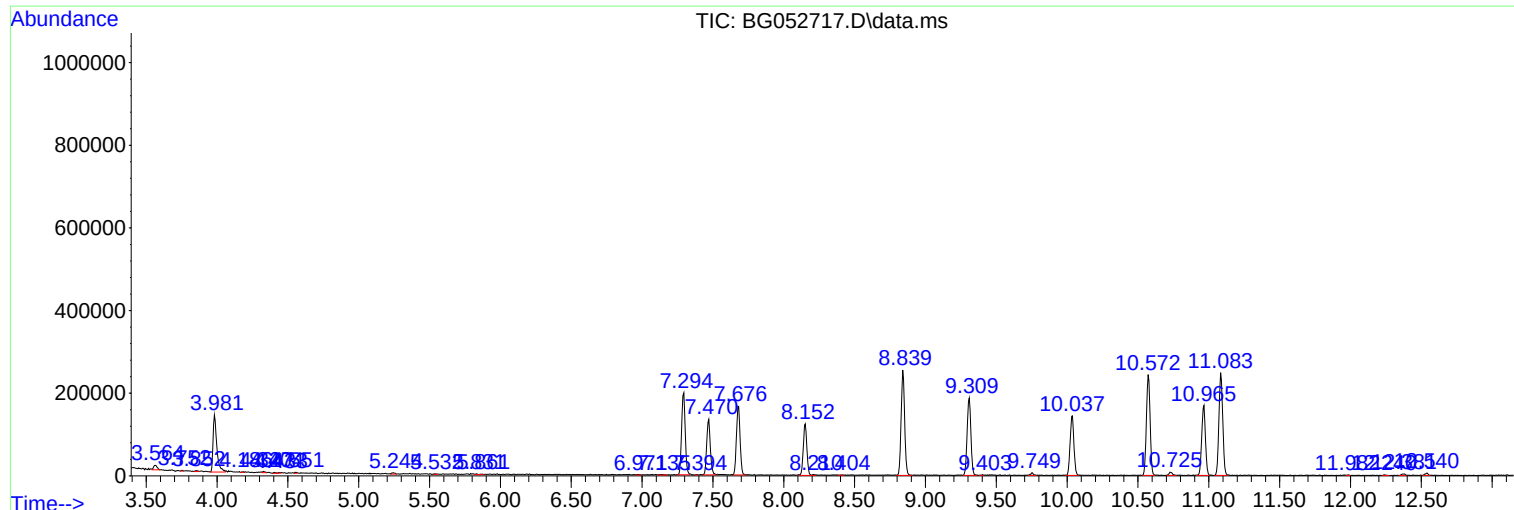

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052717.D
Acq On : 18 Mar 2022 19:39
Operator : CG/JU
Sample : N1882-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRZ2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.428	2.51 ng/ul	86958	Chrysene-d12	21.798

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonadecene			266	C19H38	018435-45-5	91
2	1-Tetracosene			336	C24H48	010192-32-2	91
3	Cyclotetradecane			196	C14H28	000295-17-0	90
4	3-Eicosene, (E)-			280	C20H40	074685-33-9	90
5	9-Eicosene, (E)-			280	C20H40	074685-29-3	87

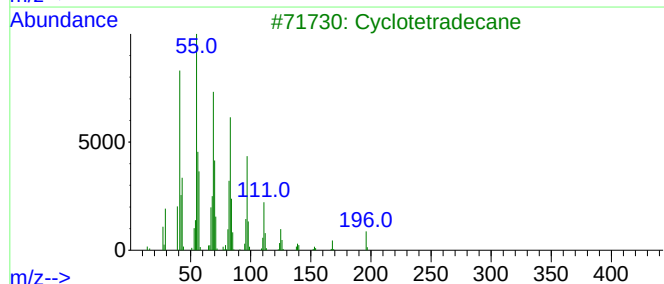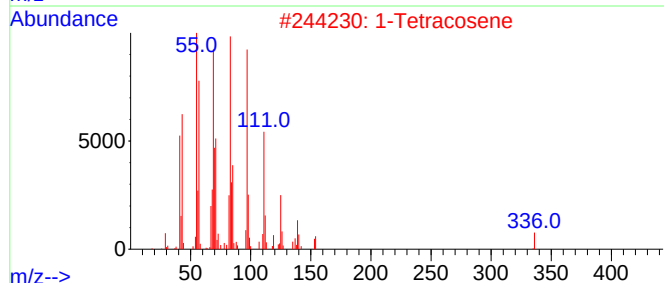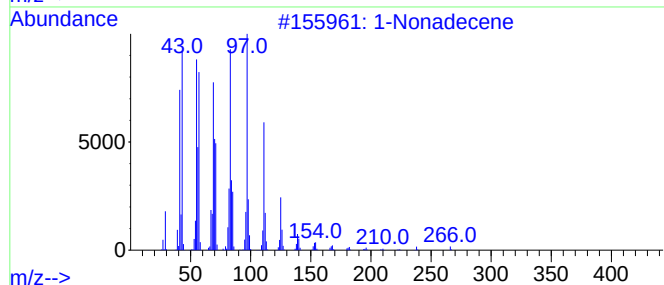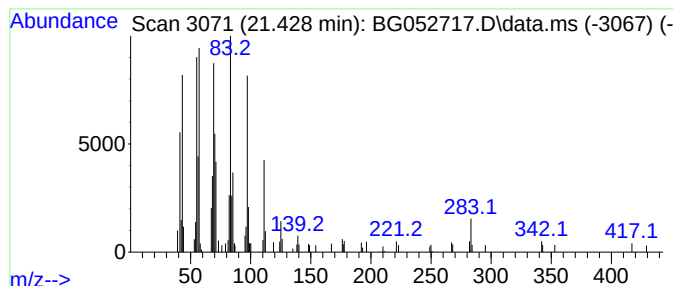

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052717.D
Acq On : 18 Mar 2022 19:39
Operator : CG/JU
Sample : N1882-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.428	2.5	ng/u1	86958	5	21.798	693404	20.0