

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052721.D
 Acq On : 18 Mar 2022 22:15
 Operator : CG/JU
 Sample : N1882-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.978	97	100	109	rBV	90725	156375	17.38%	1.683%
2	5.458	350	352	354	rVB2	2188	1529	0.17%	0.016%
3	6.051	450	453	455	rBV3	1044	1351	0.15%	0.015%
4	6.574	541	542	548	rVB5	1254	1473	0.16%	0.016%
5	6.803	579	581	584	rBV3	1251	1230	0.14%	0.013%
6	7.291	656	664	671	rBV	128964	225879	25.11%	2.431%
7	7.467	687	694	708	rBV	93527	167340	18.60%	1.801%
8	7.620	717	720	723	rBV2	1620	2632	0.29%	0.028%
9	7.679	723	730	737	rVB	121395	210040	23.35%	2.260%
10	8.149	803	810	817	rBV	131069	222203	24.70%	2.391%
11	8.460	862	863	868	rBV	1167	1394	0.15%	0.015%
12	8.842	920	928	936	rBV	147230	263769	29.32%	2.838%
13	9.306	998	1007	1015	rVB	117922	217037	24.12%	2.335%
14	9.435	1025	1029	1032	rVB3	1053	1454	0.16%	0.016%
15	9.752	1079	1083	1087	rBV4	4592	6739	0.75%	0.073%
16	10.034	1123	1131	1138	rBV	90376	158463	17.61%	1.705%
17	10.128	1143	1147	1149	rBV	1051	1849	0.21%	0.020%
18	10.575	1213	1223	1231	rBV	146657	268162	29.81%	2.886%
19	10.739	1249	1251	1258	rVB3	1468	2124	0.24%	0.023%
20	10.962	1281	1289	1299	rVB	169089	311854	34.66%	3.356%
21	11.086	1303	1310	1320	rBV	151357	276006	30.68%	2.970%
22	11.797	1429	1431	1435	rVB2	1817	1617	0.18%	0.017%
23	12.049	1473	1474	1480	rBV	997	1277	0.14%	0.014%
24	12.308	1516	1518	1522	rBV	1344	1421	0.16%	0.015%
25	12.372	1524	1529	1535	rVB4	5630	9078	1.01%	0.098%
26	12.531	1552	1556	1560	rBV2	3695	4867	0.54%	0.052%
27	12.995	1630	1635	1636	rBV	1094	1415	0.16%	0.015%
28	13.171	1662	1665	1669	rVB3	2075	2447	0.27%	0.026%
29	13.312	1686	1689	1692	rBV3	1915	2310	0.26%	0.025%
30	13.559	1728	1731	1733	rBV2	1204	1402	0.16%	0.015%
31	13.600	1733	1738	1744	rVB4	7837	10547	1.17%	0.113%
32	14.164	1828	1834	1844	rBV	282248	425671	47.32%	4.580%
33	14.246	1844	1848	1852	rVB2	1378	2363	0.26%	0.025%
34	14.464	1878	1885	1892	rBV	320461	510299	56.72%	5.491%
35	14.669	1917	1920	1922	rBV2	1791	1494	0.17%	0.016%
36	14.769	1929	1937	1944	rBV	277456	446203	49.60%	4.801%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052721.D
 Acq On : 18 Mar 2022 22:15
 Operator : CG/JU
 Sample : N1882-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBRX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	14.928	1956	1964	1974	rBV	127147	208456	23.17%	2.243%
38	15.386	2041	2042	2048	rVB2	1111	1307	0.15%	0.014%
39	15.568	2068	2073	2076	rBV4	1985	3122	0.35%	0.034%
40	15.615	2078	2081	2083	rVB2	1286	1401	0.16%	0.015%
41	15.656	2083	2088	2089	rBV	1043	1400	0.16%	0.015%
42	15.756	2098	2105	2112	rVB	413634	638043	70.92%	6.866%
43	15.856	2116	2122	2131	rBV2	98127	147764	16.42%	1.590%
44	16.009	2146	2148	2151	rVB2	1476	1318	0.15%	0.014%
45	16.273	2191	2193	2197	rVB2	1582	1818	0.20%	0.020%
46	16.561	2239	2242	2246	rBV2	1189	1977	0.22%	0.021%
47	16.902	2297	2300	2302	rVB2	1394	1377	0.15%	0.015%
48	17.037	2321	2323	2325	rBV2	1390	1313	0.15%	0.014%
49	17.113	2332	2336	2337	rBV	2290	1702	0.19%	0.018%
50	17.195	2347	2350	2351	rBV2	2187	1575	0.18%	0.017%
51	17.266	2358	2362	2364	rBV3	1631	1958	0.22%	0.021%
52	17.295	2364	2367	2368	rBV2	1399	1324	0.15%	0.014%
53	17.512	2397	2404	2412	rVB	386485	578444	64.30%	6.224%
54	17.606	2414	2420	2427	rVV2	458664	711641	79.10%	7.658%
55	17.689	2432	2434	2436	rVB3	3723	2465	0.27%	0.027%
56	18.170	2512	2516	2523	rBV5	7442	11151	1.24%	0.120%
57	18.264	2530	2532	2537	rVB3	3788	2412	0.27%	0.026%
58	18.341	2543	2545	2549	rVB3	2442	1534	0.17%	0.017%
59	18.388	2549	2553	2558	rBV4	24054	32955	3.66%	0.355%
60	18.552	2579	2581	2583	rVB3	2143	1586	0.18%	0.017%
61	18.652	2597	2598	2600	rVB	2568	1324	0.15%	0.014%
62	18.676	2600	2602	2605	rBV4	1782	2622	0.29%	0.028%
63	18.834	2627	2629	2631	rVB2	1953	1557	0.17%	0.017%
64	18.952	2647	2649	2650	rBV2	2687	1880	0.21%	0.020%
65	19.463	2731	2736	2739	rBV5	7616	11517	1.28%	0.124%
66	19.892	2803	2809	2821	rBV	629943	899652	100.00%	9.681%
67	21.795	3127	3133	3141	rVB	408689	682155	75.82%	7.340%
68	24.885	3651	3659	3671	rVB2	281166	833729	92.67%	8.971%
69	25.114	3690	3698	3707	rBV2	209767	579438	64.41%	6.235%




Sum of corrected areas: 9293231

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052721.D
Acq On : 18 Mar 2022 22:15
Operator : CG/JU
Sample : N1882-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

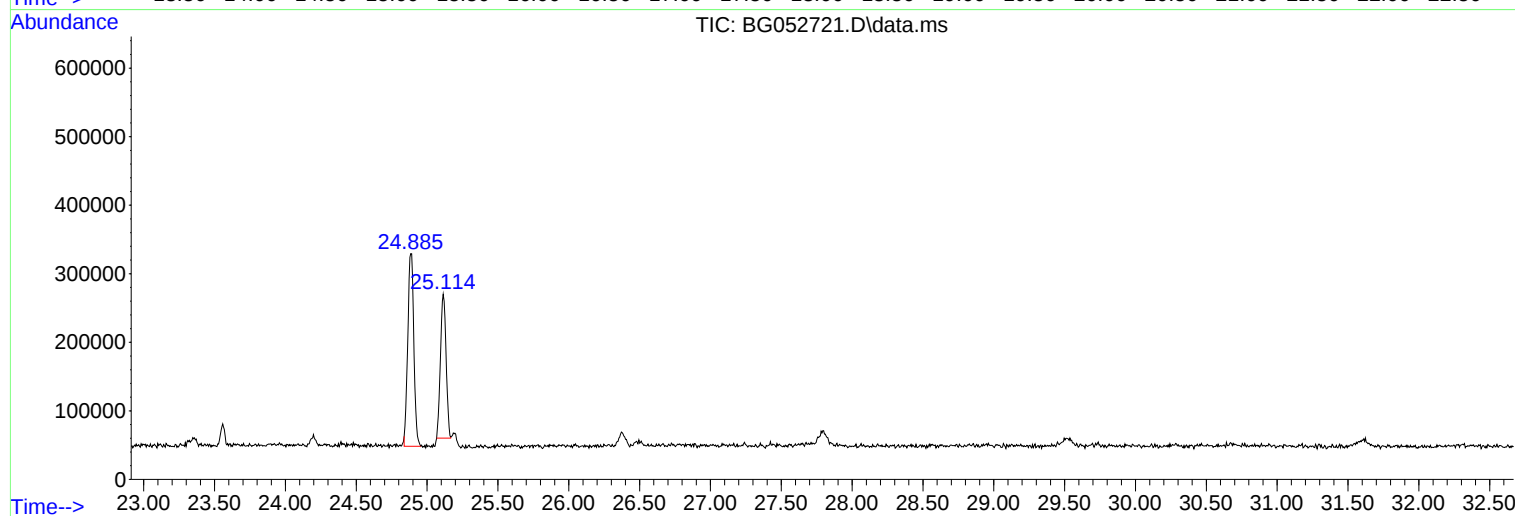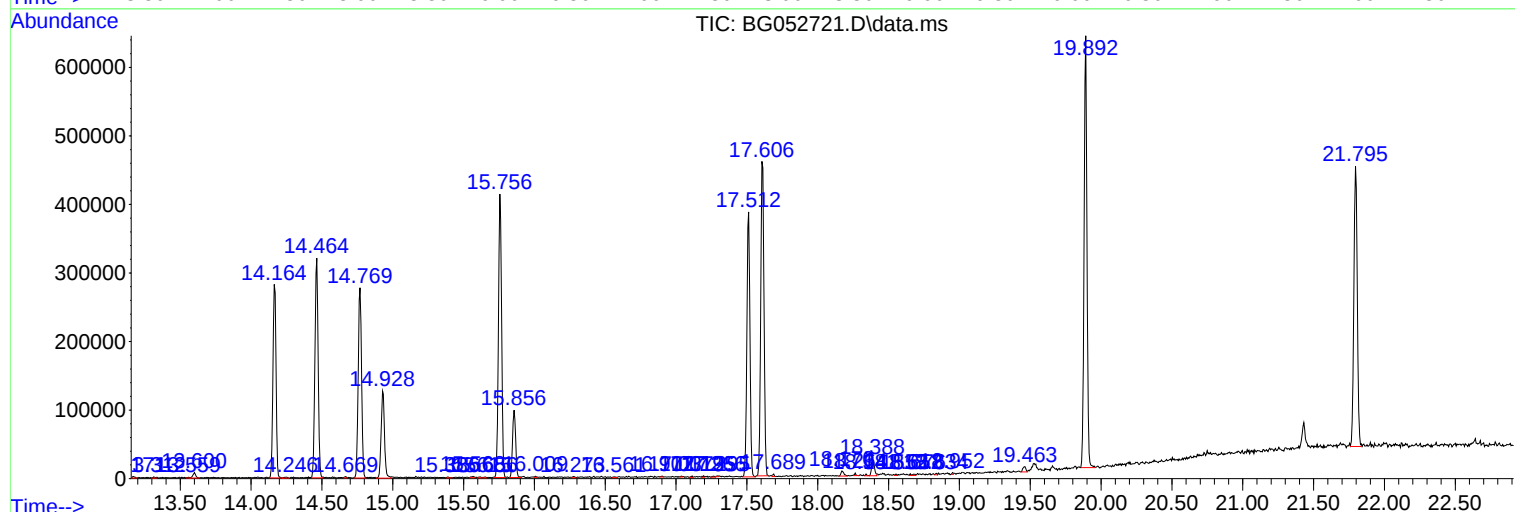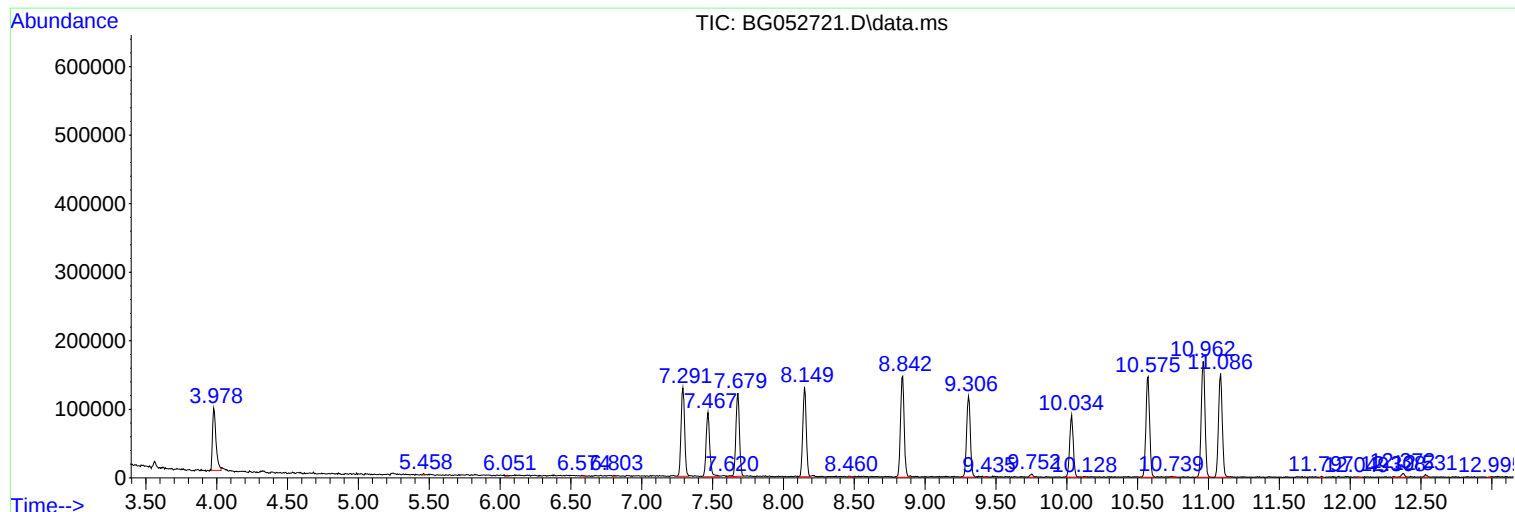

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052721.D
Acq On : 18 Mar 2022 22:15
Operator : CG/JU
Sample : N1882-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052721.D
Acq On : 18 Mar 2022 22:15
Operator : CG/JU
Sample : N1882-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBRX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc