

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052732.D
 Acq On : 19 Mar 2022 6:02
 Operator : CG/JU
 Sample : PB143360BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	6	8	9	rBV2	2664	1895	0.12%	0.013%
2	3.563	26	30	34	rBV2	13406	21174	1.38%	0.148%
3	3.728	56	58	59	rBV2	2134	1840	0.12%	0.013%
4	3.845	76	78	80	rBV3	2083	1803	0.12%	0.013%
5	3.892	84	86	89	rVB4	2085	2367	0.15%	0.017%
6	3.980	97	101	111	rBV	157358	280573	18.35%	1.967%
7	4.115	122	124	129	rVB5	3197	4571	0.30%	0.032%
8	4.162	129	132	133	rBV3	1605	1567	0.10%	0.011%
9	4.280	150	152	154	rBV3	1711	1701	0.11%	0.012%
10	4.321	155	159	166	rVB5	6794	9968	0.65%	0.070%
11	4.674	217	219	222	rVB3	1620	1540	0.10%	0.011%
12	4.773	233	236	242	rVB5	2528	5254	0.34%	0.037%
13	4.815	242	243	245	rBV2	2168	1753	0.11%	0.012%
14	4.832	245	246	251	rVV4	2626	2269	0.15%	0.016%
15	4.926	260	262	264	rVV2	1889	1672	0.11%	0.012%
16	5.008	274	276	278	rBV2	2182	1875	0.12%	0.013%
17	5.185	303	306	310	rVB4	1405	1696	0.11%	0.012%
18	5.478	353	356	357	rBV2	2012	1833	0.12%	0.013%
19	5.502	357	360	364	rVB4	1858	2980	0.19%	0.021%
20	5.931	431	433	437	rVB3	1424	1575	0.10%	0.011%
21	6.219	480	482	485	rVB4	1554	1910	0.12%	0.013%
22	6.254	485	488	490	rBV3	1440	1609	0.11%	0.011%
23	6.412	510	515	518	rBV4	1223	1933	0.13%	0.014%
24	6.724	565	568	572	rBV3	1428	1811	0.12%	0.013%
25	6.888	593	596	599	rBV4	1152	1821	0.12%	0.013%
26	7.023	617	619	625	rVB4	874	1536	0.10%	0.011%
27	7.288	657	664	673	rBV	216136	379851	24.84%	2.663%
28	7.464	688	694	705	rVV	154370	265936	17.39%	1.864%
29	7.675	723	730	738	rBV	199470	350603	22.93%	2.458%
30	7.910	768	770	773	rBV3	1615	1621	0.11%	0.011%
31	8.151	803	811	818	rVB	142527	252396	16.50%	1.769%
32	8.838	919	928	936	rVV2	256921	441909	28.90%	3.098%
33	9.062	961	966	967	rBV	1177	1571	0.10%	0.011%
34	9.132	972	978	981	rBV2	1379	2468	0.16%	0.017%
35	9.303	1000	1007	1015	rBV	192992	360804	23.59%	2.529%
36	9.367	1015	1018	1020	rVB2	1193	1533	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052732.D
 Acq On : 19 Mar 2022 6:02
 Operator : CG/JU
 Sample : PB143360BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	9.473	1031	1036	1038	rBV	1869	2049	0.13%	0.014%
38	9.943	1113	1116	1120	rVB4	1419	1664	0.11%	0.012%
39	10.031	1120	1131	1138	rBV	159747	281652	18.42%	1.974%
40	10.231	1162	1165	1169	rVB2	2128	1656	0.11%	0.012%
41	10.571	1215	1223	1231	rBV	254221	455681	29.80%	3.194%
42	10.959	1281	1289	1298	rVV	190244	354966	23.21%	2.488%
43	11.083	1302	1310	1319	rBV	242487	455419	29.78%	3.192%
44	11.312	1346	1349	1353	rBV2	1281	1953	0.13%	0.014%
45	12.533	1551	1557	1564	rBV4	6288	9026	0.59%	0.063%
46	13.515	1719	1724	1726	rBV2	958	1567	0.10%	0.011%
47	14.167	1828	1835	1842	rBV	479578	696962	45.58%	4.886%
48	14.460	1876	1885	1892	rVV	523497	832224	54.42%	5.834%
49	14.766	1930	1937	1945	rBV	306536	494797	32.36%	3.468%
50	14.930	1958	1965	1973	rVV	255388	391725	25.62%	2.746%
51	14.983	1973	1974	1979	rVB3	2764	2867	0.19%	0.020%
52	15.759	2096	2106	2115	rVB	652181	1022464	66.86%	7.167%
53	15.858	2116	2123	2130	rBV	201306	292610	19.13%	2.051%
54	16.005	2143	2148	2150	rVV4	2241	3271	0.21%	0.023%
55	16.258	2190	2191	2198	rVB2	1649	1812	0.12%	0.013%
56	16.428	2217	2220	2224	rVB3	1404	2018	0.13%	0.014%
57	17.292	2363	2367	2370	rBV4	2768	4280	0.28%	0.030%
58	17.368	2376	2380	2382	rBV3	1967	2533	0.17%	0.018%
59	17.509	2397	2404	2411	rBV	436613	662874	43.35%	4.647%
60	17.609	2415	2421	2428	rVV	771956	1189576	77.79%	8.339%
61	17.709	2435	2438	2439	rBV2	1479	1565	0.10%	0.011%
62	17.773	2448	2449	2454	rVB5	1576	1836	0.12%	0.013%
63	17.873	2464	2466	2469	rVV2	2418	3242	0.21%	0.023%
64	18.008	2486	2489	2493	rVV4	1437	1770	0.12%	0.012%
65	18.044	2493	2495	2498	rVB4	1503	1699	0.11%	0.012%
66	18.067	2498	2499	2502	rBV3	1656	1686	0.11%	0.012%
67	18.514	2574	2575	2578	rVB2	2589	2279	0.15%	0.016%
68	18.549	2578	2581	2584	rBV4	2339	3005	0.20%	0.021%
69	18.572	2584	2585	2588	rBV2	2184	1905	0.12%	0.013%
70	18.660	2597	2600	2602	rBV3	2287	2702	0.18%	0.019%
71	18.919	2641	2644	2647	rVB4	2528	3059	0.20%	0.021%
72	19.007	2658	2659	2663	rBV4	1671	1889	0.12%	0.013%
73	19.459	2731	2736	2739	rVB3	11848	15464	1.01%	0.108%
74	19.524	2743	2747	2753	rBV	12361	18435	1.21%	0.129%
75	19.577	2755	2756	2758	rBV2	2992	2346	0.15%	0.016%
76	19.671	2770	2772	2775	rBV3	2671	3212	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052732.D
Acq On : 19 Mar 2022 6:02
Operator : CG/JU
Sample : PB143360BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK360

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Title : SVOA CALIBRATION

77	19.888	2803	2809	2816	rVB	1027776	1529261	100.00%	10.720%
78	20.511	2913	2915	2917	rVB3	4383	2559	0.17%	0.018%
79	20.605	2929	2931	2933	rBV3	4932	4609	0.30%	0.032%
80	21.057	3006	3008	3009	rBV2	5705	4285	0.28%	0.030%
81	21.797	3127	3134	3142	rVB	509736	841105	55.00%	5.896%
82	24.887	3649	3660	3676	rVB2	513687	1481004	96.84%	10.381%
83	25.116	3689	3699	3709	rBV2	260908	752133	49.18%	5.272%




Sum of corrected areas: 14265914

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052732.D
Acq On : 19 Mar 2022 6:02
Operator : CG/JU
Sample : PB143360BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK360

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

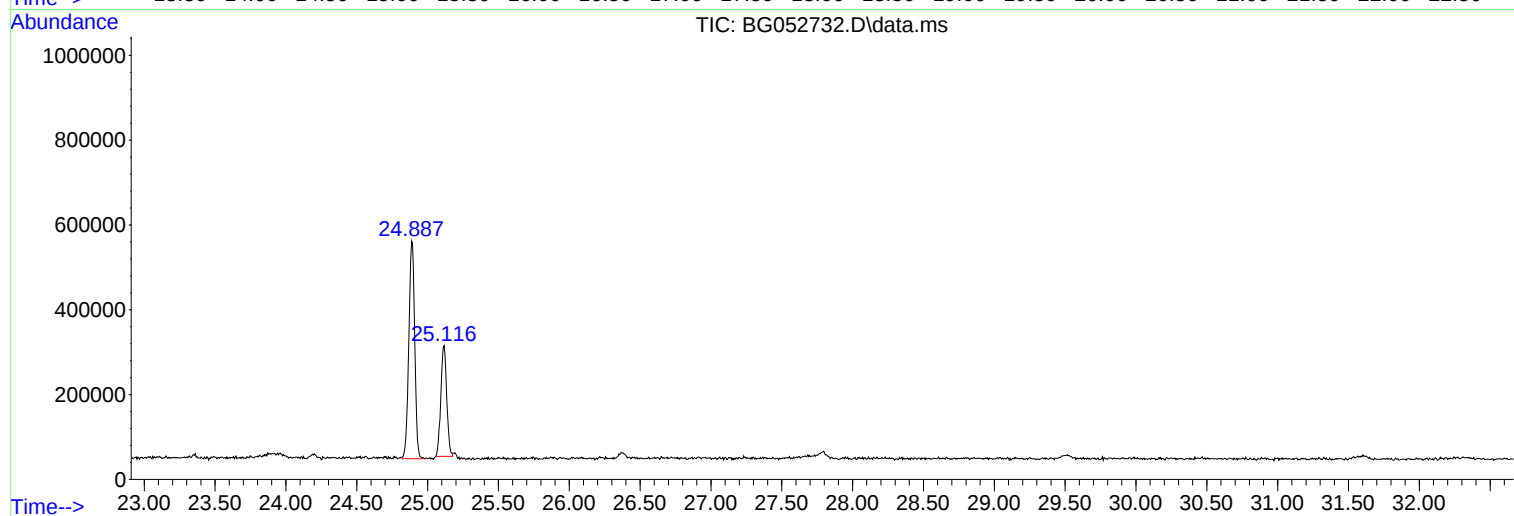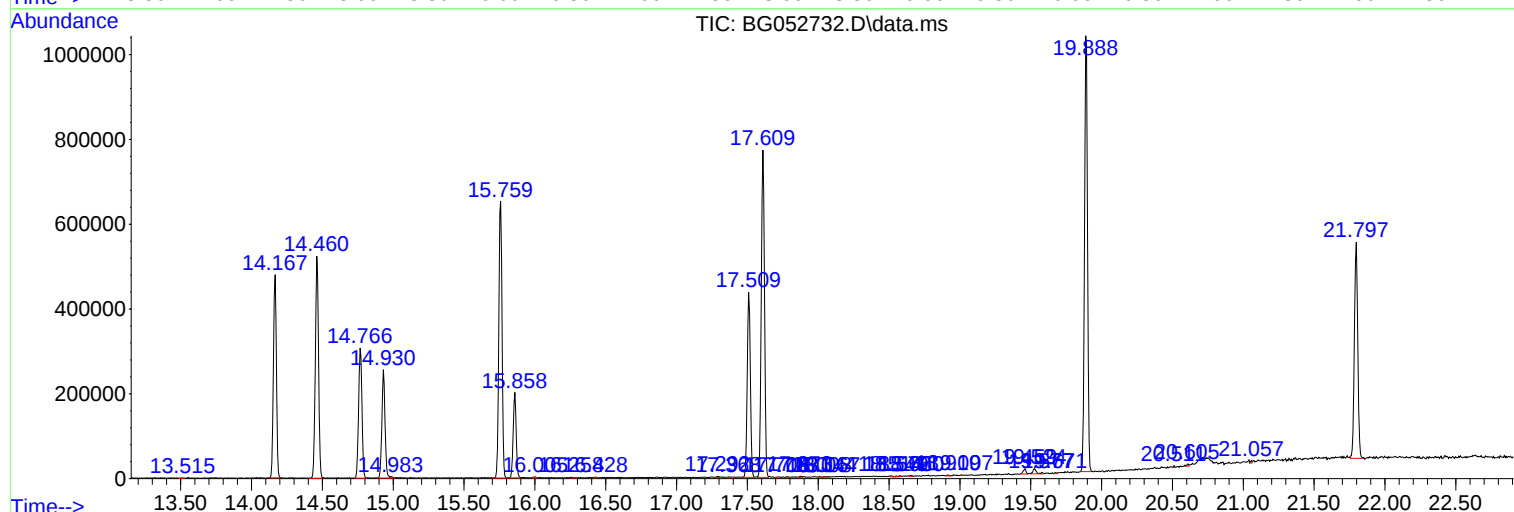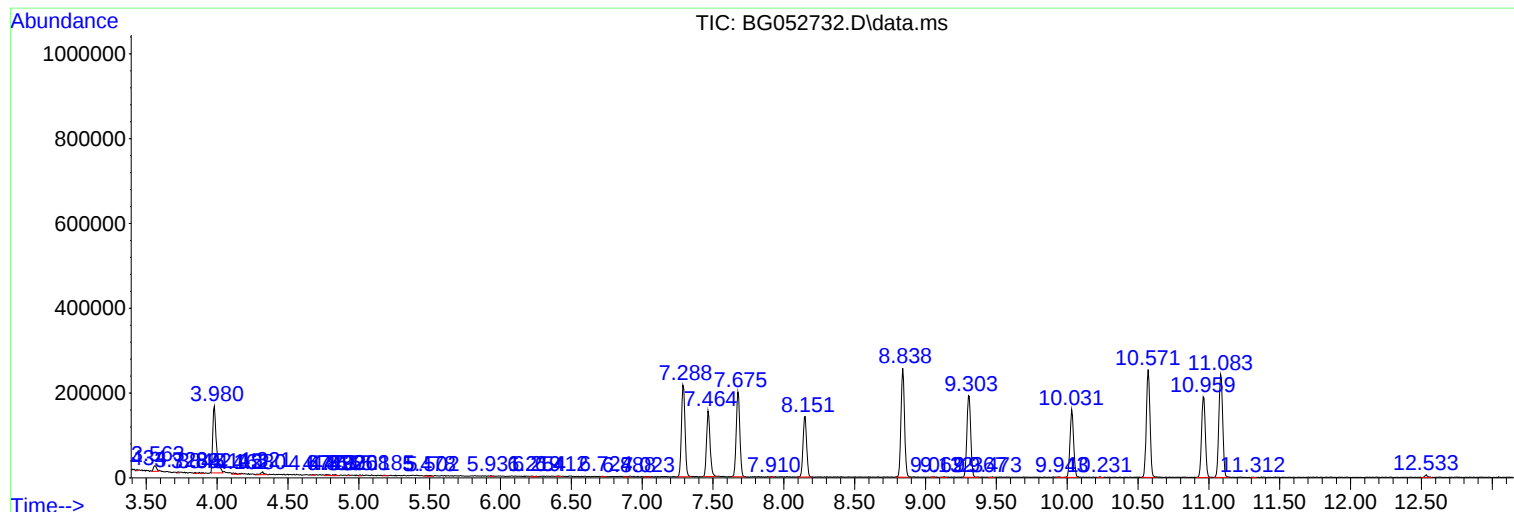

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052732.D
Acq On : 19 Mar 2022 6:02
Operator : CG/JU
Sample : PB143360BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK360

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052732.D
Acq On : 19 Mar 2022 6:02
Operator : CG/JU
Sample : PB143360BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK360

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc