

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052733.D
 Acq On : 19 Mar 2022 6:41
 Operator : CG/JU
 Sample : N1883-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.981	97	101	113	rBV	102557	182250	18.60%	1.737%
2	4.598	205	206	209	rBV2	2770	2983	0.30%	0.028%
3	6.013	445	447	451	rVB3	1549	1519	0.16%	0.014%
4	6.436	515	519	521	rBV3	1472	1971	0.20%	0.019%
5	6.812	579	583	588	rBV5	1402	2202	0.22%	0.021%
6	7.006	613	616	619	rBV3	1840	2262	0.23%	0.022%
7	7.288	657	664	675	rVB	153215	282143	28.79%	2.689%
8	7.464	688	694	704	rBV	107031	182403	18.61%	1.739%
9	7.570	709	712	714	rVB3	1860	2200	0.22%	0.021%
10	7.676	723	730	737	rVV	143123	246099	25.11%	2.346%
11	7.729	737	739	744	rVB3	1403	1510	0.15%	0.014%
12	7.881	763	765	767	rBV2	1604	1709	0.17%	0.016%
13	7.964	776	779	782	rBV2	1256	1677	0.17%	0.016%
14	8.146	802	810	818	rVB	144044	255673	26.09%	2.437%
15	8.669	896	899	901	rBV2	1364	1378	0.14%	0.013%
16	8.839	920	928	937	rVB	175028	304364	31.06%	2.901%
17	8.962	946	949	952	rVB	1966	2563	0.26%	0.024%
18	8.992	952	954	957	rBV2	1466	1999	0.20%	0.019%
19	9.303	999	1007	1015	rBV	139776	251721	25.69%	2.399%
20	9.479	1033	1037	1041	rVB4	2610	3040	0.31%	0.029%
21	9.738	1079	1081	1087	rVB3	1972	2730	0.28%	0.026%
22	10.032	1124	1131	1142	rVB	106094	193551	19.75%	1.845%
23	10.126	1142	1147	1148	rBV3	938	1335	0.14%	0.013%
24	10.319	1177	1180	1185	rVB2	1050	1607	0.16%	0.015%
25	10.572	1214	1223	1231	rBV	179258	311138	31.75%	2.966%
26	10.731	1244	1250	1254	rBV4	4242	6511	0.66%	0.062%
27	10.807	1261	1263	1267	rVB3	1584	1404	0.14%	0.013%
28	10.960	1280	1289	1298	rBV	194855	357416	36.47%	3.407%
29	11.083	1300	1310	1319	rVB	167709	308811	31.51%	2.943%
30	11.324	1346	1351	1352	rBV4	1137	1610	0.16%	0.015%
31	12.540	1552	1558	1560	rBV4	2809	3905	0.40%	0.037%
32	13.139	1656	1660	1664	rBV2	990	1408	0.14%	0.013%
33	13.321	1688	1691	1695	rBV2	1632	2104	0.21%	0.020%
34	13.597	1734	1738	1742	rVB4	4047	5445	0.56%	0.052%
35	14.161	1828	1834	1842	rBV	313442	476188	48.59%	4.539%
36	14.302	1856	1858	1860	rVB2	1422	1308	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052733.D
 Acq On : 19 Mar 2022 6:41
 Operator : CG/JU
 Sample : N1883-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	14.402	1871	1875	1878	rBV5	4246	4950	0.51%	0.047%
38	14.461	1878	1885	1892	rVB	361546	571324	58.30%	5.445%
39	14.549	1898	1900	1903	rVB2	1236	1324	0.14%	0.013%
40	14.661	1916	1919	1923	rBV2	2825	3940	0.40%	0.038%
41	14.766	1931	1937	1944	rBV	310732	500299	51.05%	4.769%
42	14.931	1959	1965	1972	rBV2	145285	227367	23.20%	2.167%
43	15.160	2002	2004	2009	rVB2	1886	2216	0.23%	0.021%
44	15.277	2022	2024	2027	rVB2	1635	1480	0.15%	0.014%
45	15.389	2042	2043	2049	rVB2	2306	2912	0.30%	0.028%
46	15.565	2069	2073	2076	rBV3	5674	6541	0.67%	0.062%
47	15.612	2078	2081	2083	rVV4	1743	1654	0.17%	0.016%
48	15.759	2099	2106	2113	rVB	458920	707630	72.21%	6.745%
49	15.859	2116	2123	2133	rVB	110061	169038	17.25%	1.611%
50	16.000	2142	2147	2149	rBV2	2992	3373	0.34%	0.032%
51	16.164	2171	2175	2176	rVB2	2513	1903	0.19%	0.018%
52	16.235	2185	2187	2191	rVB4	1471	1479	0.15%	0.014%
53	16.294	2196	2197	2201	rVB2	2123	1822	0.19%	0.017%
54	16.393	2211	2214	2217	rBV2	1632	2034	0.21%	0.019%
55	16.628	2251	2254	2255	rBV3	1848	1681	0.17%	0.016%
56	16.640	2255	2256	2263	rVB4	2352	4036	0.41%	0.038%
57	16.752	2272	2275	2280	rBV3	1185	2034	0.21%	0.019%
58	16.922	2301	2304	2305	rBV2	1851	1772	0.18%	0.017%
59	17.222	2353	2355	2357	rBV2	1718	1302	0.13%	0.012%
60	17.263	2357	2362	2363	rVV4	3216	3685	0.38%	0.035%
61	17.392	2380	2384	2385	rBV	1331	1681	0.17%	0.016%
62	17.410	2385	2387	2393	rVB6	2763	3945	0.40%	0.038%
63	17.510	2397	2404	2411	rBV	439216	645919	65.91%	6.156%
64	17.609	2414	2421	2428	rBV2	516199	787069	80.31%	7.502%
65	17.792	2449	2452	2455	rBV4	2401	3420	0.35%	0.033%
66	17.880	2465	2467	2469	rVB3	1798	1465	0.15%	0.014%
67	18.085	2499	2502	2503	rBV2	2261	2328	0.24%	0.022%
68	18.121	2506	2508	2509	rBV	1942	1495	0.15%	0.014%
69	18.179	2513	2518	2520	rBV5	3518	5302	0.54%	0.051%
70	18.385	2549	2553	2559	rBV7	13929	21039	2.15%	0.201%
71	18.467	2562	2567	2572	rBV4	6746	10389	1.06%	0.099%
72	18.596	2587	2589	2592	rVB5	2155	2007	0.20%	0.019%
73	18.743	2612	2614	2615	rBV2	2279	1737	0.18%	0.017%
74	18.814	2625	2626	2628	rBV2	2297	1518	0.15%	0.014%
75	18.931	2645	2646	2648	rVB2	2736	1476	0.15%	0.014%
76	19.002	2656	2658	2663	rVB6	3298	4468	0.46%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052733.D
Acq On : 19 Mar 2022 6:41
Operator : CG/JU
Sample : N1883-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Title : SVOA CALIBRATION

77	19.460	2732	2736	2740	rBV7	8075	11920	1.22%	0.114%
78	19.525	2744	2747	2753	rBV2	6768	13593	1.39%	0.130%
79	19.636	2764	2766	2767	rBV	3619	2383	0.24%	0.023%
80	19.654	2767	2769	2772	rVV4	4386	4408	0.45%	0.042%
81	19.889	2803	2809	2816	rVB	655874	979992	100.00%	9.341%
82	21.798	3128	3134	3141	rVB	432486	751529	76.69%	7.163%
83	24.888	3651	3660	3671	rVB	332061	927597	94.65%	8.841%
84	25.117	3690	3699	3707	rBV2	240034	671065	68.48%	6.396%




Sum of corrected areas: 10491678

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052733.D
Acq On : 19 Mar 2022 6:41
Operator : CG/JU
Sample : N1883-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

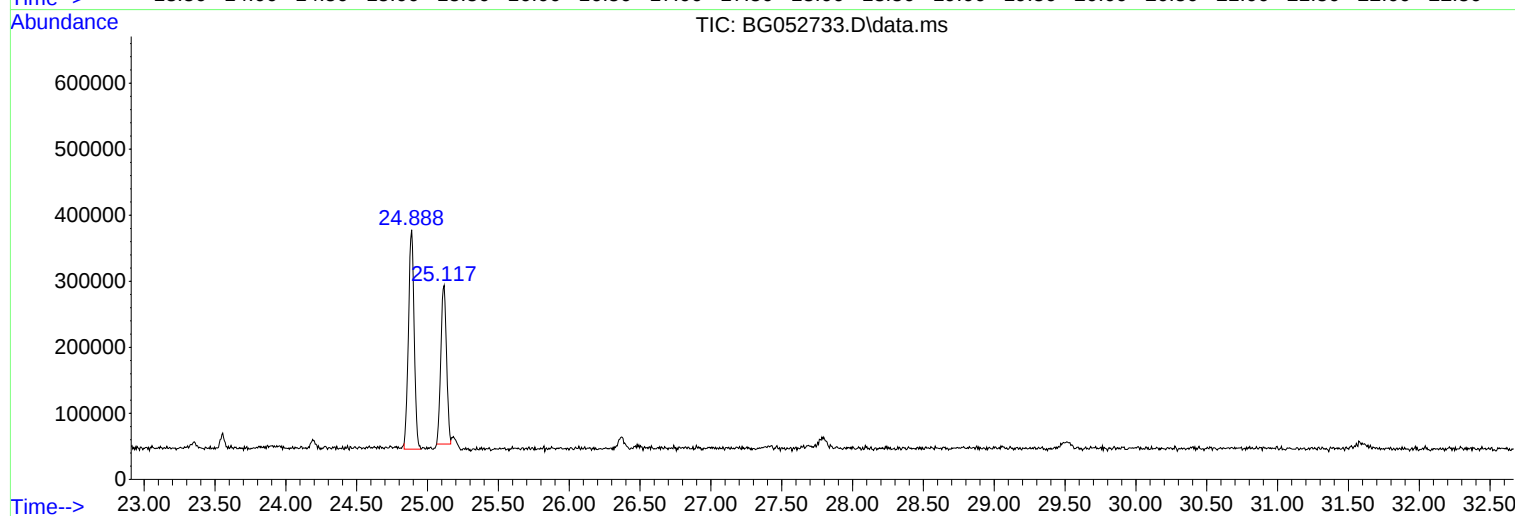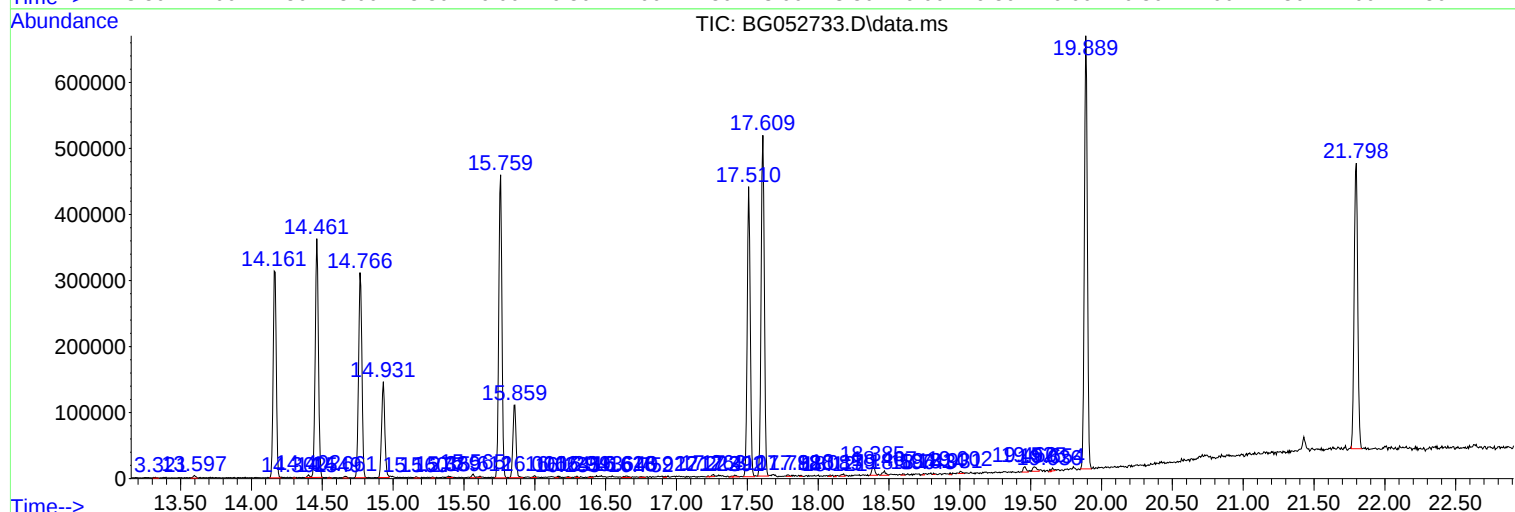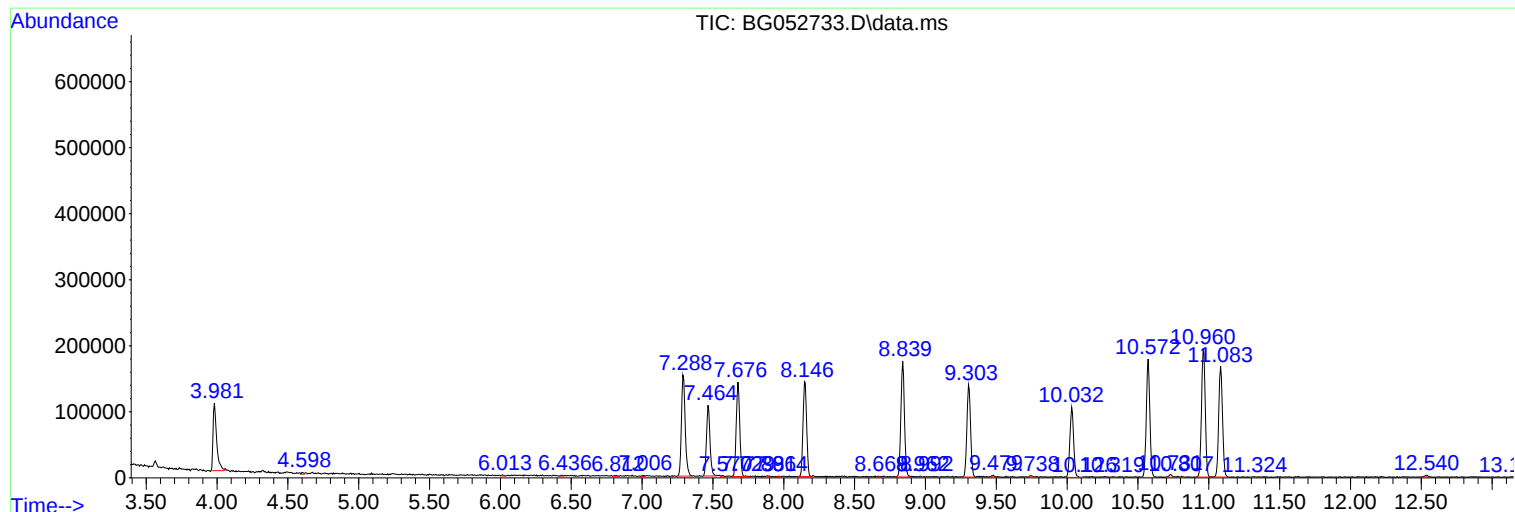

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052733.D
Acq On : 19 Mar 2022 6:41
Operator : CG/JU
Sample : N1883-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052733.D
Acq On : 19 Mar 2022 6:41
Operator : CG/JU
Sample : N1883-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc