

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052742.D
 Acq On : 19 Mar 2022 12:30
 Operator : CG/JU
 Sample : N1883-13
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.980	97	101	110	rBV	108913	184644	17.22%	1.633%
2	4.903	256	258	260	rVB3	2366	1544	0.14%	0.014%
3	5.655	385	386	390	rVB4	2132	1916	0.18%	0.017%
4	6.171	472	474	477	rBV2	1629	2072	0.19%	0.018%
5	7.100	631	632	637	rBV3	1580	2157	0.20%	0.019%
6	7.288	657	664	677	rVB	157037	293865	27.41%	2.600%
7	7.411	682	685	688	rBV4	900	1692	0.16%	0.015%
8	7.464	688	694	703	rBV	107632	190980	17.82%	1.689%
9	7.675	723	730	741	rVB	148285	252837	23.59%	2.237%
10	8.145	803	810	818	rBV	142209	247212	23.06%	2.187%
11	8.216	818	822	824	rVV4	1224	1582	0.15%	0.014%
12	8.439	857	860	864	rBV3	1176	1483	0.14%	0.013%
13	8.515	871	873	878	rVB4	1054	1575	0.15%	0.014%
14	8.838	919	928	937	rVB2	192636	327056	30.51%	2.893%
15	9.303	1000	1007	1016	rBV	145593	264388	24.66%	2.339%
16	9.473	1030	1036	1039	rBV4	3323	5451	0.51%	0.048%
17	9.749	1076	1083	1087	rBV4	5065	8342	0.78%	0.074%
18	10.031	1123	1131	1140	rBV	115780	208077	19.41%	1.841%
19	10.436	1198	1200	1202	rBV2	1343	1513	0.14%	0.013%
20	10.571	1216	1223	1232	rVB	188752	331359	30.91%	2.931%
21	10.730	1244	1250	1257	rBV2	7178	12233	1.14%	0.108%
22	10.959	1282	1289	1298	rVB	202383	356521	33.26%	3.154%
23	11.082	1303	1310	1317	rVB	172354	318146	29.68%	2.814%
24	11.306	1346	1348	1353	rBV3	1098	1733	0.16%	0.015%
25	11.411	1363	1366	1369	rBV2	1238	1900	0.18%	0.017%
26	12.375	1527	1530	1534	rVB2	1312	1818	0.17%	0.016%
27	12.533	1552	1557	1561	rBV2	3663	6774	0.63%	0.060%
28	13.144	1655	1661	1664	rBV	1486	2490	0.23%	0.022%
29	13.168	1664	1665	1669	rVB	1389	1481	0.14%	0.013%
30	13.379	1696	1701	1707	rBV2	2709	4908	0.46%	0.043%
31	13.514	1720	1724	1726	rBV2	1721	1925	0.18%	0.017%
32	13.597	1733	1738	1743	rVB2	5201	7095	0.66%	0.063%
33	14.161	1828	1834	1841	rBV	344627	510775	47.65%	4.518%
34	14.296	1851	1857	1858	rBV2	1175	1729	0.16%	0.015%
35	14.402	1870	1875	1879	rBV5	8005	13393	1.25%	0.118%
36	14.460	1879	1885	1896	rVB	396966	613144	57.20%	5.424%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052742.D
 Acq On : 19 Mar 2022 12:30
 Operator : CG/JU
 Sample : N1883-13
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	14.660	1915	1919	1923	rVB3	4340	5600	0.52%	0.050%
38	14.766	1930	1937	1945	rVB	317235	513980	47.95%	4.547%
39	14.930	1958	1965	1973	rBV	139954	228638	21.33%	2.023%
40	15.001	1975	1977	1983	rVB2	2825	3532	0.33%	0.031%
41	15.165	1999	2005	2009	rBV3	2322	3728	0.35%	0.033%
42	15.277	2021	2024	2028	rBV3	1836	2081	0.19%	0.018%
43	15.394	2041	2044	2048	rBV2	6115	6350	0.59%	0.056%
44	15.559	2066	2072	2077	rBV5	6854	12472	1.16%	0.110%
45	15.612	2077	2081	2084	rVB4	3613	5653	0.53%	0.050%
46	15.753	2098	2105	2112	rBV	490157	772655	72.08%	6.835%
47	15.858	2116	2123	2129	rBV	110427	169386	15.80%	1.498%
48	15.999	2143	2147	2150	rVB4	2881	4397	0.41%	0.039%
49	16.117	2162	2167	2169	rBV2	1927	3608	0.34%	0.032%
50	16.164	2172	2175	2179	rVV2	3533	4144	0.39%	0.037%
51	16.223	2183	2185	2189	rVB3	1687	2328	0.22%	0.021%
52	16.281	2194	2195	2201	rVB3	1875	3311	0.31%	0.029%
53	16.387	2211	2213	2214	rBV2	2070	1501	0.14%	0.013%
54	16.428	2218	2220	2224	rVV5	2581	4033	0.38%	0.036%
55	16.469	2224	2227	2230	rVB5	4693	5474	0.51%	0.048%
56	16.646	2253	2257	2260	rVB3	4085	5135	0.48%	0.045%
57	16.810	2281	2285	2286	rBV2	1825	1822	0.17%	0.016%
58	16.875	2294	2296	2299	rBV3	2175	2991	0.28%	0.026%
59	16.980	2310	2314	2316	rBV4	4769	4615	0.43%	0.041%
60	17.057	2323	2327	2329	rBV4	2270	3486	0.33%	0.031%
61	17.086	2329	2332	2336	rVV5	1652	2657	0.25%	0.024%
62	17.121	2336	2338	2341	rVB3	1886	1899	0.18%	0.017%
63	17.209	2350	2353	2357	rBV4	1905	3107	0.29%	0.027%
64	17.256	2358	2361	2365	rVV4	6613	7828	0.73%	0.069%
65	17.292	2365	2367	2369	rBV3	1980	2096	0.20%	0.019%
66	17.397	2381	2385	2386	rBV3	2753	3739	0.35%	0.033%
67	17.421	2386	2389	2394	rVB4	8101	10429	0.97%	0.092%
68	17.509	2397	2404	2412	rVV	426762	658801	61.45%	5.828%
69	17.609	2415	2421	2428	rVB2	581584	863757	80.57%	7.641%
70	17.674	2430	2432	2433	rBV2	2879	2423	0.23%	0.021%
71	17.785	2448	2451	2452	rBV2	2179	2049	0.19%	0.018%
72	17.873	2463	2466	2467	rBV3	2694	2972	0.28%	0.026%
73	18.003	2484	2488	2489	rBV3	2942	2496	0.23%	0.022%
74	18.167	2513	2516	2523	rVB6	6137	8851	0.83%	0.078%
75	18.390	2549	2554	2561	rBV2	33990	52388	4.89%	0.463%
76	18.602	2588	2590	2592	rVB2	3073	2125	0.20%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052742.D
 Acq On : 19 Mar 2022 12:30
 Operator : CG/JU
 Sample : N1883-13
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBSB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	18.690	2602	2605	2606	rBV2	3372	3439	0.32%	0.030%
78	18.819	2623	2627	2629	rBV5	8711	8553	0.80%	0.076%
79	19.154	2682	2684	2686	rBV3	4433	4226	0.39%	0.037%
80	19.453	2732	2735	2738	rBV5	8378	10582	0.99%	0.094%
81	19.653	2766	2769	2774	rBV6	12647	18294	1.71%	0.162%
82	19.759	2785	2787	2788	rBV2	4884	2702	0.25%	0.024%
83	19.888	2803	2809	2816	rBV	739569	1072006	100.00%	9.483%
84	21.427	3067	3071	3076	rBV4	64322	88012	8.21%	0.779%
85	21.797	3127	3134	3141	rBV	464429	786427	73.36%	6.957%
86	24.887	3651	3660	3670	rVB2	355231	1014094	94.60%	8.971%
87	25.116	3690	3699	3710	rBV2	244183	711955	66.41%	6.298%




Sum of corrected areas: 11304637

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052742.D
Acq On : 19 Mar 2022 12:30
Operator : CG/JU
Sample : N1883-13
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

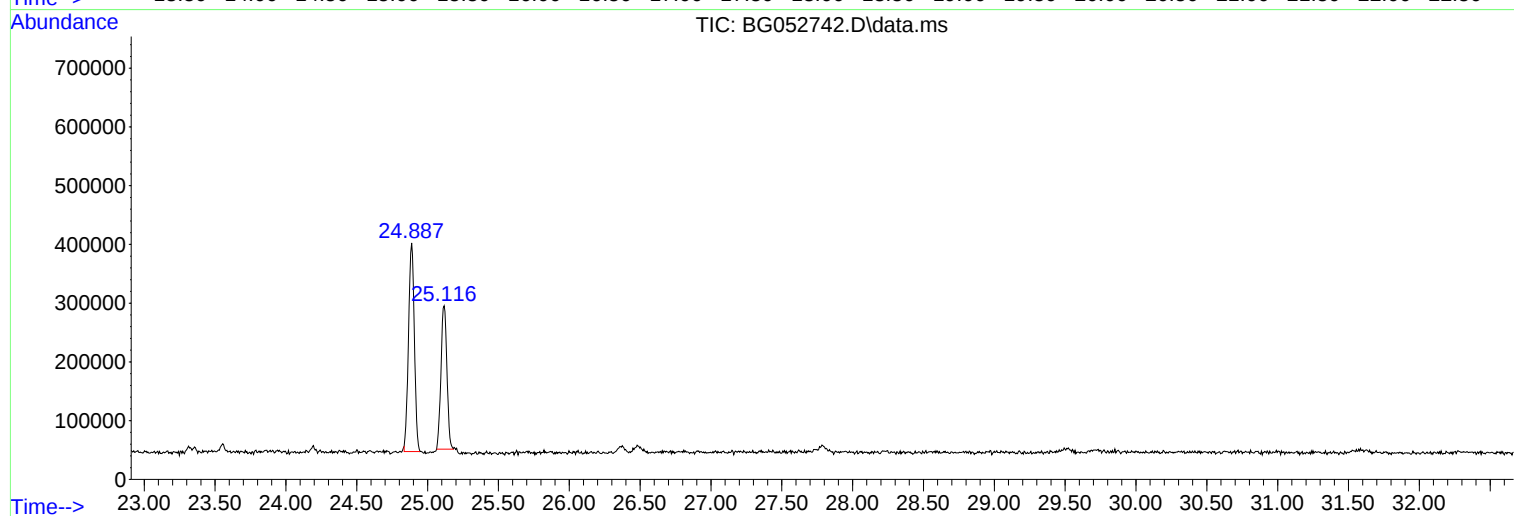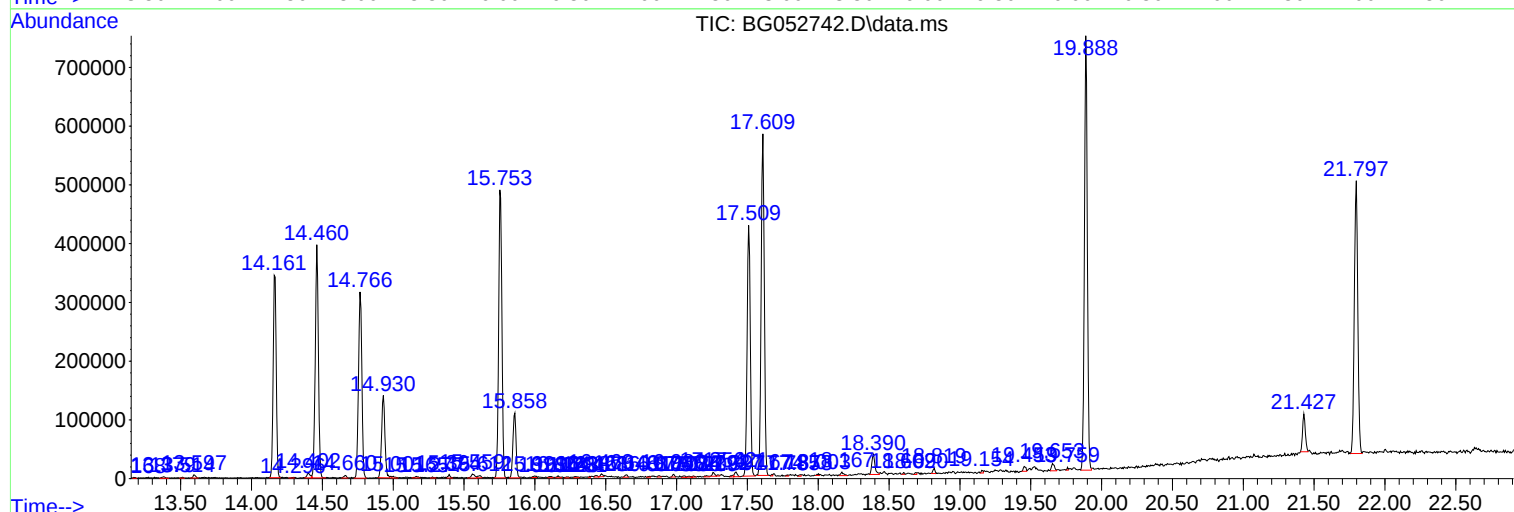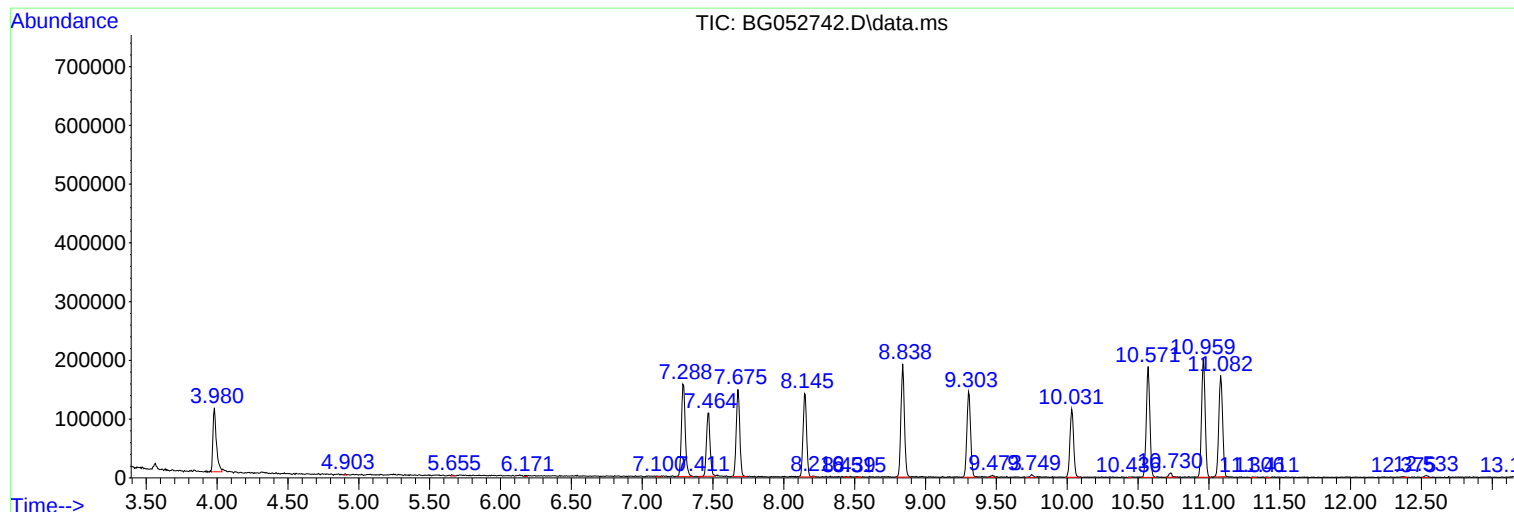

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052742.D
Acq On : 19 Mar 2022 12:30
Operator : CG/JU
Sample : N1883-13
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSB0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.427	2.24 ng/ul	88012	Chrysene-d12	21.797

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Tricosene			322	C23H46	018835-32-0	90
2	1-Heptadecene			238	C17H34	006765-39-5	76
3	1-Heptadecene			238	C17H34	006765-39-5	76
4	3-Eicosene, (E)-			280	C20H40	074685-33-9	74
5	Trifluoroacetoxy hexadecane			338	C18H33F3O2	006222-03-3	70

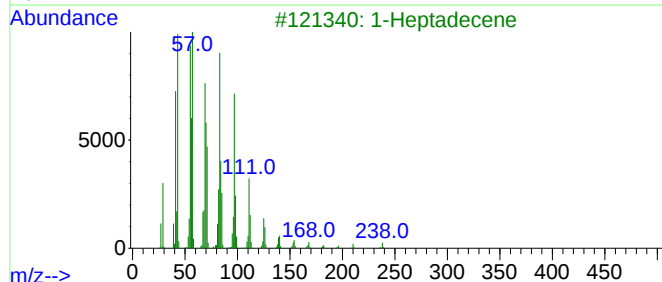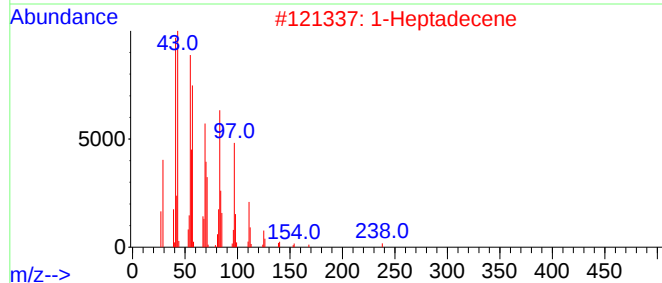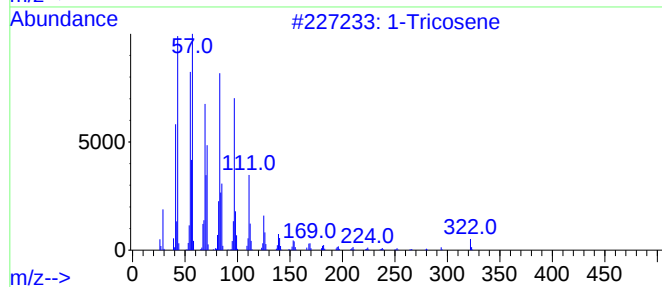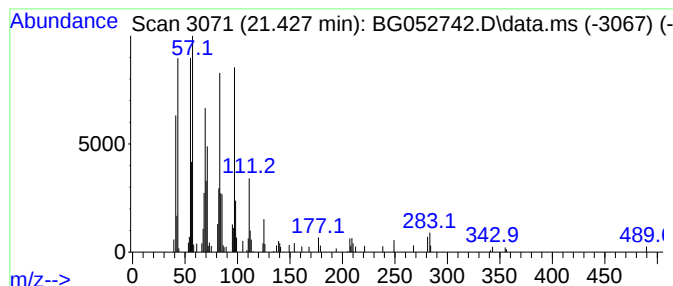

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052742.D
Acq On : 19 Mar 2022 12:30
Operator : CG/JU
Sample : N1883-13
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBSB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.427	2.2	ng/u1	88012	5	21.797	786427	20.0