

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052747.D
 Acq On : 19 Mar 2022 16:23
 Operator : CG/JU
 Sample : PB143280BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.560	24	29	34	rBV4	12826	19512	1.36%	0.147%
2	3.977	96	100	109	rBV	144473	244316	17.08%	1.846%
3	4.248	143	146	149	rBV4	1795	2056	0.14%	0.016%
4	4.318	154	158	159	rBV4	3379	3512	0.25%	0.027%
5	4.488	184	187	191	rVB2	1885	2546	0.18%	0.019%
6	4.947	264	265	268	rBV2	1465	1496	0.10%	0.011%
7	5.035	279	280	286	rBV5	1139	1691	0.12%	0.013%
8	5.405	341	343	346	rVB4	1480	1488	0.10%	0.011%
9	5.587	371	374	376	rVB3	1514	1561	0.11%	0.012%
10	5.616	376	379	381	rBV3	1359	1448	0.10%	0.011%
11	6.180	473	475	477	rBV3	1657	1540	0.11%	0.012%
12	6.280	488	492	496	rBV2	1331	2420	0.17%	0.018%
13	7.014	614	617	618	rBV2	1510	1565	0.11%	0.012%
14	7.290	657	664	672	rVV	196171	342564	23.95%	2.588%
15	7.467	686	694	703	rBV	133924	241411	16.88%	1.824%
16	7.678	722	730	739	rBV	177442	313675	21.93%	2.370%
17	8.148	803	810	817	rVB	133421	224799	15.72%	1.699%
18	8.283	830	833	835	rBV3	1450	1539	0.11%	0.012%
19	8.835	920	927	936	rBV	225350	396043	27.69%	2.993%
20	8.965	946	949	952	rBV2	1236	1918	0.13%	0.014%
21	9.235	992	995	998	rBV2	1547	1969	0.14%	0.015%
22	9.305	1000	1007	1016	rVV	178039	327177	22.87%	2.472%
23	9.364	1016	1017	1022	rVB4	1431	1657	0.12%	0.013%
24	10.034	1123	1131	1139	rVB	147563	258725	18.09%	1.955%
25	10.568	1215	1222	1231	rVB	228251	408573	28.57%	3.087%
26	10.962	1282	1289	1296	rVB2	174222	320637	22.42%	2.423%
27	11.085	1300	1310	1319	rBV	226419	416485	29.12%	3.147%
28	11.814	1427	1434	1437	rBV2	983	1792	0.13%	0.014%
29	12.536	1552	1557	1561	rBV	5568	9011	0.63%	0.068%
30	13.083	1647	1650	1654	rVB2	1088	1520	0.11%	0.011%
31	13.517	1720	1724	1727	rVB2	1457	2085	0.15%	0.016%
32	13.547	1727	1729	1732	rBV	1184	1677	0.12%	0.013%
33	14.163	1827	1834	1841	rBV	472240	672346	47.01%	5.080%
34	14.463	1877	1885	1892	rBV	473071	774707	54.16%	5.854%
35	14.769	1930	1937	1945	rVB	298300	481352	33.65%	3.637%
36	14.933	1958	1965	1973	rBV	235173	369493	25.83%	2.792%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
 Data File : BG052747.D
 Acq On : 19 Mar 2022 16:23
 Operator : CG/JU
 Sample : PB143280BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.015	1977	1979	1982	rVV2	1677	1558	0.11%	0.012%
38	15.562	2069	2072	2076	rBV2	1552	1856	0.13%	0.014%
39	15.755	2099	2105	2115	rVB	647541	985197	68.88%	7.444%
40	15.855	2115	2122	2129	rBV	195136	293046	20.49%	2.214%
41	15.996	2142	2146	2149	rVB4	2862	3004	0.21%	0.023%
42	16.701	2264	2266	2270	rBV	1542	1607	0.11%	0.012%
43	17.289	2363	2366	2370	rVB4	2118	2936	0.21%	0.022%
44	17.506	2394	2403	2412	rVB	413132	644821	45.08%	4.872%
45	17.606	2412	2420	2429	rBV	725704	1133170	79.23%	8.562%
46	17.776	2447	2449	2452	rVB3	1472	1515	0.11%	0.011%
47	17.952	2475	2479	2480	rBV2	1232	1457	0.10%	0.011%
48	17.982	2482	2484	2487	rVB3	2266	2122	0.15%	0.016%
49	18.023	2487	2491	2492	rBV4	1533	2012	0.14%	0.015%
50	18.205	2519	2522	2524	rBV2	1277	1861	0.13%	0.014%
51	18.475	2564	2568	2569	rBV3	1632	1931	0.14%	0.015%
52	18.599	2587	2589	2592	rBV3	1448	1738	0.12%	0.013%
53	18.652	2594	2598	2600	rVV4	1592	2206	0.15%	0.017%
54	18.734	2608	2612	2614	rVB4	1964	2373	0.17%	0.018%
55	18.881	2634	2637	2639	rBV3	2009	2297	0.16%	0.017%
56	18.916	2641	2643	2648	rVB4	2434	2623	0.18%	0.020%
57	18.980	2650	2654	2656	rBV3	2069	3548	0.25%	0.027%
58	19.268	2699	2703	2704	rVB4	2013	2321	0.16%	0.018%
59	19.321	2709	2712	2714	rBV3	1965	2139	0.15%	0.016%
60	19.462	2729	2736	2740	rBV5	12261	22378	1.56%	0.169%
61	19.527	2742	2747	2751	rBV3	10218	17383	1.22%	0.131%
62	19.591	2756	2758	2760	rVB3	1836	1598	0.11%	0.012%
63	19.668	2769	2771	2772	rBV2	2447	2177	0.15%	0.016%
64	19.703	2775	2777	2780	rBV4	2243	2398	0.17%	0.018%
65	19.762	2785	2787	2789	rVV2	2009	1470	0.10%	0.011%
66	19.826	2796	2798	2801	rBV3	2531	3376	0.24%	0.026%
67	19.891	2801	2809	2817	rVV	965849	1430291	100.00%	10.808%
68	20.267	2871	2873	2875	rVB2	3122	1437	0.10%	0.011%
69	20.290	2875	2877	2878	rBV2	3435	1650	0.12%	0.012%
70	20.467	2905	2907	2908	rBV2	4652	2987	0.21%	0.023%
71	21.794	3126	3133	3144	rBV	454356	765204	53.50%	5.782%
72	23.345	3395	3397	3398	rBV2	9729	7544	0.53%	0.057%
73	24.890	3650	3660	3672	rVB3	448770	1327698	92.83%	10.032%
74	25.113	3689	3698	3710	rBV3	237884	693003	48.45%	5.236%

Sum of corrected areas: 13234238

Instrument :

BNA_G

ClientSampleId :




SBLK280

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052747.D
Acq On : 19 Mar 2022 16:23
Operator : CG/JU
Sample : PB143280BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

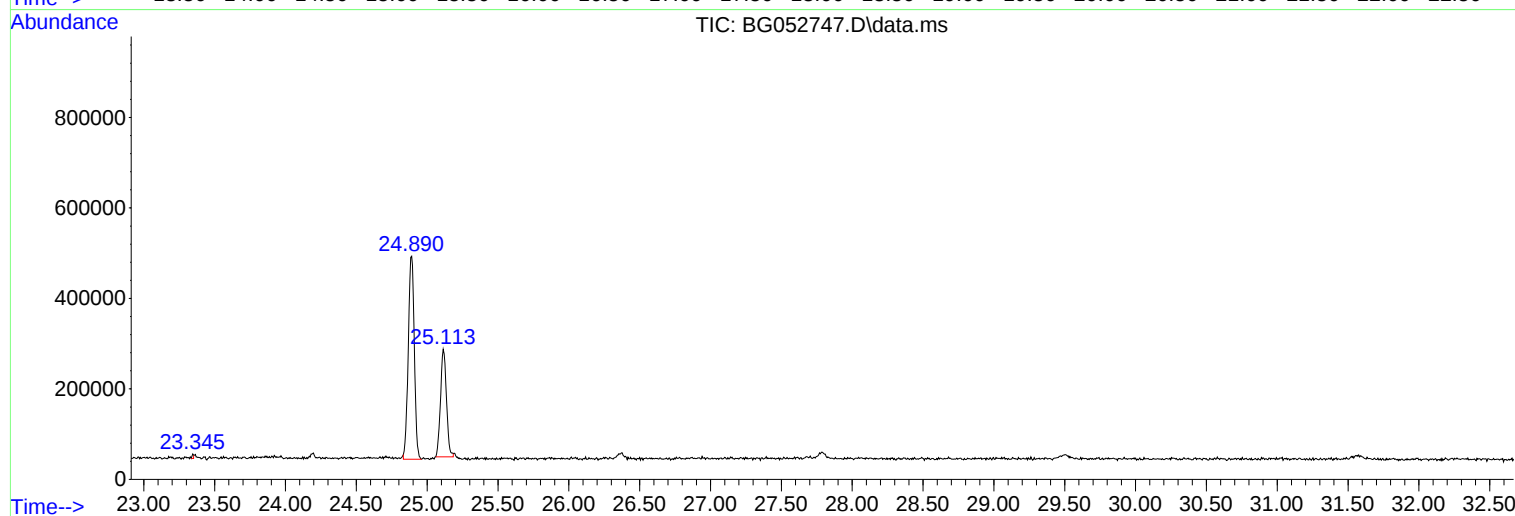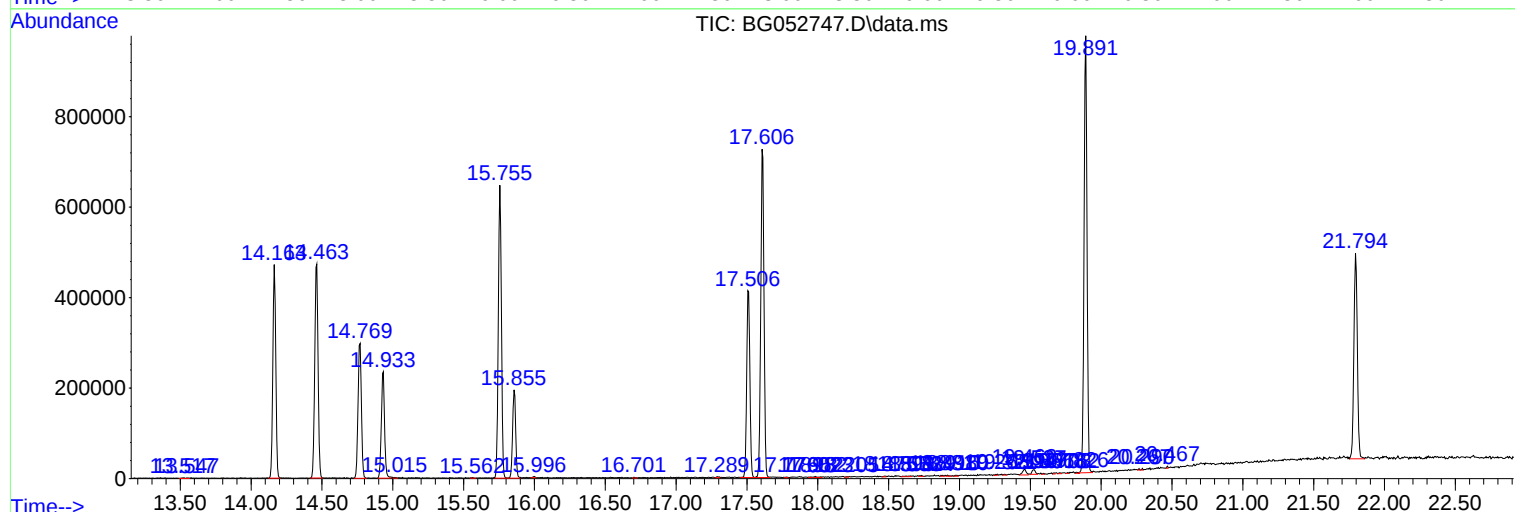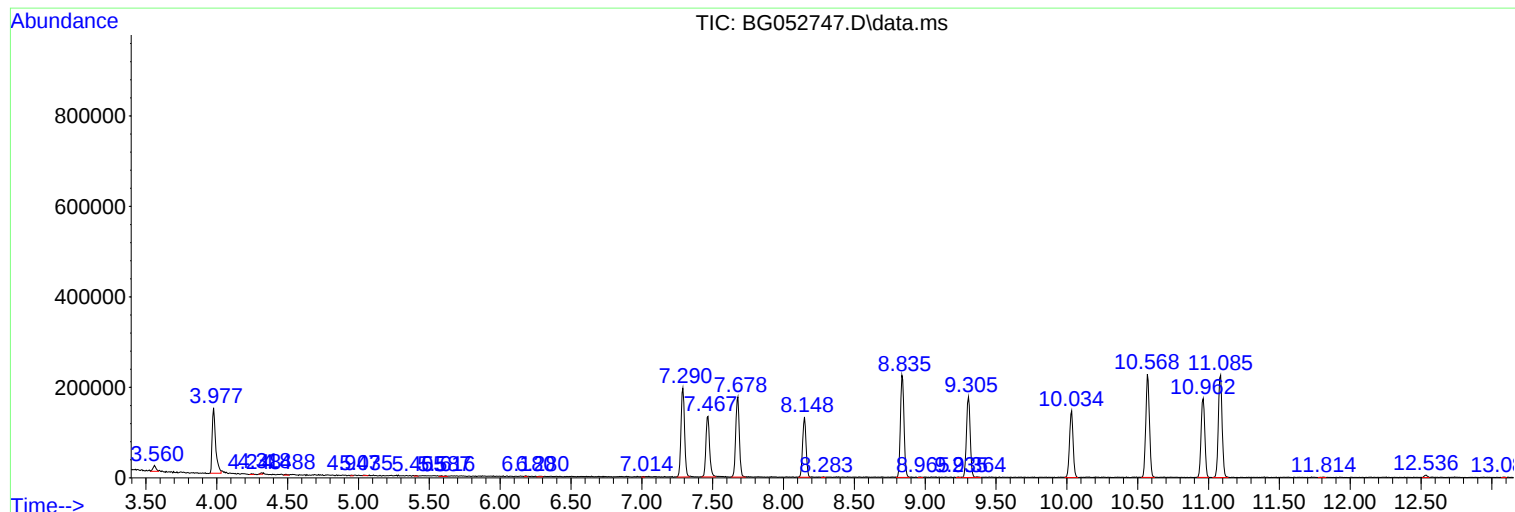

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052747.D
Acq On : 19 Mar 2022 16:23
Operator : CG/JU
Sample : PB143280BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031822\
Data File : BG052747.D
Acq On : 19 Mar 2022 16:23
Operator : CG/JU
Sample : PB143280BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK280

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------