
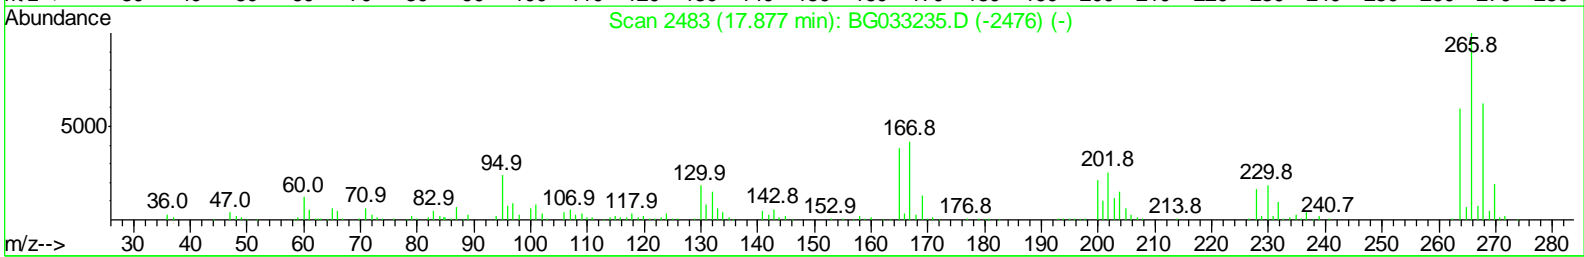
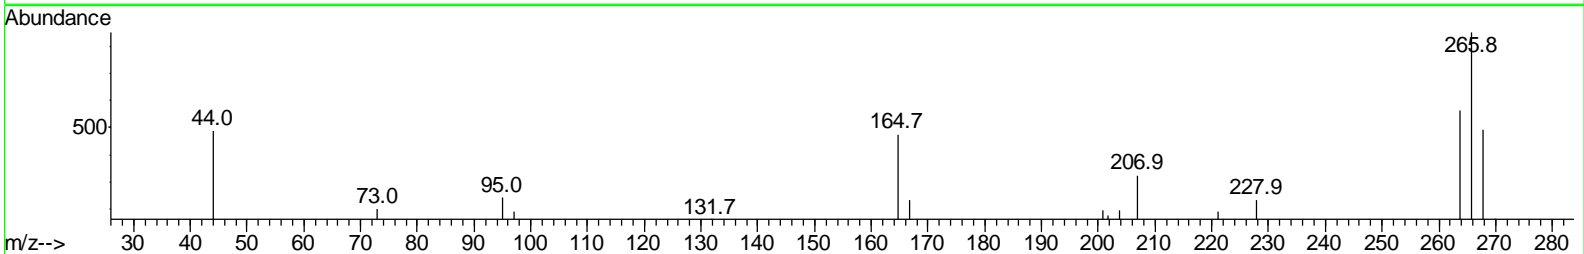


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG031918\
 Data File : BG033245.D
 Acq On : 19 Mar 2018 18:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:18:56 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 19 16:48:53 2018
 Response via : Initial Calibration

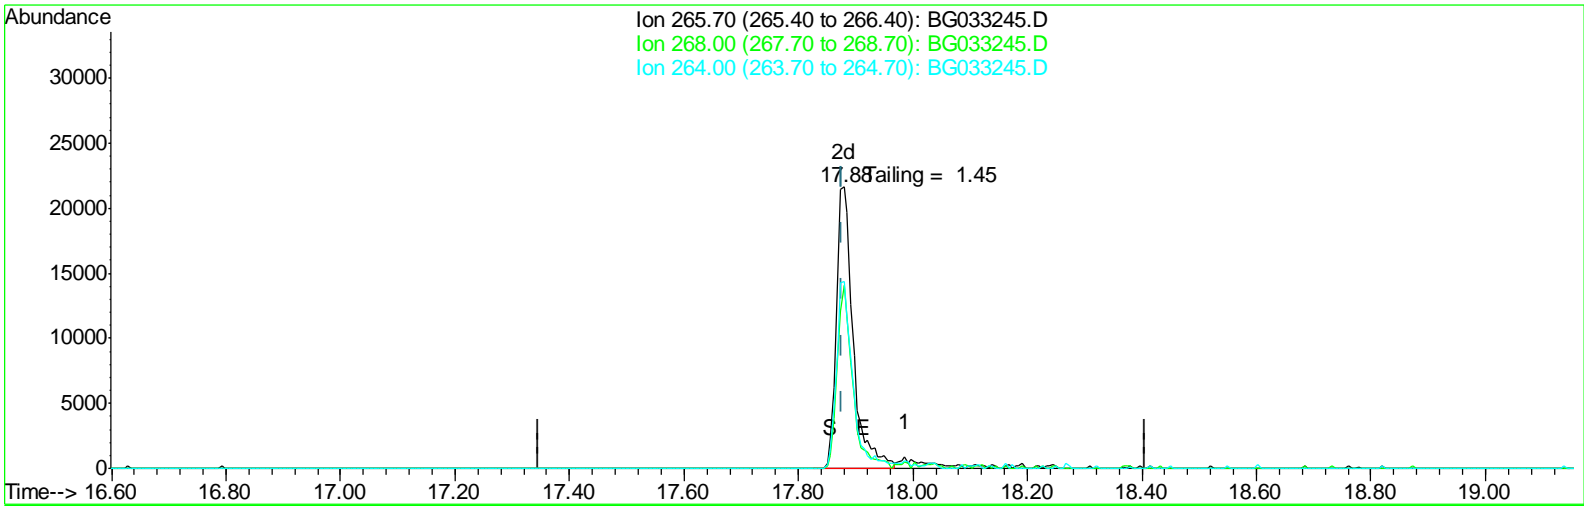

TIC: BG033245.D

(69) Pentachlorophenol (C)




17.985min (+0.109) 635.52ng

response 1730

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.65
264.00	62.00	66.47
0.00	0.00	0.00

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG031918\
 Data File : BG033245.D
 Acq On : 19 Mar 2018 18:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:18:56 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 19 16:48:53 2018
 Response via : Initial Calibration

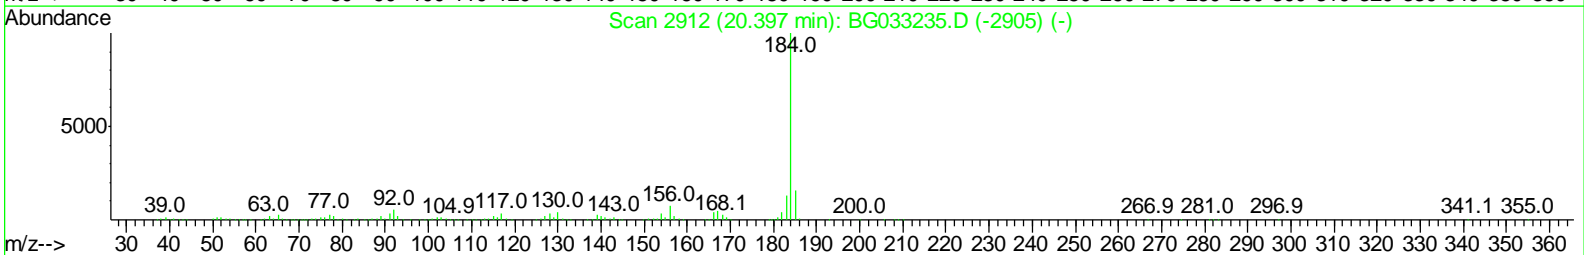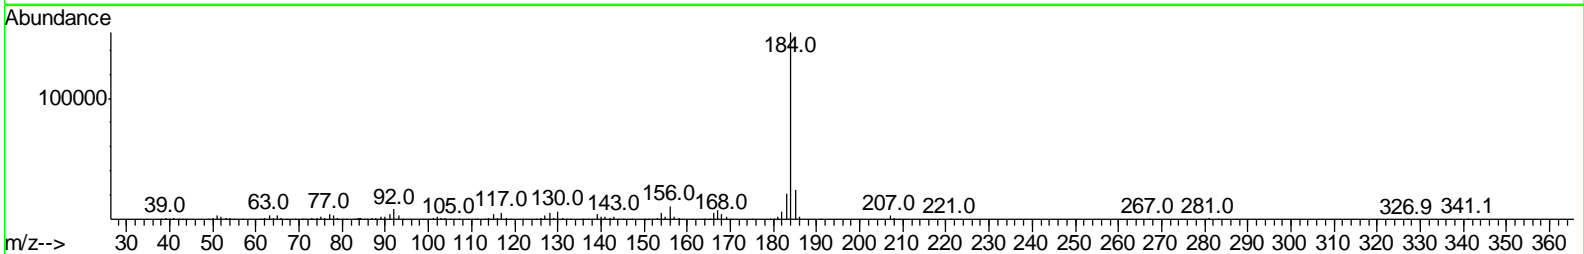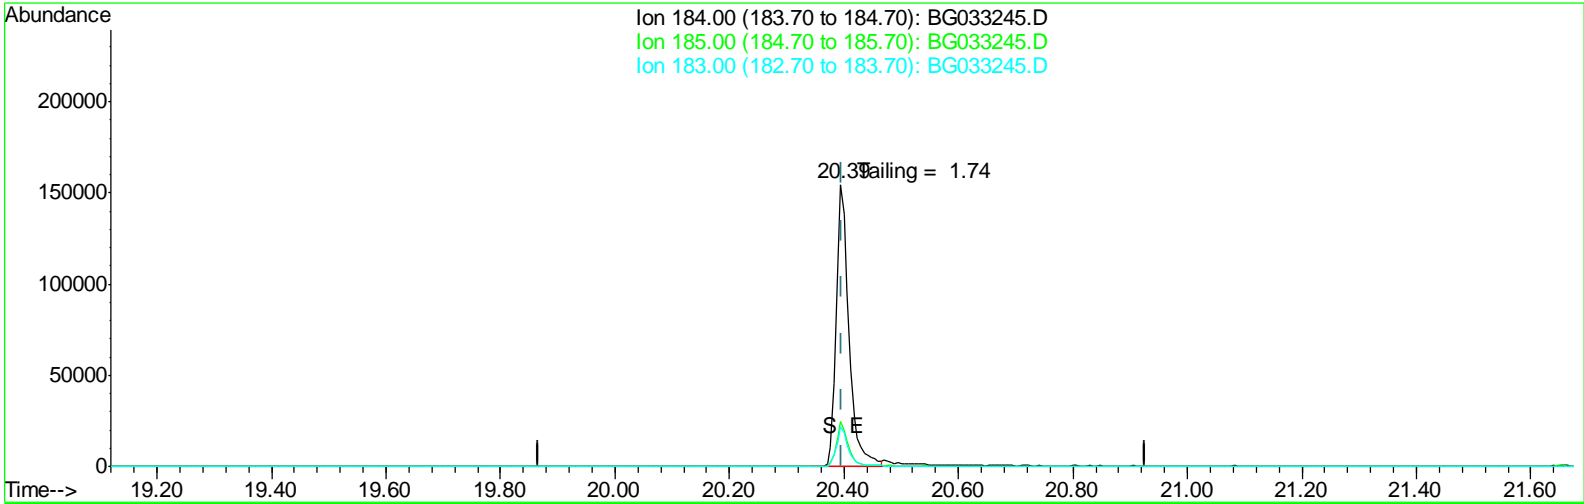

TIC: BG033245.D

(76) Benzidine

20.394min (-0.003) 0.00ng

response 249332

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.93
183.00	13.30	13.97
0.00	0.00	0.00