


Data Path : Z:\HPCHEM1\BNA G\DATA\BG031918\
 Data File : BG033231.D
 Acq On : 19 Mar 2018 8:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 19 16:48:53 2018

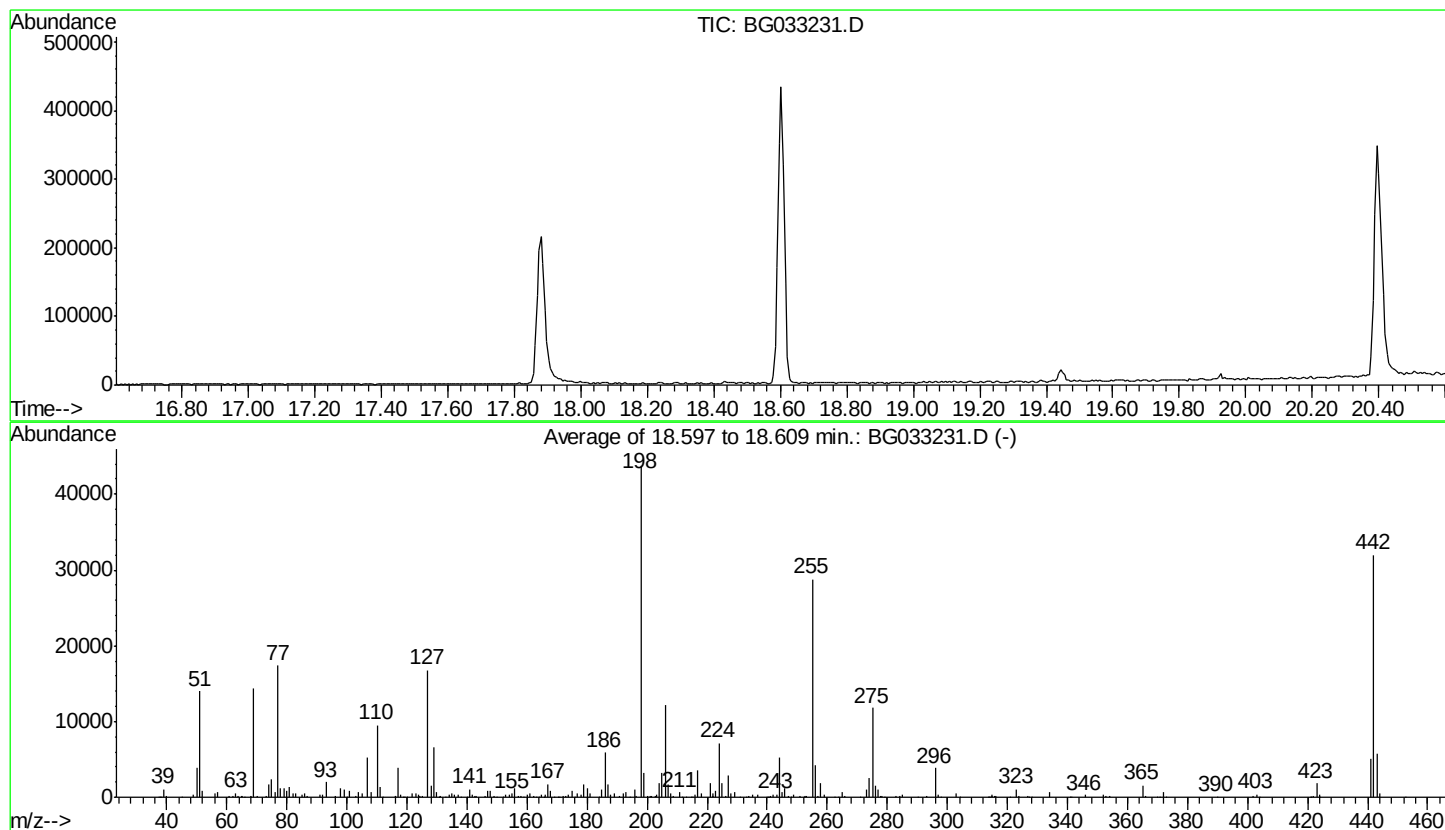

AutoFind: Scans 2605, 2606, 2607; Background Corrected with Scan 2598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	13948	PASS
68	69	0.00	2	1.2	179	PASS
69	198	0.00	100	32.7	14330	PASS
70	69	0.00	2	0.6	90	PASS
127	198	10	80	38.2	16744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43778	PASS
199	198	5	9	7.2	3143	PASS
275	198	10	60	27.0	11803	PASS
365	198	1	100	3.6	1572	PASS
441	443	0.01	100	87.6	5093	PASS
442	198	50	100	73.0	31973	PASS
443	442	15	24	18.2	5812	PASS