


Data Path : Z:\HPCHEM1\BNA G\DATA\BG031918\
 Data File : BG033245.D
 Acq On : 19 Mar 2018 18:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 19 16:48:53 2018

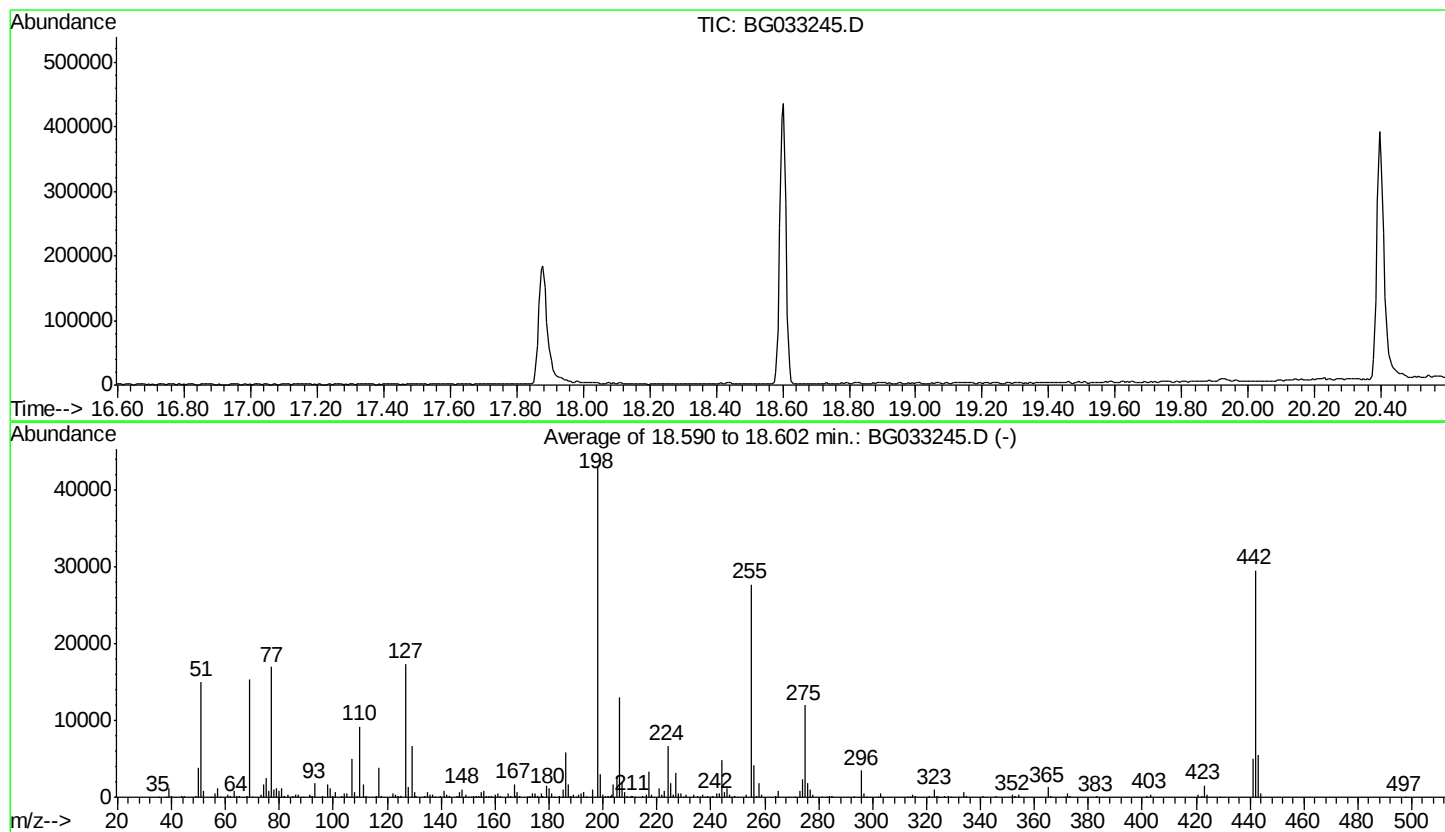

AutoFind: Scans 2604, 2605, 2606; Background Corrected with Scan 2598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	15025	PASS
68	69	0.00	2	0.6	99	PASS
69	198	0.00	100	35.5	15301	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	40.3	17365	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43120	PASS
199	198	5	9	7.1	3043	PASS
275	198	10	60	27.7	11933	PASS
365	198	1	100	3.0	1299	PASS
441	443	0.01	100	89.3	4971	PASS
442	198	50	100	68.4	29493	PASS
443	442	15	24	18.9	5564	PASS