
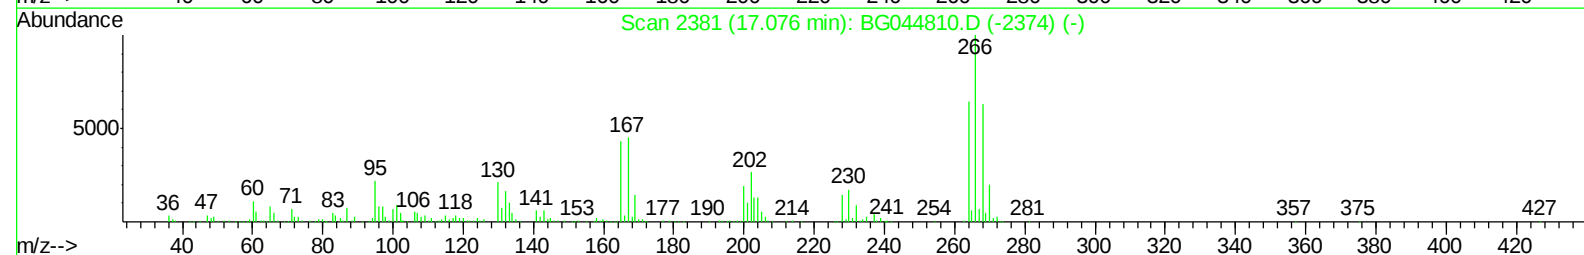
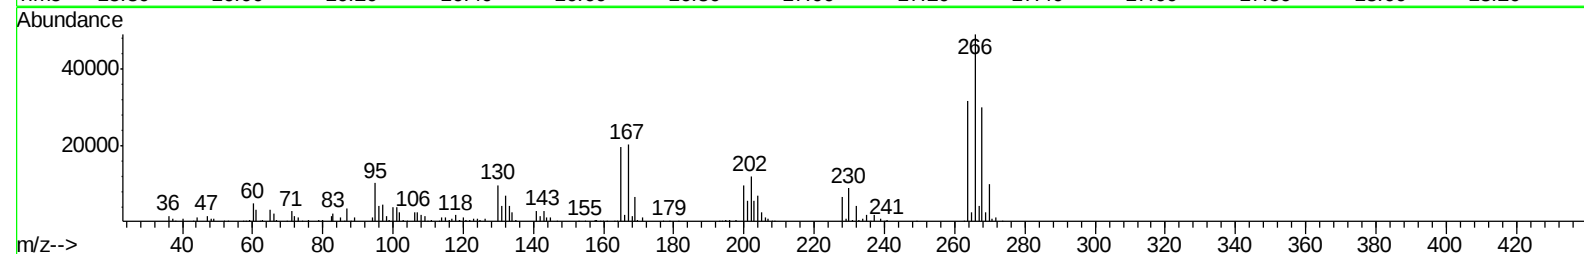


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031920\
 Data File : BG044899.D
 Acq On : 19 Mar 2020 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 02:05:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 17:37:15 2020
 Response via : Initial Calibration

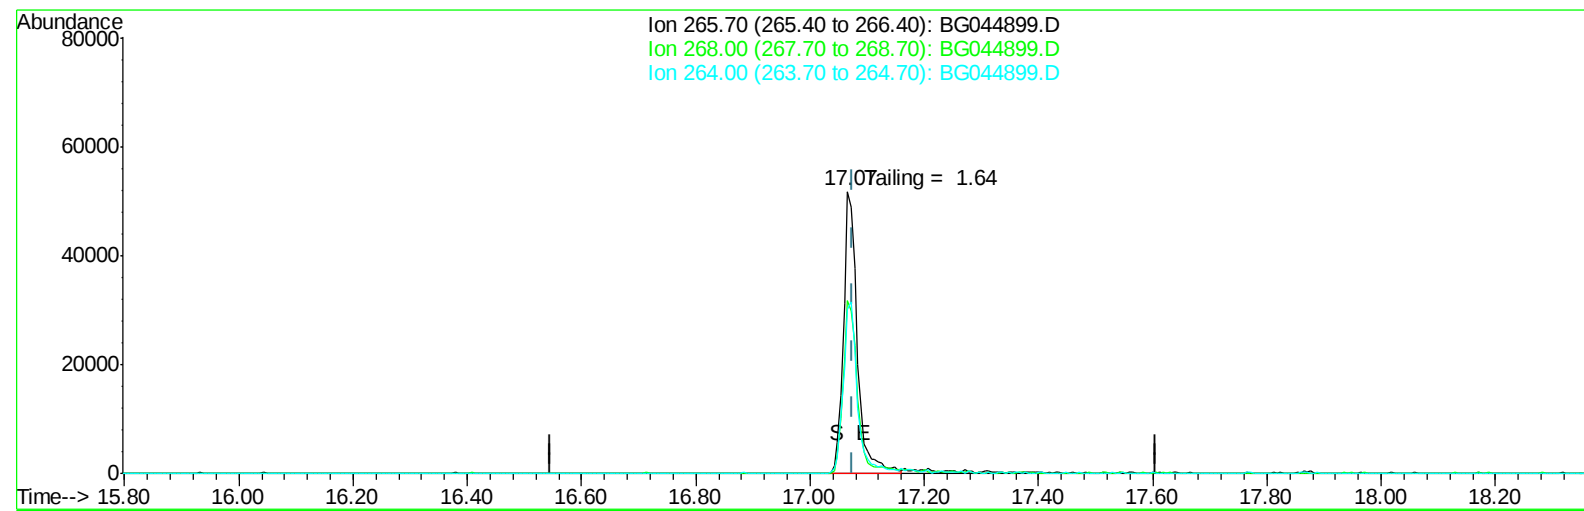

TIC: BG044899.D

(70) Pentachlorophenol (C)




17.066min (-0.010) 197160.54ng

response 86806

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	61.45
264.00	64.30	58.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031920\
 Data File : BG044899.D
 Acq On : 19 Mar 2020 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 02:05:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 16 17:37:15 2020
 Response via : Initial Calibration

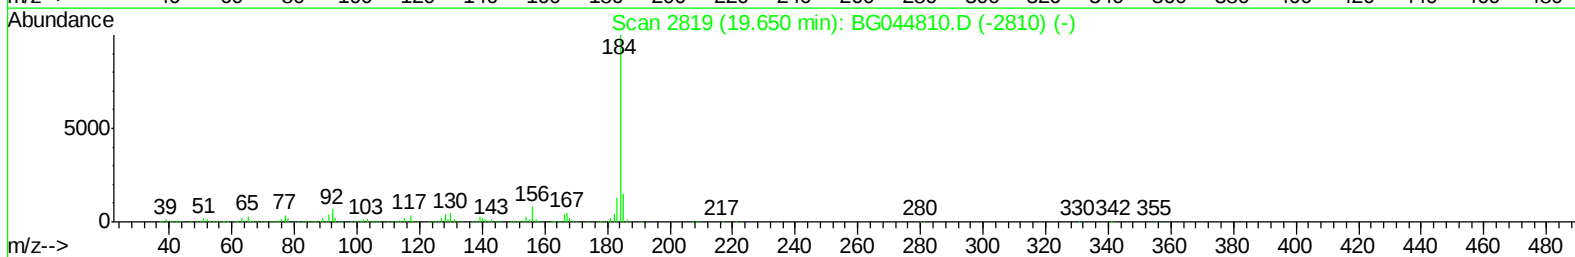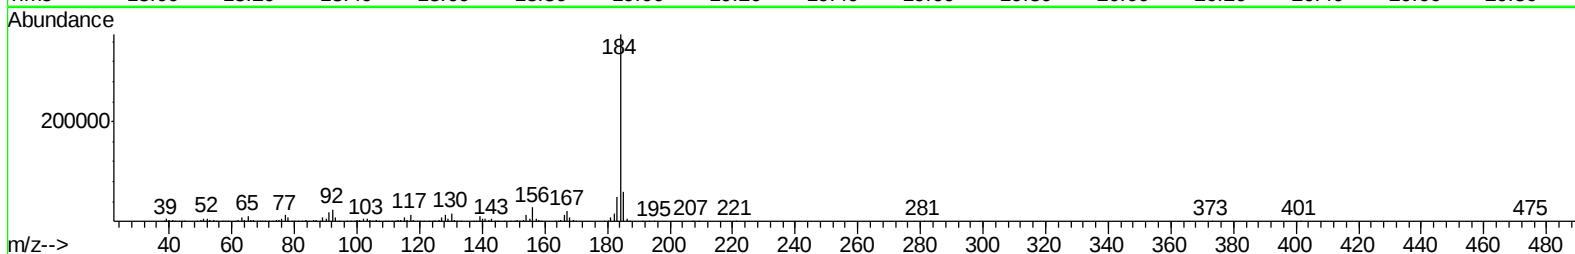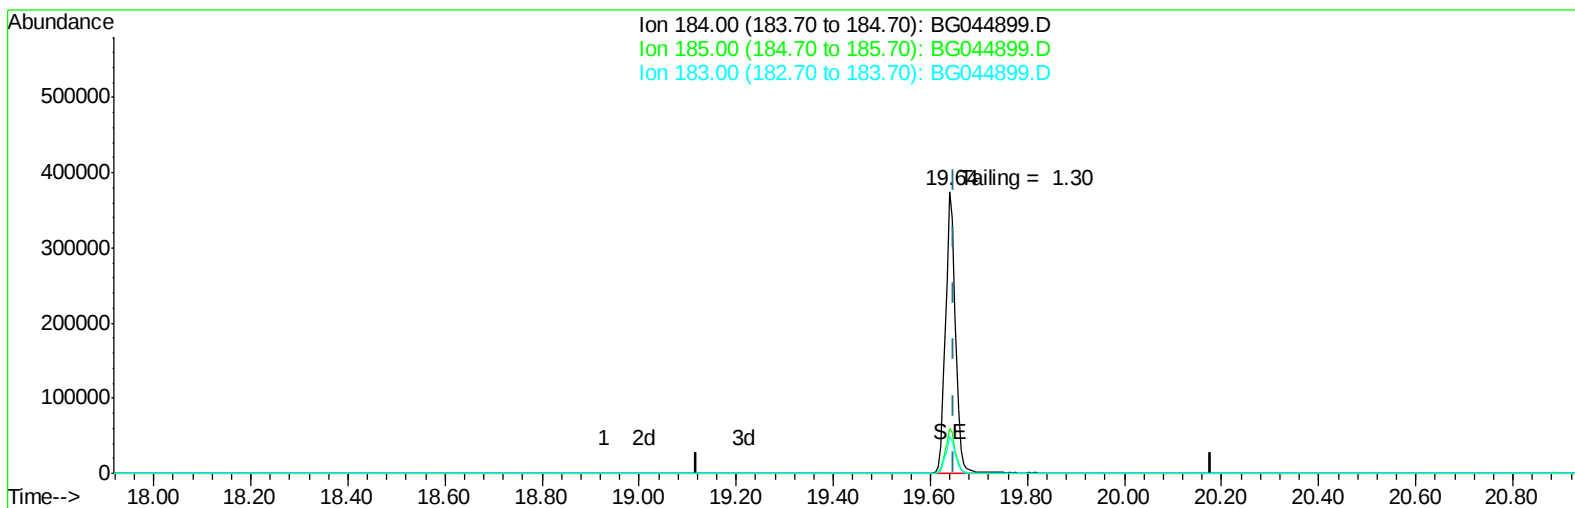

TIC: BG044899.D

(77) Benzidine

18.928min (-0.721) 0.49ng

response 63

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	0.00#
183.00	13.40	0.00#
0.00	0.00	0.00