


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG031920\
 Data File : BG044899.D
 Acq On : 19 Mar 2020 16:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 16 17:37:15 2020

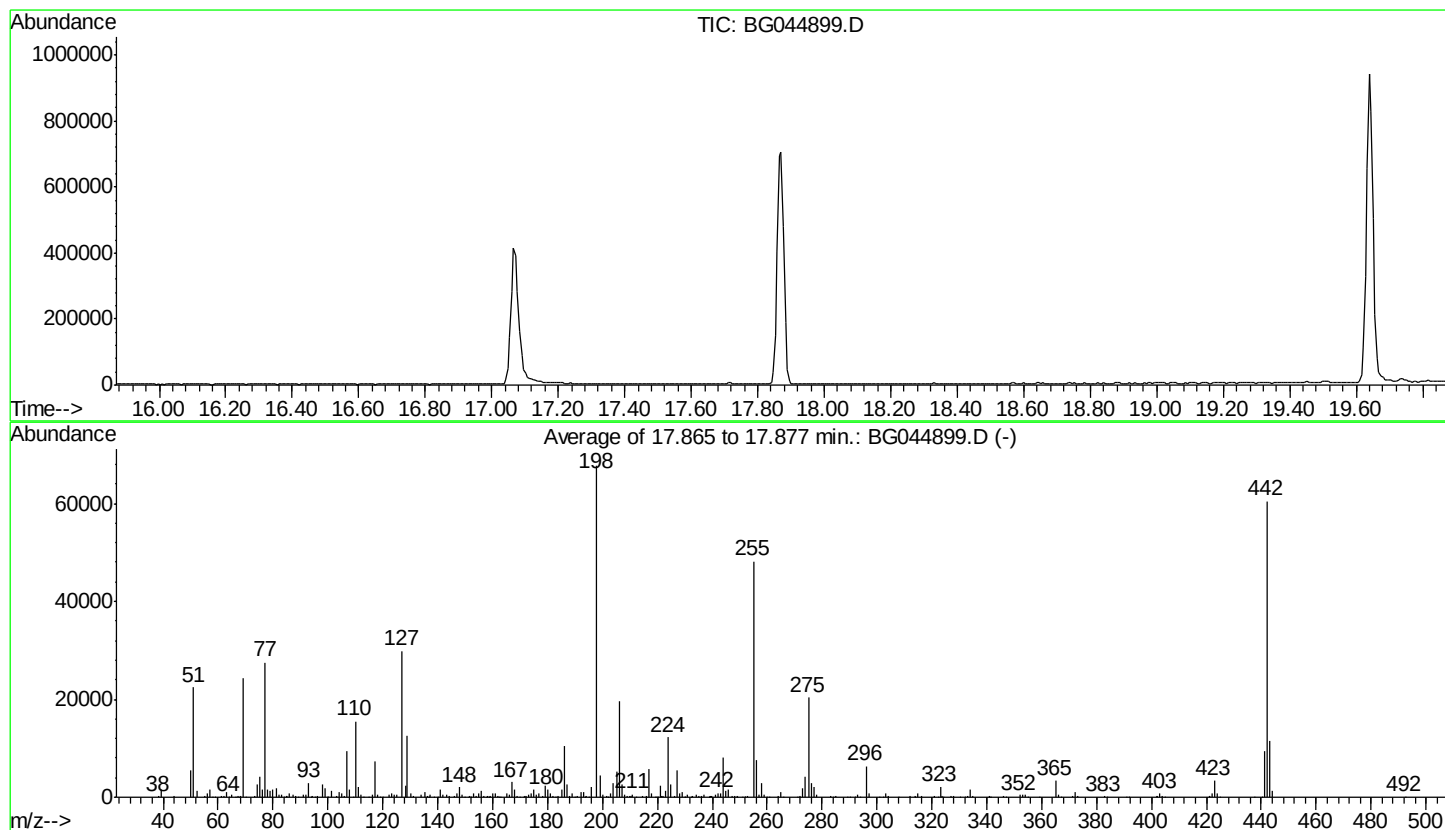

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	22430	PASS
68	69	0.00	2	1.6	396	PASS
69	198	0.00	100	36.1	24436	PASS
70	69	0.00	2	0.3	76	PASS
127	198	10	80	44.1	29904	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67746	PASS
199	198	5	9	6.7	4567	PASS
275	198	10	60	30.1	20381	PASS
365	198	1	100	4.8	3285	PASS
441	198	0.01	100	14.0	9478	PASS
442	198	50	100	89.3	60501	PASS
443	442	15	24	18.9	11429	PASS