
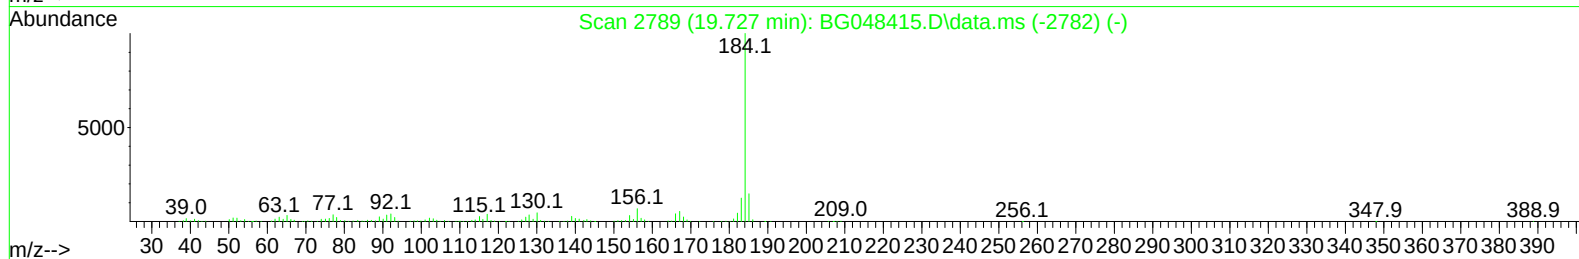
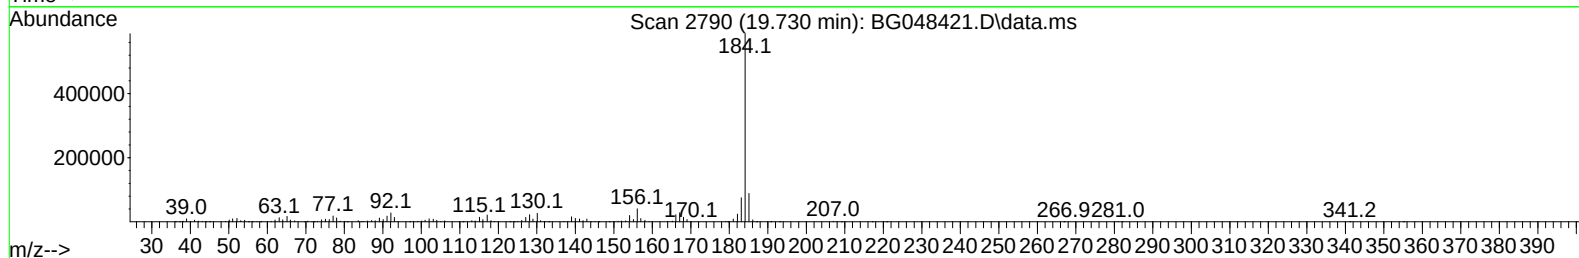


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
Data File : BG048421.D
Acq On : 19 Mar 2021 12:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 13:56:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

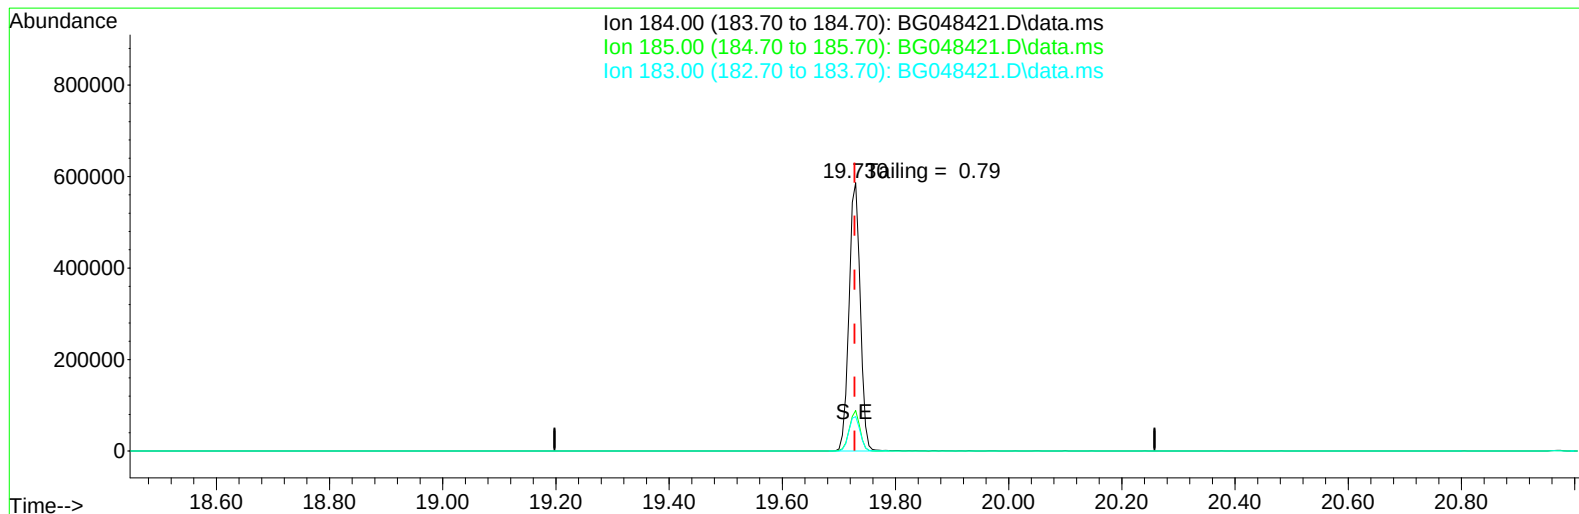




TIC: BG048421.D\data.ms

(77) Benzidine**19.730min (+ 0.002) 509166.92 ng****response 808356**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.08
183.00	13.20	12.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
Data File : BG048421.D
Acq On : 19 Mar 2021 12:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 13:56:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

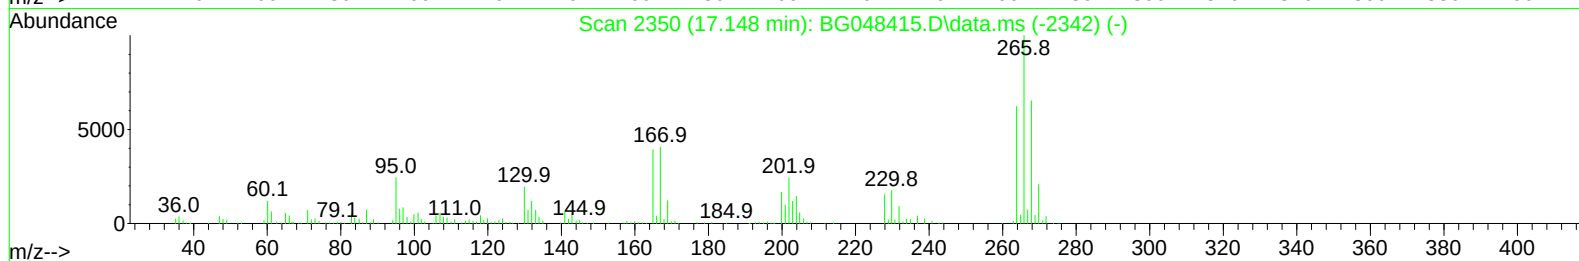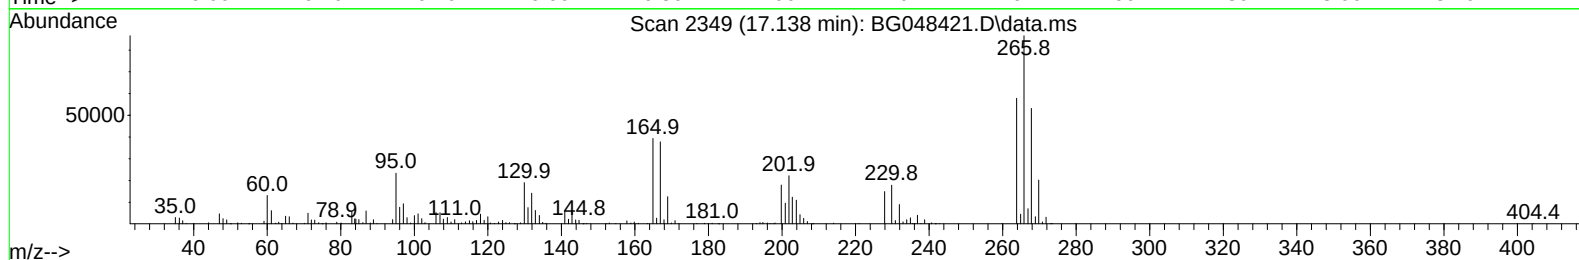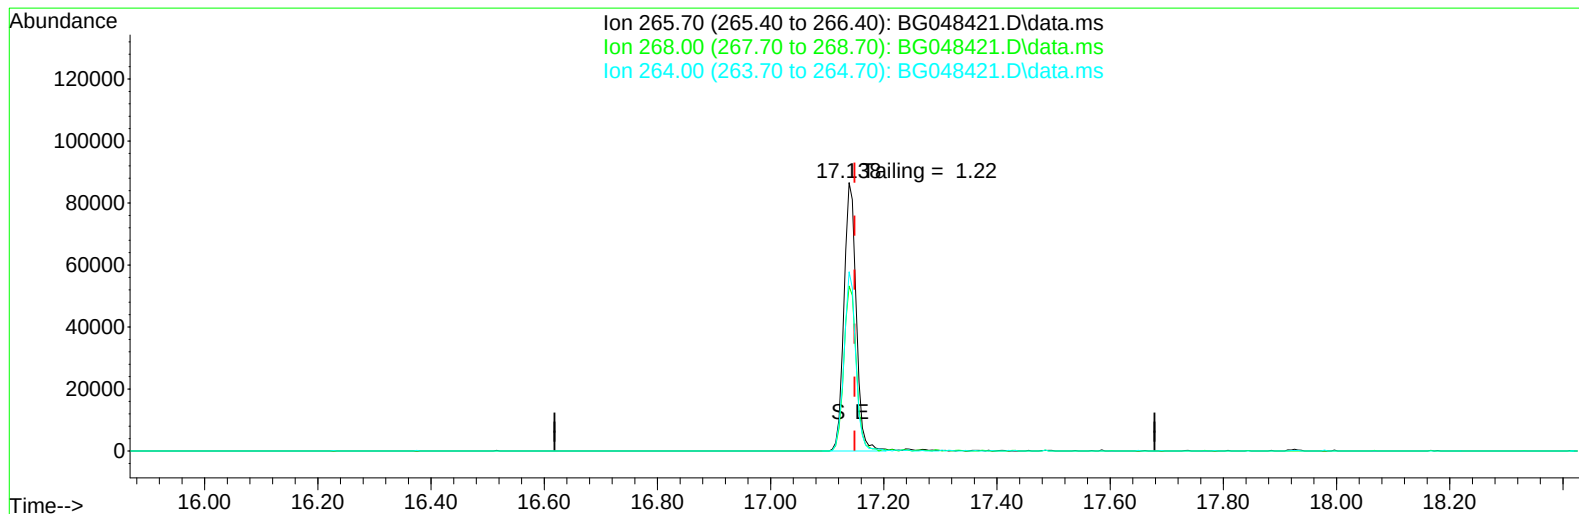

TIC: BG048421.D\data.ms

(70) Pentachlorophenol (C)

17.138min (-0.010) 224545.07 ng

response 130940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.47
264.00	61.60	66.76
0.00	0.00	0.00