

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
 Data File : BG048426.D
 Acq On : 19 Mar 2021 16:23
 Operator : CG/JU
 Sample : M1723-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RO124027

Quant Time: Mar 19 17:07:10 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 18 16:38:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.108	152	38378	20.00	ng	0.00
21) Naphthalene-d8	10.928	136	142499	20.00	ng	# 0.00
39) Acenaphthene-d10	14.747	164	110708	20.00	ng	0.00
64) Phenanthrene-d10	17.497	188	309358	20.00	ng	# 0.00
76) Chrysene-d12	21.792	240	390163	20.00	ng	# 0.00
86) Perylene-d12	25.129	264	401551	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.652	112	238292	102.68	ng	0.00
7) Phenol-d6	7.250	99	313306	92.78	ng	0.00
23) Nitrobenzene-d5	9.271	82	235076	65.96	ng	0.00
42) 2,4,6-Tribromophenol	16.234	330	167496	93.03	ng	0.00
45) 2-Fluorobiphenyl	13.373	172	433279	56.30	ng	0.00
79) Terphenyl-d14	20.106	244	775570	35.85	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	7.239	77	31634	10.14	ng	# 40
10) Phenol	7.274	94	7255	2.10	ng	# 48
15) Benzyl Alcohol	8.337	79	106427	35.50	ng	# 79
50) Dimethylphthalate	14.195	163	32937	3.66	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
Data File : BG048426.D
Acq On : 19 Mar 2021 16:23
Operator : CG/JU
Sample : M1723-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RO124027

Quant Time: Mar 19 17:07:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration




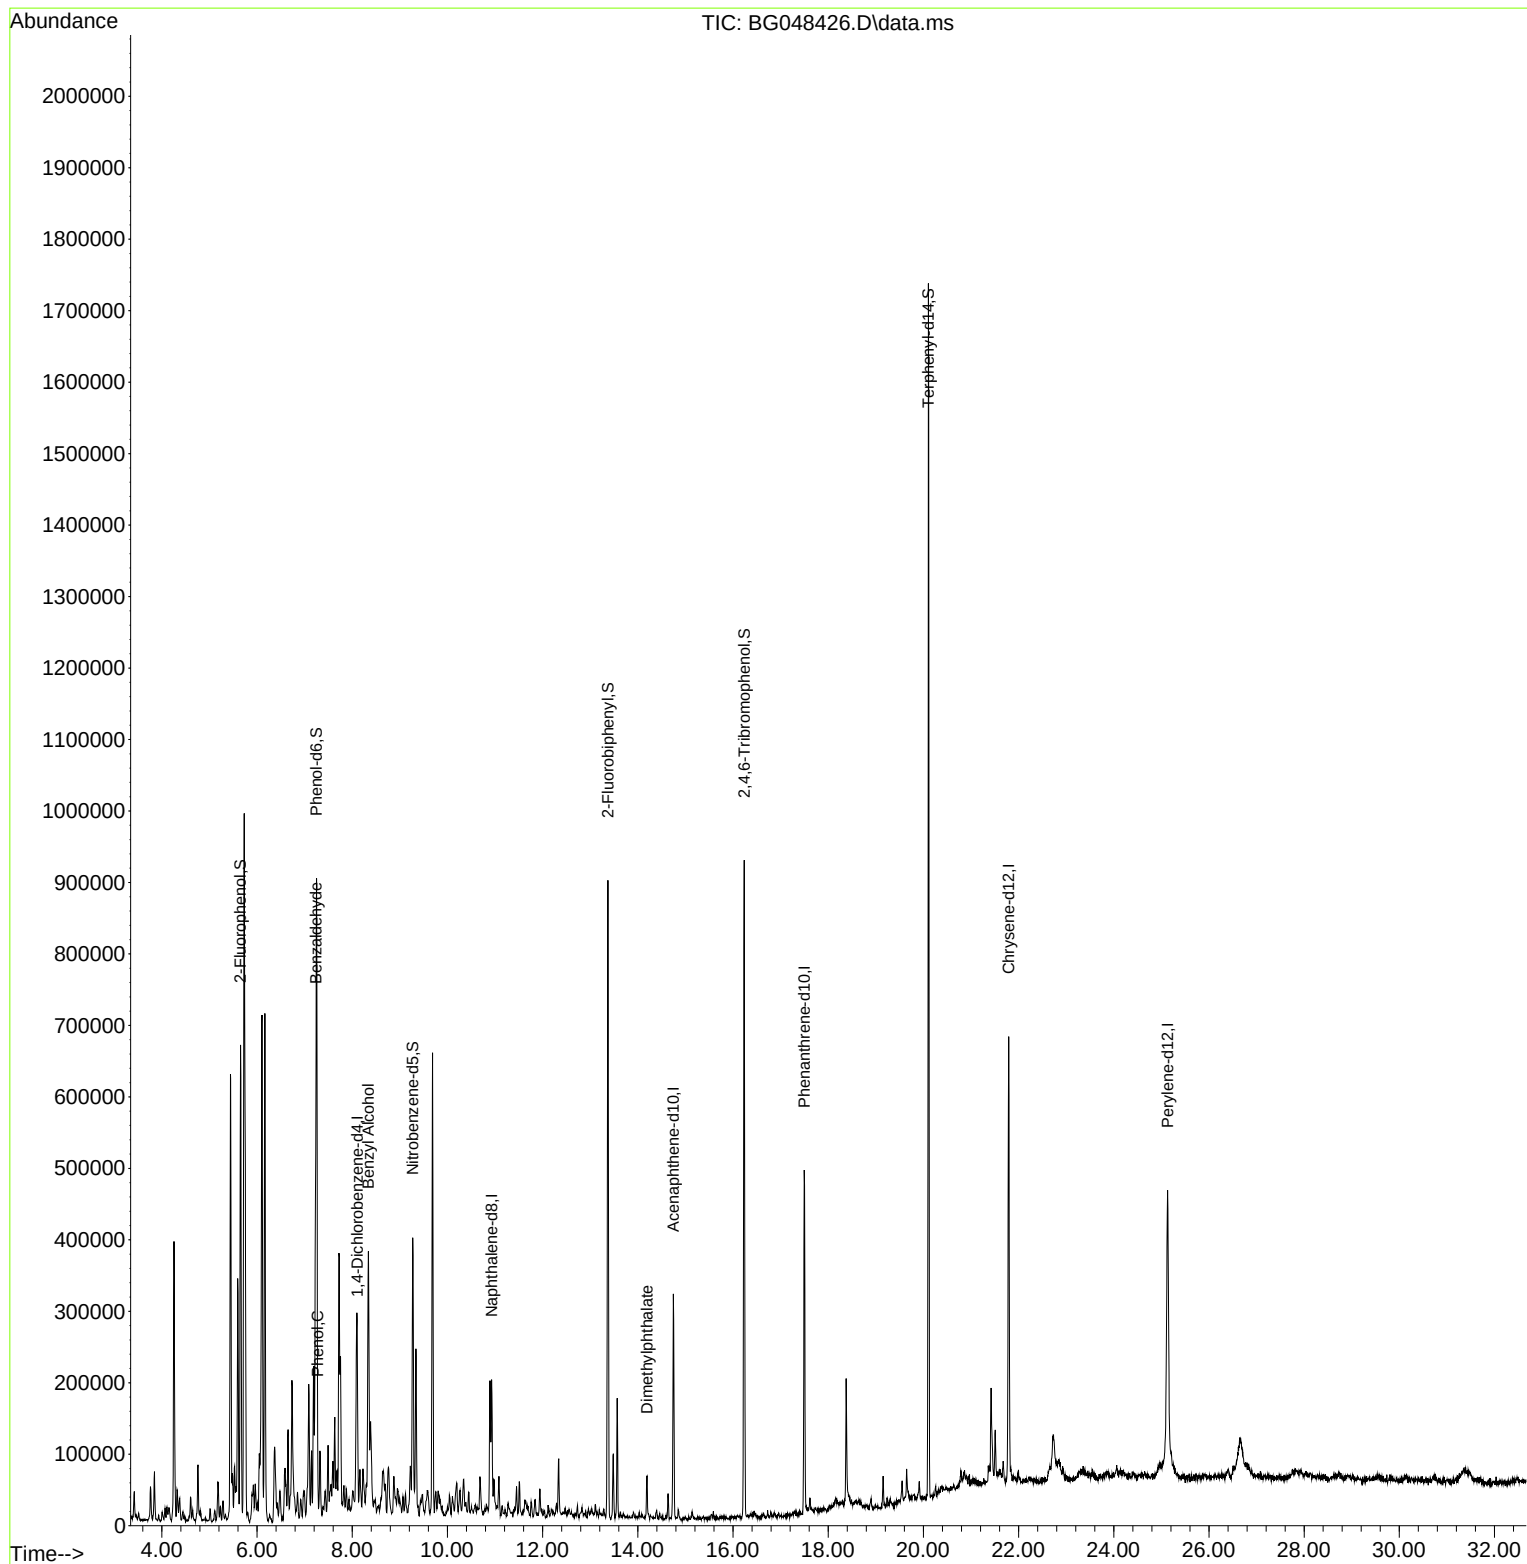




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.108 min Scan# 812
Delta R.T. -0.004 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampleId :
RO124027


Tgt Ion:152 Resp: 38378
Ion Ratio Lower Upper
152 100
150 158.4 125.0 187.6
115 62.0 41.8 62.6

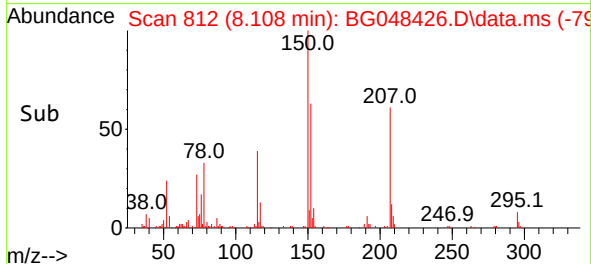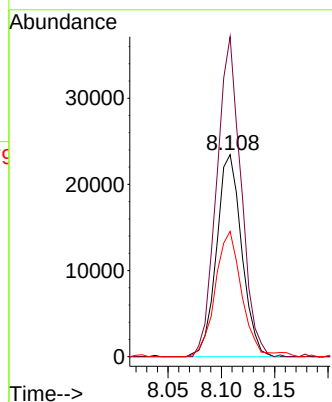

#5
2-Fluorophenol
Concen: 102.68 ng
RT: 5.652 min Scan# 394
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion:112 Resp: 238292
Ion Ratio Lower Upper
112 100
64 66.3 46.7 70.1
63 40.2 22.8 34.2#


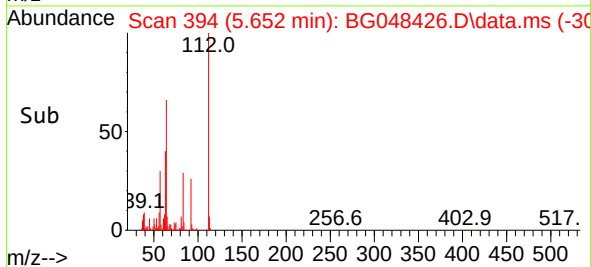
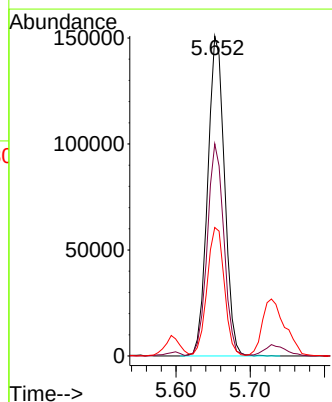
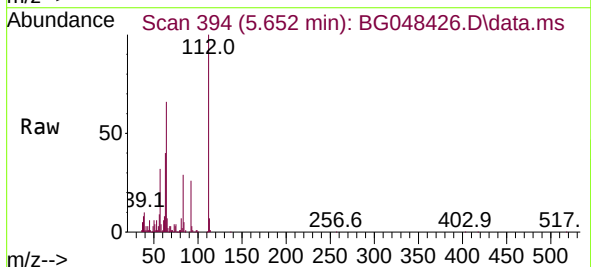




#7
Phenol-d6
Concen: 92.78 ng
RT: 7.250 min Scan# 666
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampleId :
RO124027


Tgt Ion: 99 Resp: 313306
Ion Ratio Lower Upper
99 100
42 23.9 12.8 19.2#
71 57.4 24.6 36.8#

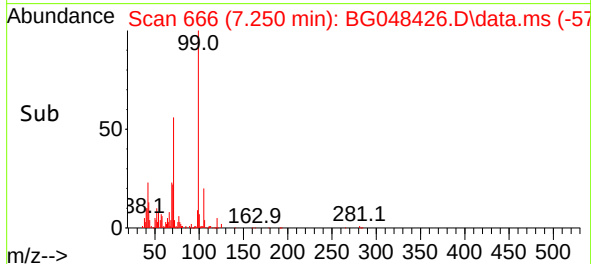

#9
Benzaldehyde
Concen: 10.14 ng
RT: 7.239 min Scan# 664
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion: 77 Resp: 31634
Ion Ratio Lower Upper
77 100
105 200.7 85.9 125.9#
106 74.6 80.9 120.9#


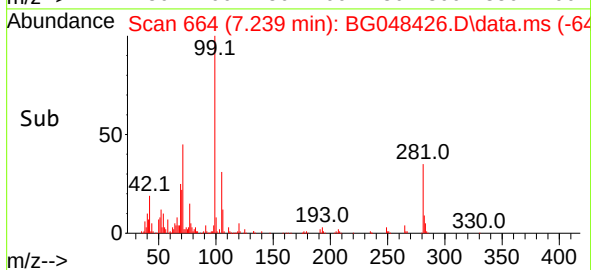

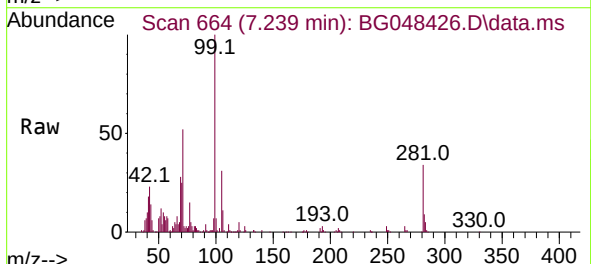




#10
Phenol
Concen: 2.10 ng
RT: 7.274 min Scan# 670
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampled :
RO124027


Tgt Ion: 94 Resp: 7255
Ion Ratio Lower Upper
94 100
65 45.4 6.6 46.6
66 71.0 13.9 53.9#

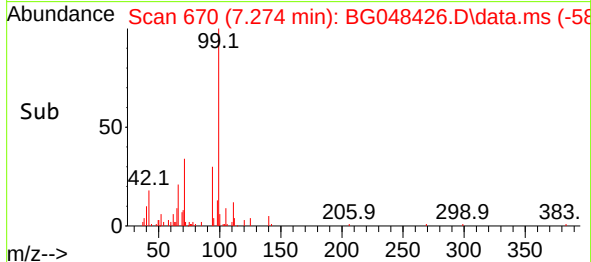

#15
Benzyl Alcohol
Concen: 35.50 ng
RT: 8.337 min Scan# 851
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion: 79 Resp: 106427
Ion Ratio Lower Upper
79 100
108 56.1 65.5 98.3#
77 71.7 50.1 75.1


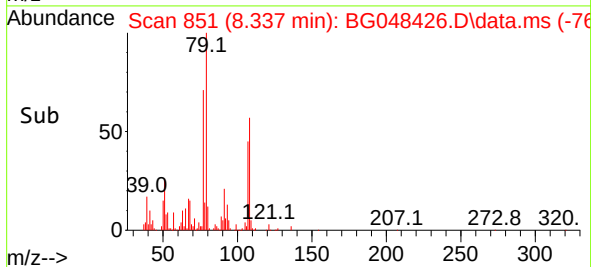

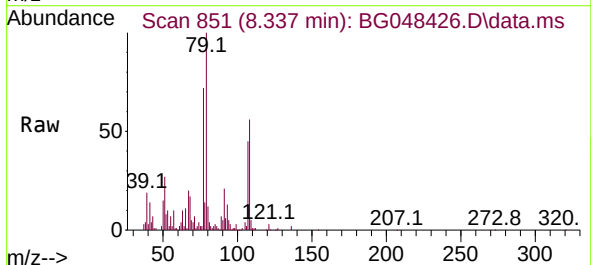




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.928 min Scan# 1292
Delta R.T. -0.009 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampleId :
RO124027


Tgt Ion:	136	Resp:	142499
Ion Ratio	Lower	Upper	
136	100		
137	12.3	9.1	13.7
54	7.2	6.2	9.4
68	4.4	5.0	7.4

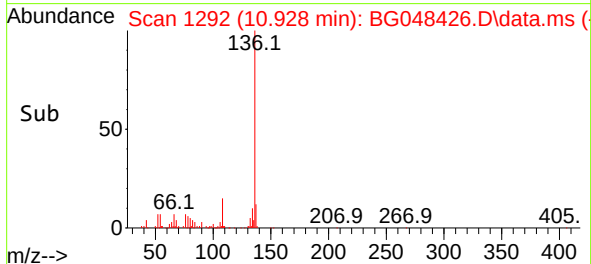

#23
Nitrobenzene-d5
Concen: 65.96 ng
RT: 9.271 min Scan# 1010
Delta R.T. -0.009 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion:	82	Resp:	235076
Ion Ratio	Lower	Upper	
82	100		
128	30.5	37.0	55.6
54	48.5	39.0	58.4


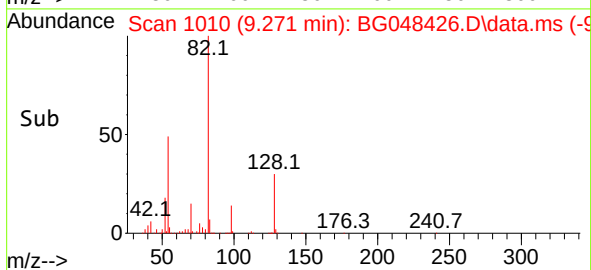

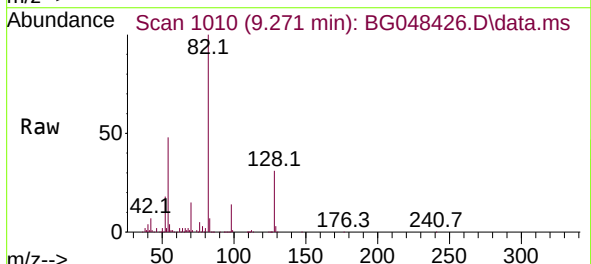




#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.747 min Scan# 1942
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampleId :
RO124027


Tgt Ion:164 Resp: 110708
Ion Ratio Lower Upper
164 100
162 97.9 82.3 123.5
160 42.3 35.3 52.9

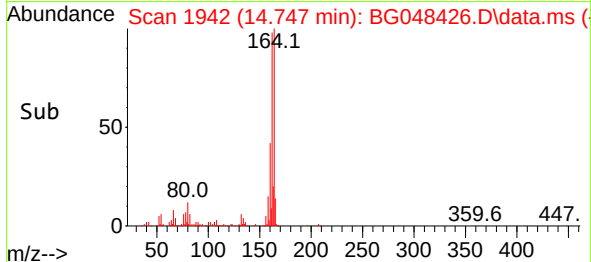

#42
2,4,6-Tribromophenol
Concen: 93.03 ng
RT: 16.234 min Scan# 2195
Delta R.T. -0.009 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion:330 Resp: 167496
Ion Ratio Lower Upper
330 100
332 96.3 76.5 114.7
141 35.3 26.0 39.0


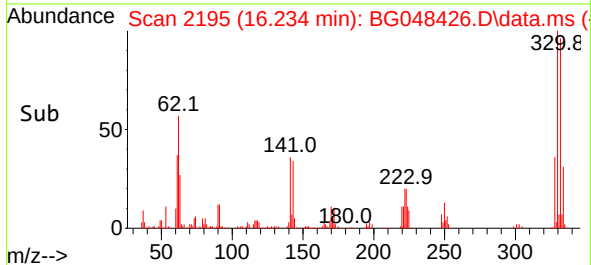

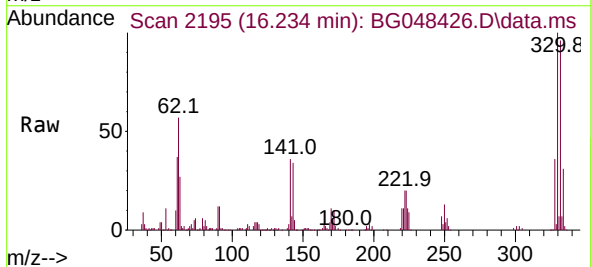




#45
2-Fluorobiphenyl
Concen: 56.30 ng
RT: 13.373 min Scan# 1708
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampleId :
RO124027


Tgt Ion:172	Resp:	433279	
Ion	Ratio	Lower	Upper
172	100		
171	38.0	31.3	46.9
170	23.9	20.8	31.2

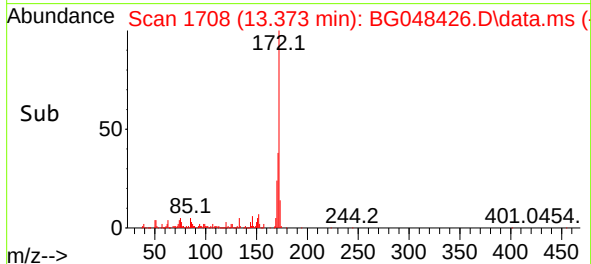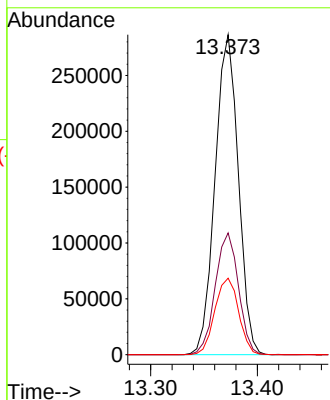

#50
Dimethylphthalate
Concen: 3.66 ng
RT: 14.195 min Scan# 1848
Delta R.T. -0.003 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion:163	Resp:	32937	
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.8	5.8
164	10.2	8.8	13.2


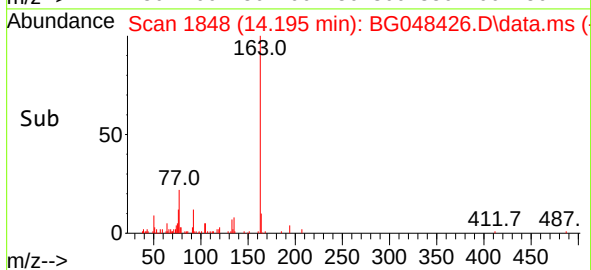
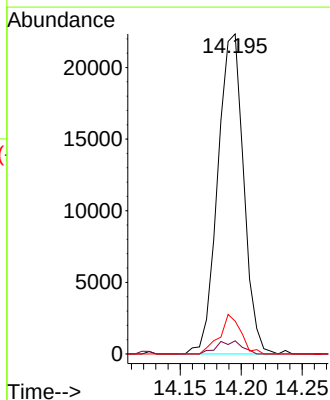
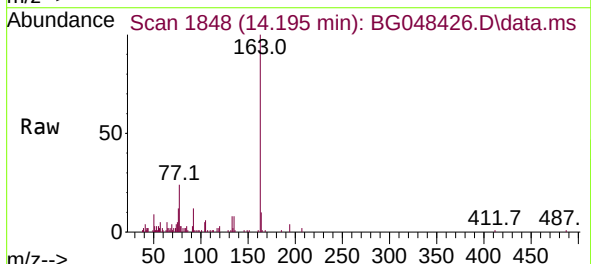




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.497 min Scan# 2410
Delta R.T. -0.009 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23




Instrument :
BNA_G
ClientSampleId :
RO124027


Tgt Ion:188 Resp: 309358
Ion Ratio Lower Upper
188 100
94 5.8 6.3 9.5#
80 6.5 7.0 10.6#

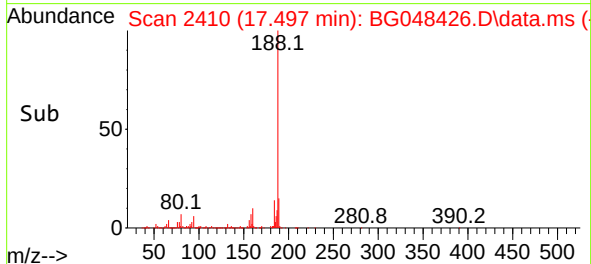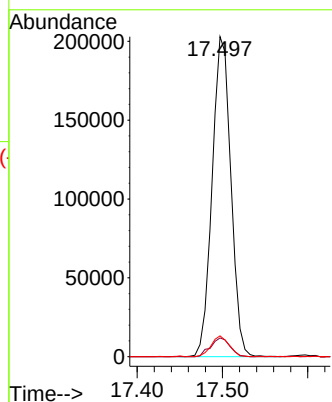

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.792 min Scan# 3141
Delta R.T. -0.009 min
Lab File: BG048426.D
Acq: 19 Mar 2021 16:23

Tgt Ion:240 Resp: 390163
Ion Ratio Lower Upper
240 100
120 4.4 6.2 9.4#
236 26.0 20.5 30.7


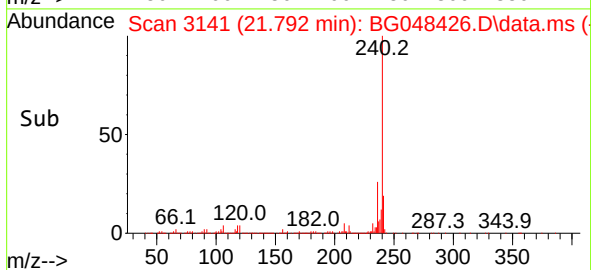

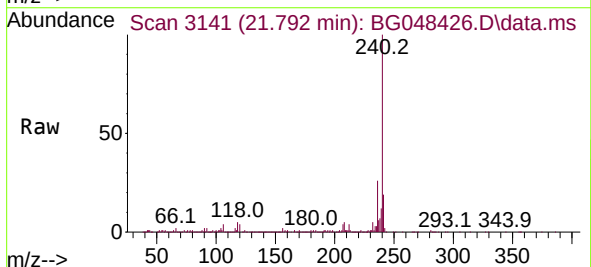




#79
 Terphenyl-d14
 Concen: 35.85 ng
 RT: 20.106 min Scan# 2854
 Delta R.T. -0.009 min
 Lab File: BG048426.D
 Acq: 19 Mar 2021 16:23

Instrument :
 BNA_G
 ClientSampleId :
 RO124027

Tgt Ion:244 Resp: 775570
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.7 10.1
 122 6.0 7.8 11.6#

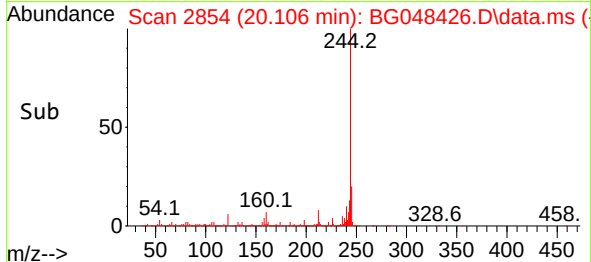

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.129 min Scan# 3709
 Delta R.T. -0.009 min
 Lab File: BG048426.D
 Acq: 19 Mar 2021 16:23

Tgt Ion:264 Resp: 401551
 Ion Ratio Lower Upper
 264 100
 260 25.1 18.8 28.2
 265 20.5 17.8 26.8

