
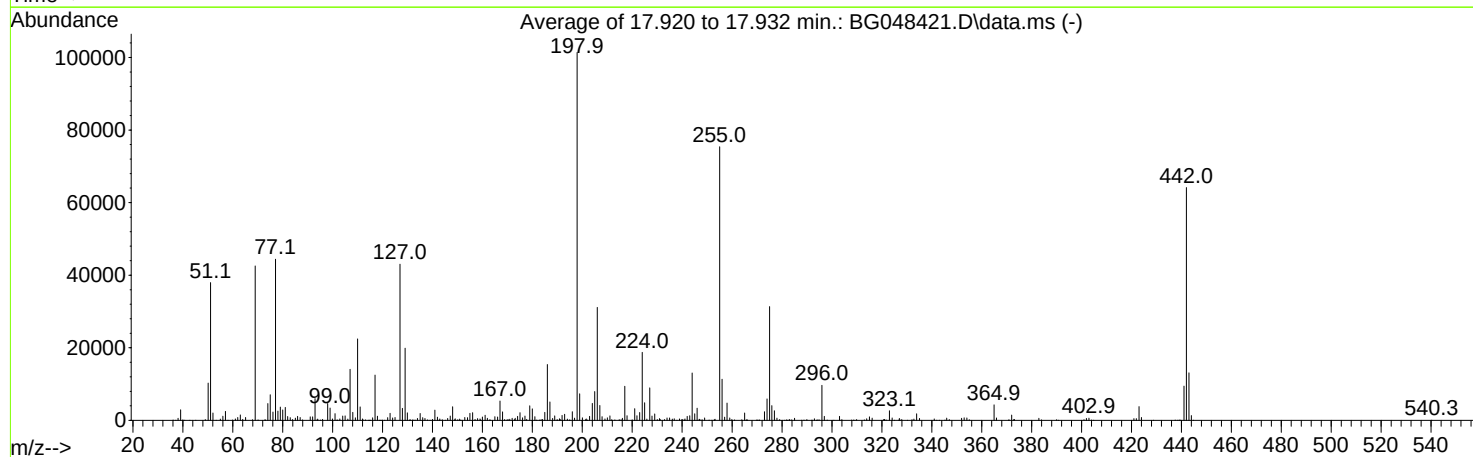


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
 Data File : BG048421.D
 Acq On : 19 Mar 2021 12:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 18 16:38:55 2021

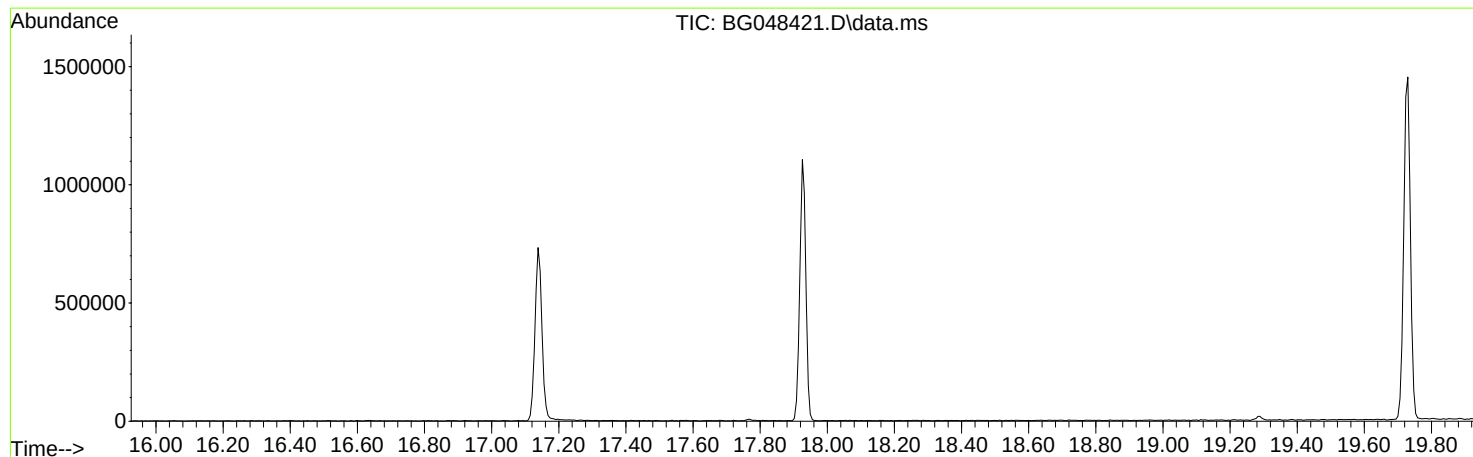

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	37979	PASS
68	69	0.00	2	0.4	186	PASS
69	198	0.00	100	42.0	42539	PASS
70	69	0.00	2	0.3	140	PASS
127	198	10	80	42.5	43051	PASS
197	198	0.00	2	0.6	620	PASS
198	198	100	100	100.0	101368	PASS
199	198	5	9	7.2	7304	PASS
275	198	10	60	30.9	31365	PASS
365	198	1	100	4.2	4282	PASS
441	198	0.01	100	9.3	9433	PASS
442	198	50	100	63.3	64171	PASS
443	442	15	24	20.4	13092	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/19/2021	BNA_G	<u>BG048421.D</u>
Compound Name	Response	Retention Time
DDT	412461	20.96
DDD	5294	20.52
DDE	806	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6100	418561	1.46

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
 Data File : BG048421.D
 Acq On : 19 Mar 2021 12:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 19 13:56:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 18 16:38:55 2021
 Response via : Initial Calibration

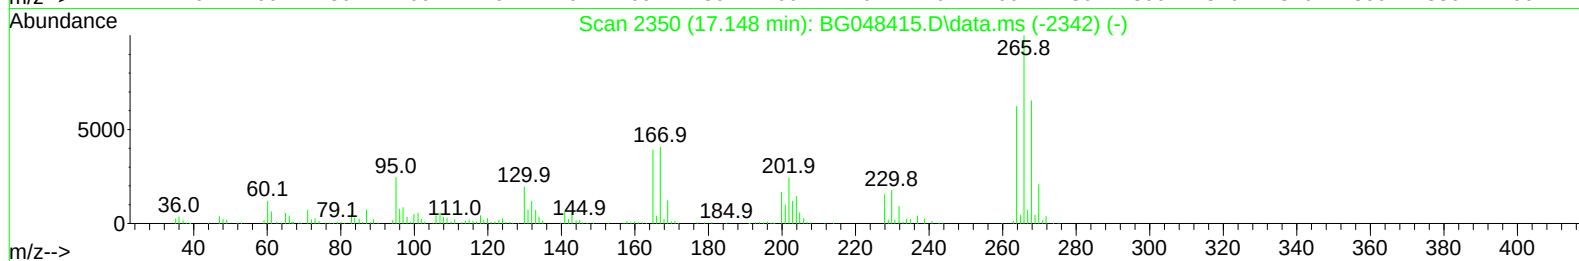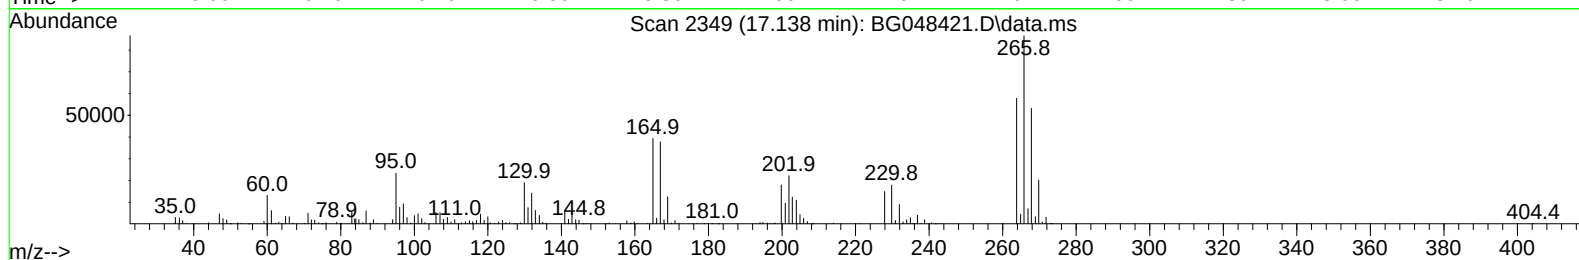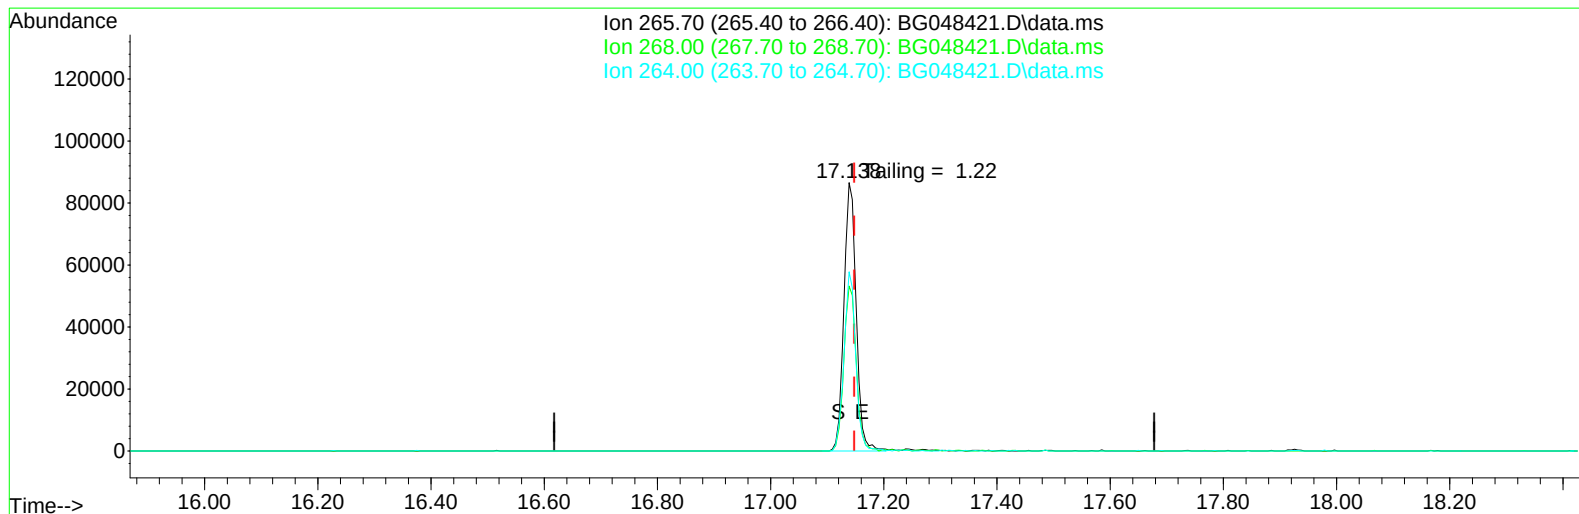

TIC: BG048421.D\data.ms

(70) Pentachlorophenol (C)

17.138min (-0.010) 224545.07 ng




response 130940

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.47
264.00	61.60	66.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031921\
Data File : BG048421.D
Acq On : 19 Mar 2021 12:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 19 13:56:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 18 16:38:55 2021
Response via : Initial Calibration

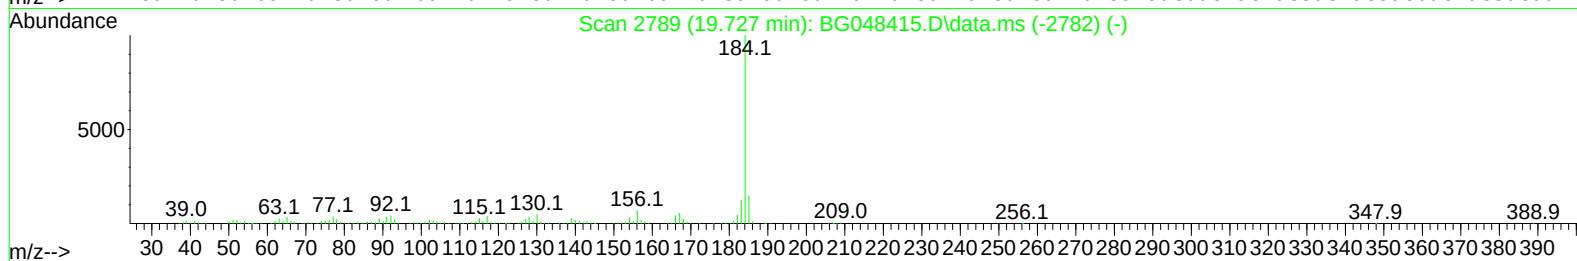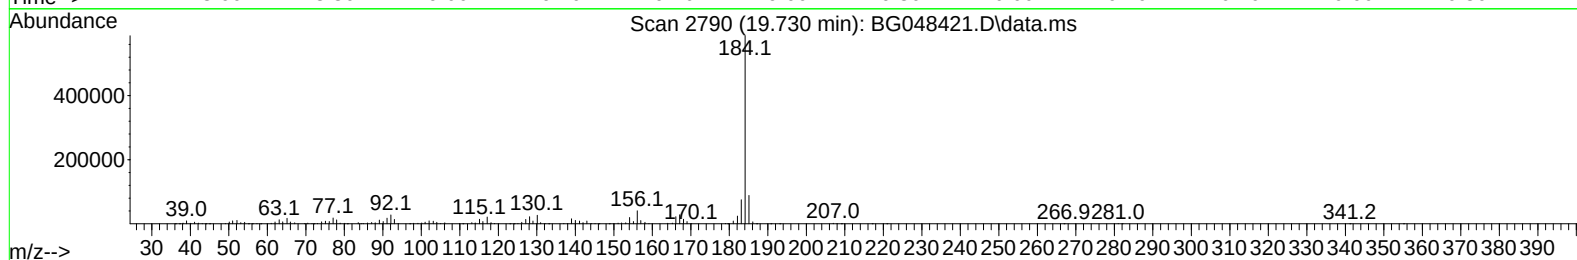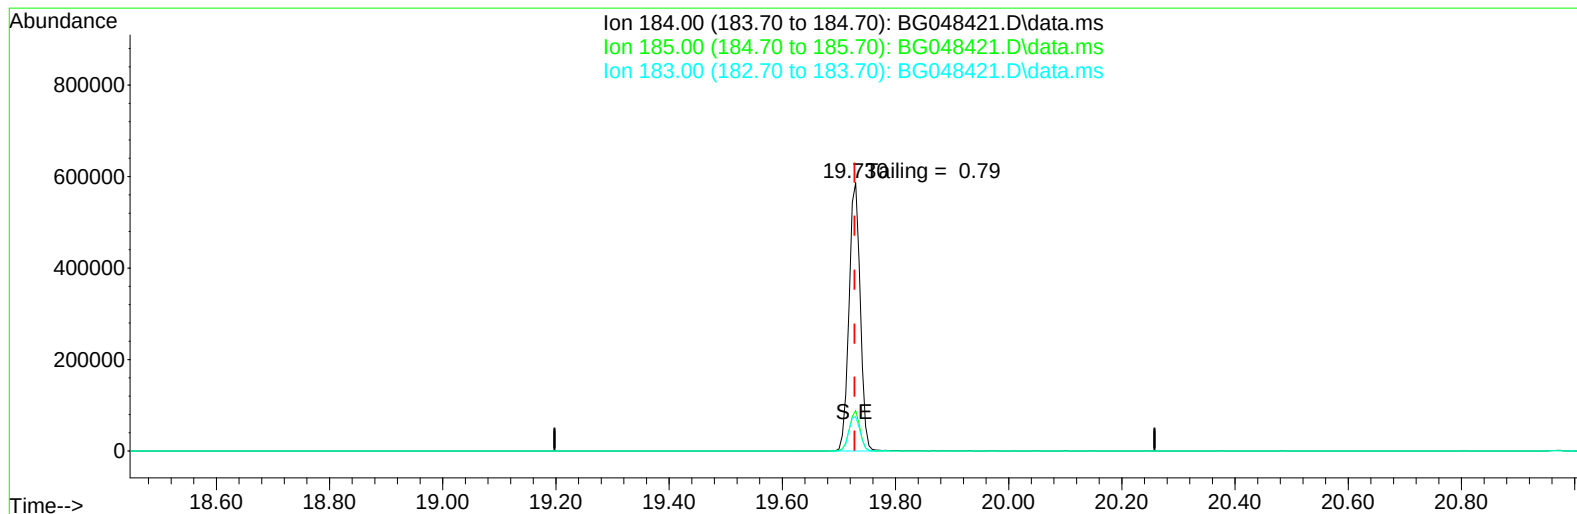

TIC: BG048421.D\data.ms

(77) Benzidine

19.730min (+ 0.002) 509166.92 ng

response 808356

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.08
183.00	13.20	12.83
0.00	0.00	0.00