
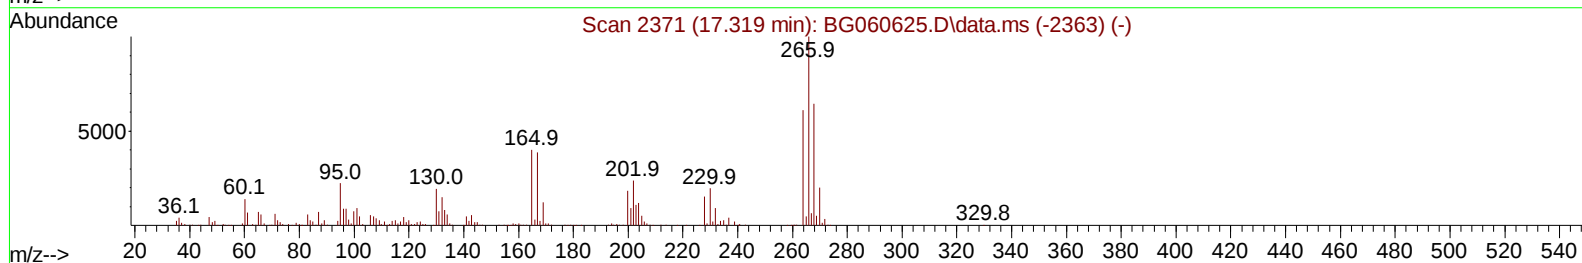
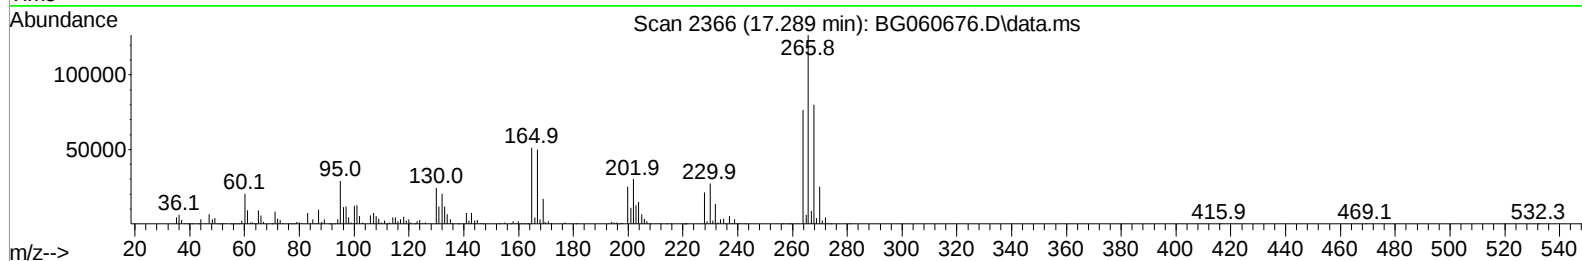


Quant Time: Mar 20 01:46:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

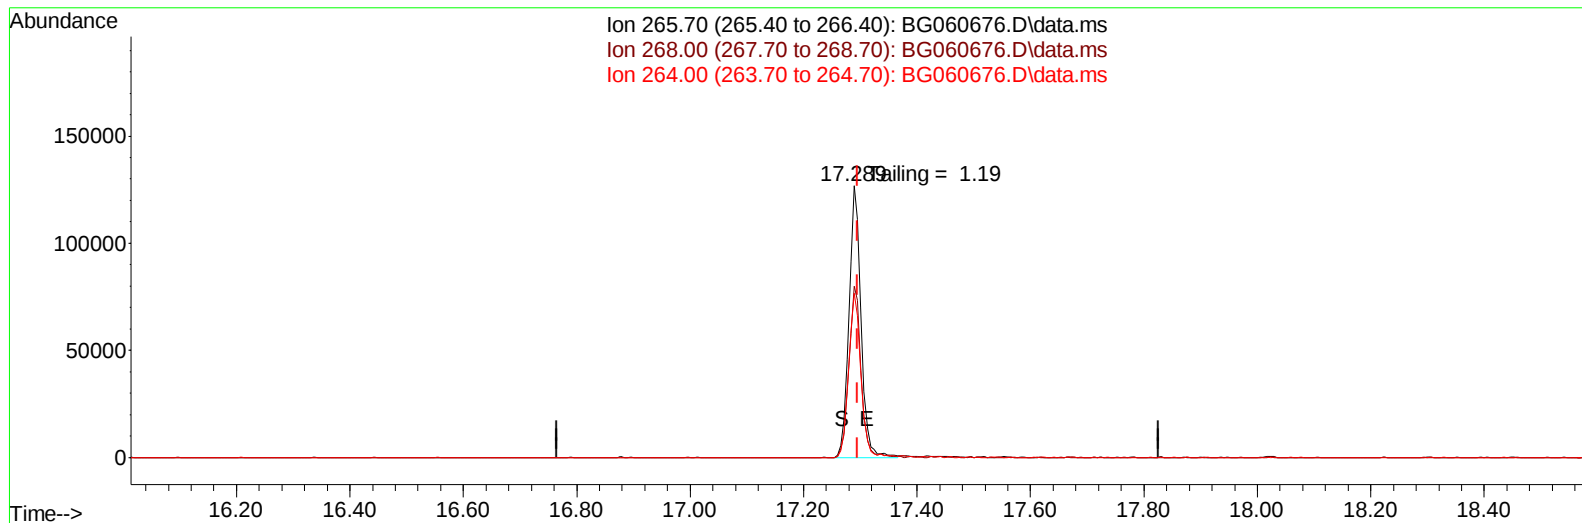

TIC: BG060676.D\data.ms




17.289min (-0.006) 339707.04 ng

response **188360**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	63.08
264.00	61.10	60.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
Data File : BG060676.D
Acq On : 19 Mar 2024 10:21
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 01:46:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 18 14:26:31 2024
Response via : Initial Calibration

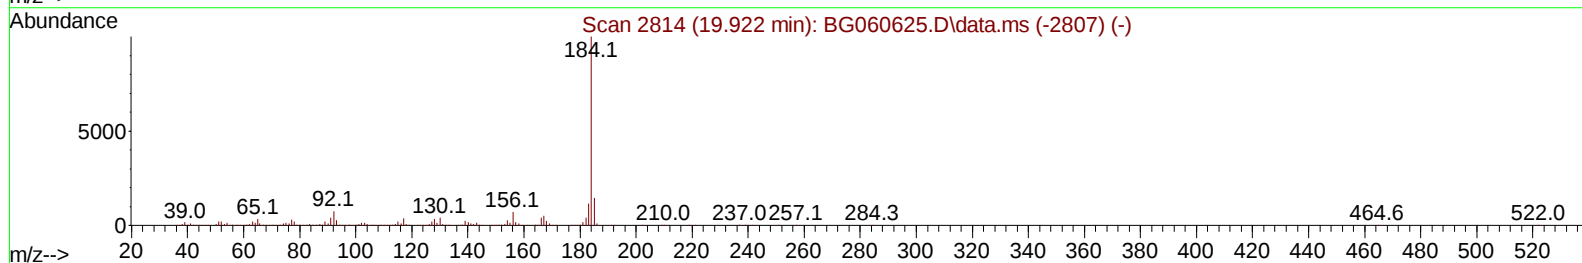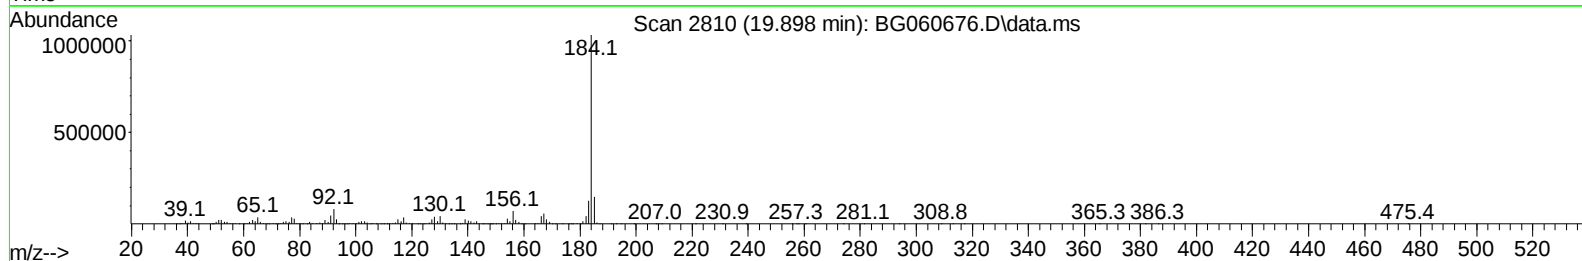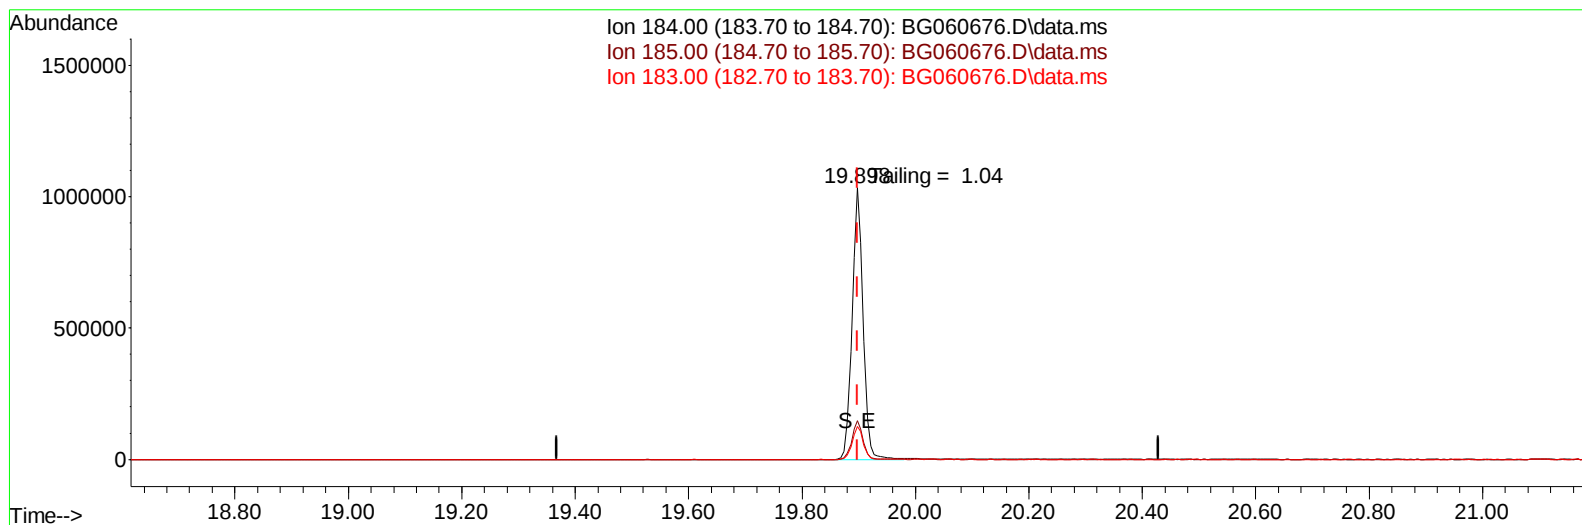

TIC: BG060676.D\data.ms

(77) Benzidine**19.898min (-0.001) 961875.67 ng****response 1388117**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	11.50	12.22
0.00	0.00	0.00