

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
 Data File : BG060682.D
 Acq On : 19 Mar 2024 15:29
 Operator : MA/JU
 Sample : P1786-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.783	398	407	417	rBV	1286153	2104938	49.94%	8.546%
2	7.410	675	684	698	rBV	1336108	2353004	55.83%	9.553%
3	8.291	825	834	842	rBV	395375	693380	16.45%	2.815%
4	9.490	1025	1038	1051	rBV	824297	1525758	36.20%	6.195%
5	11.141	1310	1319	1326	rBV	570583	1035746	24.58%	4.205%
6	13.550	1717	1729	1737	rBV	2246961	3473699	82.42%	14.104%
7	14.925	1957	1963	1970	rVV	843066	1328689	31.53%	5.395%
8	15.971	2134	2141	2148	rVB2	44634	81219	1.93%	0.330%
9	16.411	2209	2216	2224	rBV	1566040	2435538	57.79%	9.889%
10	17.674	2424	2431	2436	rBV	992283	1547030	36.71%	6.281%
11	17.716	2436	2438	2443	rVB	214958	276763	6.57%	1.124%
12	17.810	2451	2454	2458	rBV2	30199	43730	1.04%	0.178%
13	18.497	2566	2571	2575	rBV2	271347	359807	8.54%	1.461%
14	18.585	2584	2586	2592	rVB2	46059	73175	1.74%	0.297%
15	19.707	2773	2777	2782	rVB	258185	355622	8.44%	1.444%
16	20.072	2836	2839	2844	rVB	260733	349979	8.30%	1.421%
17	20.254	2865	2870	2877	rBV	3269722	4214623	100.00%	17.112%
18	21.541	3085	3089	3094	rBV2	218088	334017	7.93%	1.356%
19	21.993	3160	3166	3172	rBV	804697	1433502	34.01%	5.820%
20	22.116	3184	3187	3191	rVB	158424	223552	5.30%	0.908%
21	22.769	3295	3298	3307	rVB	232855	386189	9.16%	1.568%




Sum of corrected areas: 24629960

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
Data File : BG060682.D
Acq On : 19 Mar 2024 15:29
Operator : MA/JU
Sample : P1786-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

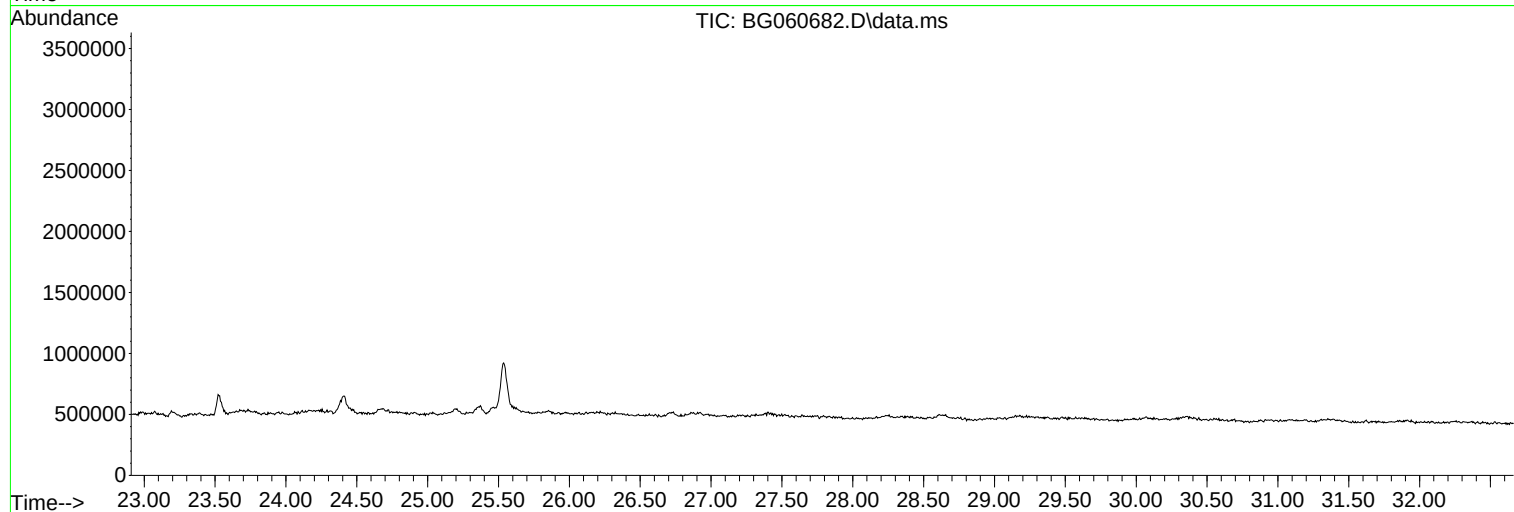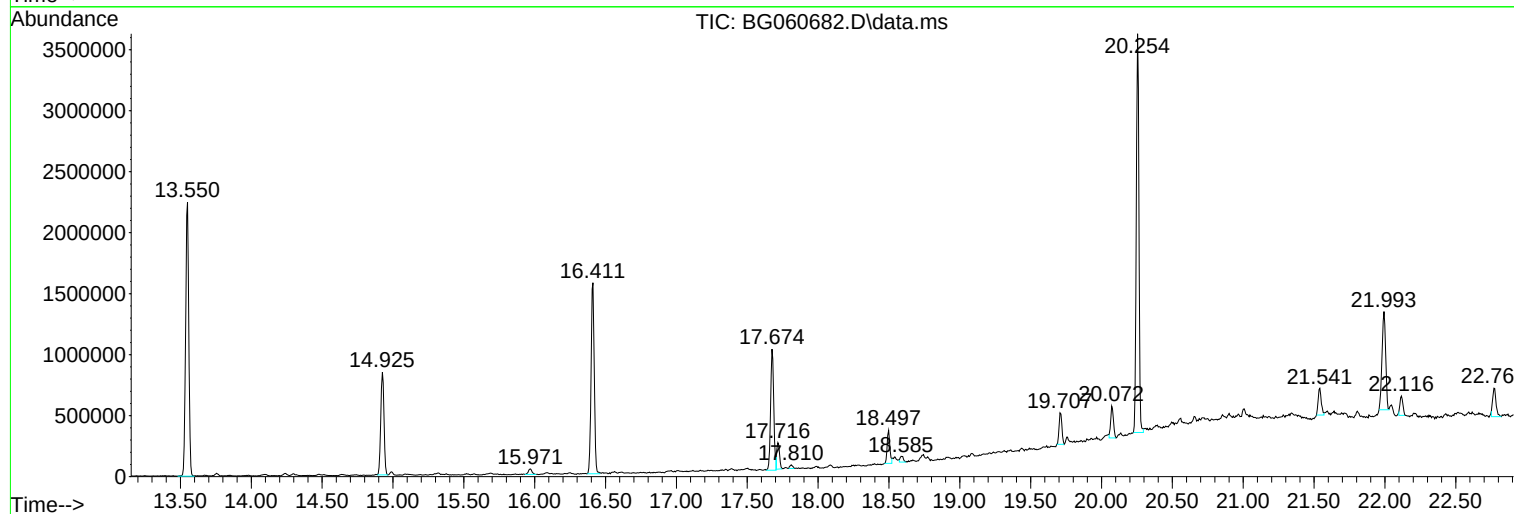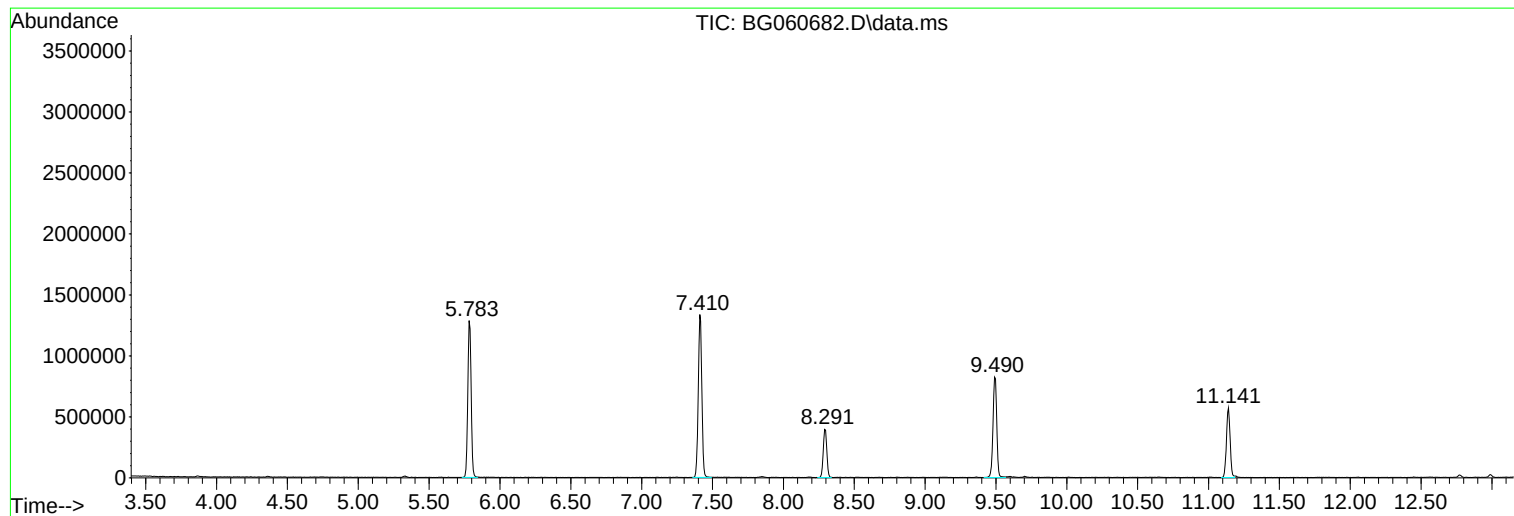

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
Data File : BG060682.D
Acq On : 19 Mar 2024 15:29
Operator : MA/JU
Sample : P1786-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031924\
Data File : BG060682.D
Acq On : 19 Mar 2024 15:29
Operator : MA/JU
Sample : P1786-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------